

**Differential pulse polarographic Determination
of Submicrogram Quantities of Carmustin and Related Compounds
in Biological Samples**

Bartosek I., Daniel S., Sykora S.

J.Pharmac.Sci. **67**, 1160-1163 (1978)

This copy, scanned from an Author's reprint, is intended for personal perusal only.
Other uses require permission of the *American Pharmaceutical Association*.

Other works by Stan Sykora can be found at www.ebyte.it

Abstract:

A polarographic method was developed to determine the antineoplastic agent carmustin and other nitrosoureas, such as N-methyl-N-nitrosourea and N-cyclohexyl-N-nitrosourea, in biological liquids at levels well below 1µg/ml or g. The stability of carmustin in different media was investigated to prevent losses during administration or assay. Examples of nitrosourea determination in biological samples are given.

Keywords: Polarography, Carmustin, Nitrosourea, Biological samples, Antineoplastics

Differential Pulse Polarographic Determination of Submicrogram Quantities of Carmustine and Related Compounds in Biological Samples

IVAN BARTOŠEK **, SONIA DANIEL †, and STANISLAV SÝKORA ‡

Received June 15, 1977, from the *Istituto di Ricerche Farmacologiche 'Mario Negri,' Via Eritrea, 62, 20157 Milan, Italy, and †Bruker Spectrospin Italiana, Via Miglioretti, 2, Milan, Italy. Accepted for publication December 16, 1977.

Abstract □ A polarographic method was developed to determine the antineoplastic agent carmustine and other nitrosoureas, such as *N*-methyl-*N*-nitrosourea and *N*-cyclohexyl-*N*-nitrosourea, in biological fluids at levels well below 1 µg/ml or g. The stability of carmustine in different media was investigated to prevent losses during administration or assay. Examples of nitrosourea determination in biological samples are given.

Keyphrases □ Carmustine—differential pulse polarographic analysis in biological samples □ Nitrosoureas, various—differential pulse polarographic analyses in biological samples □ Polarography, differential pulse—analyses, carmustine and various nitrosoureas in biological samples □ Antineoplastics—carmustine, differential pulse polarographic analysis in biological samples

N-Alkyl-*N*-nitrosoureas and, in particular, carmustine, 1,3-bis(2-chloroethyl)-1-nitrosourea (I), are widely used antineoplastic agents. Unfortunately, their determination in biological samples is hampered by the low sensitivity of the currently used colorimetric method (1, 2). Garrett and Cusimano (3) investigated the polarographic behavior of various *N*-alkyl-*N*-nitrosoureas. Since that time, however, polarographic techniques have been improved considerably (4–6), and their basic sensitivity has been increased by a factor of at least 100, pushing the limits of applicability of polarography far below the microgram level (7, 8). Therefore, the possibility of using polarography for routine assays of I and other nitrosoureas in blood and tissues was investigated.

EXPERIMENTAL

Apparatus—Measurements were made on a modular polarograph¹ with a standard polarographic vessel²; for some measurements, the thermostated vessel² was used. These vessels require a minimum sample volume of 5 ml; a microcell¹ for 0.5–5 ml also was used with success.

Reagents—All reagents (potassium chloride, hydrochloric acid, citric acid, tartaric acid, ether, and *n*-pentane) were analytical grade. An interfering peak at $E = 0.830$ v, due to an impurity, appeared in some supplies of the citric acid used as a basic electrolyte; each original bottle had to be checked before use by running a blank polarogram. All solutions were prepared with redistilled water. Tridistilled, commercially supplied mercury was used for the dropping mercury electrode.

Compound I, *N*-cyclohexyl-*N*-nitrosourea (II), and *N*-methyl-*N*-nitrosourea (III) were obtained as lyophilized powders from two sources^{3,4}. No difference in quality was observed between the different samples of I as long as the compound was stored in dry plastic bags (with silica gel inserts) at deep-freeze temperatures.

Extraction Procedures—Blood was prevented from clotting by 3.8% sodium citrate (nine parts of blood plus 1 part of citrate solution) and centrifuged (10 min at 3000 rpm) to separate plasma.

Procedure A—Plasma, 1 ml, was mixed with 1 ml of 0.2 *M* citric acid and extracted with 5 ml of *n*-pentane for 1 min. After separation of the

two phases, 4 ml of the extract was evaporated directly in the thermostated polarographic vessel at 40° with 5 or 10 ml of 0.2 *M* citric acid.

Procedure B—Plasma, 1 ml, was mixed with 1 ml of 0.2 *M* citric acid and extracted three times with 4 ml of *n*-pentane for 3 min. A 10-ml aliquot of the combined extracts was then evaporated in a test tube with 0.2 *M* citric acid at 40° and submitted to polarography at room temperature.

Polarographic Measurements—Citric acid (0.2 *M*) was used as a basic electrolyte. Dissolved oxygen was removed by bubbling high purity nitrogen gas, passed first through redistilled water to remove all mechanical impurities. A three-electrode arrangement was adopted with a dropping mercury electrode, a platinum auxiliary electrode, and a saturated calomel electrode as reference. The mercury flow rate in the dropping mercury electrode was 1.25 mg/sec, and the height of the mercury column was 120 cm.

The drop time was limited by an electronically controlled hammer; a drop time of 3 sec was optimal. The differential pulse technique was adopted with the pulse height, ΔE , of 100 mv. The sweep normally covered the interval from -250 to -750 mv, and the sweep rate in most cases was 2 mv/sec. The output signal was filtered by a resistance-capacitance filter with a time constant of 0.1 sec. In addition, a gated accumulator was inserted to suppress experimental noise.

RESULTS AND DISCUSSION

Polarographic Properties of Nitrosoureas—The collected data indicate that, qualitatively, I is to some extent representative of all *N*-alkyl-*N*-nitrosoureas and that reduction of I on the dropping mercury electrode is not a simple electrode process. A full interpretation was not attempted, but the data were used to develop a routine analytical method⁵.

Figure 1 illustrates the behavior of I in 0.1 *M* KCl acidified to varying degrees with hydrochloric acid. At pH 2.5, there was a single reduction wave (A), whose half-wave potential ($E_{1/2}$), width, and height all depended on pH. At higher pH values, wave A was still present, but a second

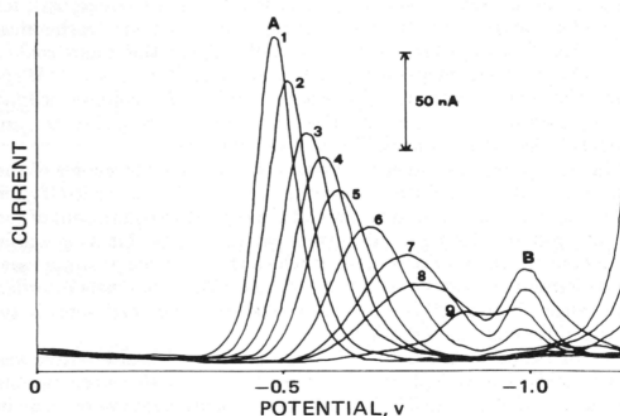


Figure 1—Polarograms of I, showing dependence on acidity in the 0.1 *M* KCl-hydrochloric acid basic electrolyte. The concentration of I was 2×10^{-5} *M*. The experimental setup was as described in Experimental, except that the differential pulse height was 20 mv and the gated accumulator was not used. Key (pH values): 1, 1.56; 2, 2.00; 3, 2.58; 4, 3.00; 5, 3.50; 6, 4.02; 7, 4.52; 8, 5.02; and 9, 5.70.

⁵ A detailed analysis of the reduction process will appear elsewhere.

¹ Universal E 310, Bruker Physik AG, 7512 Karlsruhe-Rheinstetten, Silberstreifen, West Germany.

² Metrohm, Herisau, Switzerland.

³ National Cancer Institute, Bethesda, Md.

⁴ Simes, Milan, Italy.




Figure 2—Polarograms of I, showing dependence on citric acid concentration. The concentration of I was 2×10^{-5} M. The experimental setup was as described in Experimental. The concentrations of citric acid for the curves (from top to bottom) were 0.025, 0.05, 0.1, 0.2, and 0.5 M.

wave (B) appeared at somewhat more negative potentials. The height and width of wave B also depended on pH, but its position appeared to be nearly constant.

A very tentative interpretation might be that there are two forms (A and B) of I in an equilibrium of the type $B + H^+ = A$. Form A, prevailing at low pH, is reduced at the mercury electrode in a one-electron process involving H^+ ions. Form B is reduced in a one-electron process that does not involve H^+ ions. For analytical purposes, a single sharp peak at a well-defined position is preferable. The results, therefore, indicate the necessity of a suitable acid buffer.

The choice of buffer was complicated by the fact that the compound behaved somewhat differently when weak acids, such as citric, were used as the basic electrolyte (Fig. 2). Then there was just one peak at about -500 mv, and the pH dependence of the peak parameters was very small. The width of the peak considerably exceeded the value characteristic for a one-electron process, thus indicating a complex electrochemical mechanism. The dependence of the current (I_{500}) on the square root of the height of the mercury column (\sqrt{h}) was linear. For a 2×10^{-5} M solution, the least-squares fit of the data obtained for column heights ranging from 30 to 120 cm gave the relation $I(nA) = 92.978 \cdot \sqrt{h}$ cm - 193.048; the correlation coefficient was $r = 0.998$.

When analyzing low concentrations of I (10^{-7} M), the choice of the basic electrolyte was critical for another reason. The buffer itself gave a relatively high background because of the capacitive component of the current, and this background current should be as flat as possible throughout the range of potentials at which the test drug peak appears. The background currents of a number of basic electrolytes were recorded in the range of potentials from -250 to -750 mv at very high sensitivity, and the differences were marked.

The final choice was 0.2 M citric acid (an acceptable alternative was tartaric acid). Figure 3 shows the polarograms of I at concentrations ranging from 5×10^{-8} to 5×10^{-7} M. The measurements were made in 5 ml of the basic electrolyte so the smallest quantity measured was about 50 ng. By using a microcell, this figure can be reduced by a factor of about 10. Assays at these levels must be done with the utmost care to avoid impurities (e.g., reagents, water, mercury, and glassware) and any sources of noise (e.g., bad contacts).

At low concentrations, the background current complicates quantitative evaluation of the data. Therefore, a method based on measurements of the current values I_{400} , I_{500} , and I_{600} at potentials of -400, -500, and -600 mv, respectively, was employed.

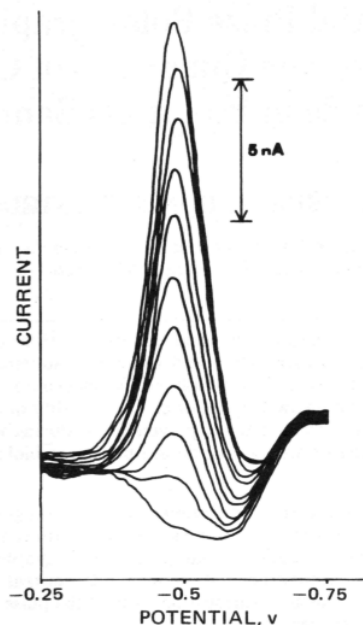


Figure 3—Calibration curves of I in 0.2 M citric acid under conditions described in Experimental. The concentrations (from bottom to top) were 0 (basic electrolyte), 5×10^{-8} , 10^{-7} , 1.5×10^{-7} , 2×10^{-7} , 2.5×10^{-7} , 3×10^{-7} , 3.5×10^{-7} , 4×10^{-7} , 4.5×10^{-7} , and 5×10^{-7} M.

The following equation is used for both the sample, S, and a blank containing only basic electrolyte, S_0 :

$$S \text{ or } S_0 = I_{500} - 0.5 \times (I_{400} + I_{600}) \quad (\text{Eq. 1})$$

The difference $s = (S - S_0)$ is then used in empirical calibration graphs; s is directly proportional to the concentration of I even at the lowest detectable level. The slope depends, of course, on the experimental setup (capillary, height of the mercury reservoir, drop time, and temperature) so a new calibration is necessary each time any relevant parameter is changed; $s = (K)$ (concentration). In Fig. 3, $k = 0.0355$ amp/mole \times liter $^{-1}$. When a calibration graph is not available, the method of standard addition can always be used; but even in this case, the quantity s should be used if the concentrations involved are close to the detection limit. Figure 4 gives the polarographic curves of some *N*-alkyl-*N*-nitrosoureas in 0.2 M citric acid at a concentration of 10^{-6} M. While all nitrosoureas are polarographically active and give rise to peaks between -0.4 and -0.8 v, differences exist between different members of this group.

Thus, assays of II can be made using the same techniques as for I, with the additional advantage of higher sensitivity. On the other hand, the




Figure 4—Polarograms of 10^{-6} M I, II, and III in 0.2 M citric acid under conditions described in Experimental. The bottom line is the basic electrolyte.




Figure 5—Polarograms of rat plasma (P) containing 10 (1) and 20 (2) μg of I/ml. The sample was prepared by adding 1 ml of plasma to 9 ml of 0.2 M citric acid. The conditions were as described in Experimental, except that the pulse height was 50 mv and the accumulator was not used.

peak of III is much broader than that of I and appears at more negative potentials where the reproducibility of the background current is lower because of common impurities in the citric acid. As a result, the sensitivity of III assays is expected to be lower than with I unless the technique is suitably modified.

Stability of I in Various Solutions—Nitrosoureas decompose easily unless the pH values are kept sufficiently low (2, 9, 10). The stability of I in various experimental circumstances was examined to establish reliable time limits for its clinical administration and assay. The pharmaceutical preparation⁴ of I was dissolved directly in the unbuffered physiological saline or 5% glucose used for infusion. The pH values of the resulting solution differed considerably from case to case; in several experiments, the pH values remained slightly above 7 and I decomposed completely in less than 1 hr. Therefore, in clinical applications involving infusions of I, pH differences in the unbuffered infusion solutions may be responsible for broad variations in drug delivery and poor reproducibility of the treatment.

On the other hand, no measurable decay was observed in animal plasma buffered with sodium citrate and kept for several weeks at -20° . The half-life of I in citric acid (0.2 M) at 0° was about 270 hr; at 20° , it was 16.9 hr. Very slow decay of the compound was observed in ethanol solution acidified by a drop of 1 M citric acid per 10 ml; the half-life of I at 20° was between 250 and 300 hr.

Routine Assays of I in Biological Samples—Figure 5 shows the polarogram of 1 ml of plasma, with and without addition of I, measured in 10 ml of 0.2 M citric acid. Surprisingly, the peak of I was at -750 mv rather than at the expected -500 mv. A possible explanation is complex formation; preferential binding of I to some plasma proteins has, in fact, been reported (2). However, assay of I in untreated plasma is hindered by the background produced by the plasma itself, which limits the usefulness of the method to concentrations exceeding about $5 \mu\text{g}/\text{ml}$ of plasma. Moreover, it is difficult to eliminate oxygen from the plasma because of foam formation. Foaming may be avoided by denaturing the plasma proteins with 5% HClO_4 and removing them by filtration prior to polarography.

The background from blank plasma treated with perchloric acid was, however, exactly the same as when the plasma was not denatured, indicating that it was not due to proteins. The nitrosourea added to the plasma before treatment was no longer detectable in the filtrate, while I added to the filtrate after removal of the proteins gave a peak at its normal position of -500 mv. This result confirms that I forms a strong complex with plasma proteins but, at the same time, precludes any possibility of using denaturation for assay purposes.

An excellent method for solving these problems is to extract the plasma with an apolar organic solvent such as ether or *n*-pentane. After separation of the phases, an aliquot of the organic phase is evaporated in a vessel containing the basic electrolyte (possibly directly in the polarographic cell). There is no detectable background due to the plasma itself. With I, the extraction yield depends on the efficiency and time of shaking.

A simple 1-min extraction (Procedure A) gave yields in the range of

85–90% for ether or *n*-pentane. The standard error of determination of parallel samples extracted with *n*-pentane did not exceed 3.3% within the concentration range studied; the calibration curve was linear. *n*-Pentane is preferred because ether usually contains traces of polarographically active peroxides that interfere with the determination of I. Ether also dissolves considerable amounts of water (7%), which end up in the basic electrolyte and may represent a complication if the final volume is to be kept small (microcell).

Extraction of whole blood directly also was attempted. While the extraction yields were essentially the same as for plasma, difficulties were encountered because of lipids in the blood cells. These were extracted and eventually led to colloid impurities in the solution to be analyzed polarographically. The colloid particles caused severe noise on the dropping mercury electrode unless they were first removed by filtration. The technique finally adopted is simple and quantitative. As described in *Experimental (Procedure B)*, it consists of removal of the blood cells by centrifugation, triple extraction by *n*-pentane, and evaporation of the organic extract in a vessel containing a known amount of the 0.2 M citric acid used as the basic electrolyte.

Disappearance of I from Rat and Mouse Plasma—Male Sprague-Dawley rats⁶, 226 ± 3 g, or male Albino Swiss mice CD-1, 20.9 ± 0.6 g, received 10 mg of I/g iv. Groups of animals were killed 2, 5, 10, 20, 30, 60, 90, and 120 min after I administration. Blood was collected (nine parts of blood plus 1 part of 3.8% sodium citrate) and centrifuged at 3000 rpm for 10 min. Prepared plasma was frozen at -20° for further analysis. Before *n*-pentane extraction, plasma samples were thawed at 37° for 5 min. Extraction Procedure B was used to determine the remaining drug. The data are reported in Table I, and kinetic analyses of these data are reported in Table II.

Table I—Disappearance of I from Rat and Mouse Plasma after Administration of 10 mg of the Drug/kg iv

Minutes	Concentration of I, $\mu\text{g}/\text{ml}$ of Plasma (Mean \pm SE)	
	Rat	Mouse
2	2.36 ± 0.41	2.41 ± 0.38
5	1.70 ± 0.18	1.02 ± 0.15
10	0.66 ± 0.04	0.16 ± 0.04
20	0.38 ± 0.02	0.08
30	0.22 ± 0.04	<0.02
60	<0.02	<0.02

Table II—Kinetic Analysis^a of the Data Reported in Tables I and III

Animal Species	Half-Life, $t_{1/2}$, min	Correlation ^b Coefficient, r	Initial Concentration, $\mu\text{g}/\text{ml}$	Volume Distribution, V_d , liters/kg
Rat	8.33 ± 0.14	0.990	2.25 ± 0.22	4.43
Mouse	2.17	0.984	4.57	2.19
Rat liver microsomes	49.74	0.999	40.0	

^a Standard error is given wherever available. ^b Decay followed first-order kinetics in all cases.

Table III—Disappearance of I after Incubation with Rat Liver Microsomes

Minutes	Concentration of I, $\mu\text{g}/\text{ml}$ of Incubation Medium
2	32.1
5	30.1
10	29.6
15	25.8
20	22.4
30	21.3
40	18.8
50	15.5
60	14.5

⁶ CD-COBS, Charles River, Italy.

Disappearance of I after Incubation with Rat Liver Microsomes—Rat liver microsomes were prepared according to the standardized technique described previously (11). The incubation medium contained 0.93 μ mole of I, 1.5 μ moles of NADP, 50 μ moles of glucose 6-phosphate, 0.7 international unit of glucose 6-phosphate dehydrogenase, 25 μ moles of magnesium chloride, 0.08 M phosphate buffer (pH 7.0), and 30 mg of microsomes in a total volume of 5 ml. Samples (1.0 ml) of the incubation medium were taken at different time intervals, acidified with citric acid (0.1 ml of 1 M solution), and immediately extracted with 5 ml of *n*-pentane for 10 min at room temperature. The results are reported in Tables II and III.

REFERENCES

- (1) T. L. Loo and R. L. Dion, *J. Pharm. Sci.*, **54**, 809 (1965).
- (2) T. L. Loo, R. L. Dion, R. L. Dixon, and D. P. Rall, *ibid.*, **55**, 492 (1966).
- (3) E. R. Garrett and A. G. Cusimano, *ibid.*, **55**, 702 (1966).
- (4) J. B. Flato, *Anal. Chem.* **44**, 75 A (1972).
- (5) P. J. Elving, in "Electroanalytical Chemistry," H. W. Nurnberg, Ed., Wiley, London, England, 1974, p. 197.
- (6) H. Hoffman and J. Volke, in *ibid.*, p. 287.
- (7) A. M. Brooks, J. A. F. De Silva, and R. M. Hackman, *Am. Lab.*, **1974**, 23.
- (8) D. J. Pietrzyk, *Anal. Chem.*, **46**, 52 R (1974).
- (9) E. R. Garrett, S. Goto, and J. F. Stubbins, *J. Pharm. Sci.*, **54**, 119 (1965).
- (10) J. A. Montgomery, R. James, G. S. McCaleb, and T. P. Johnston, *J. Med. Chem.*, **10**, 668 (1967).
- (11) D. L. Cinti, P. Moldeus, and J. B. Schenkman, *Biochem. Pharmacol.*, **21**, 3249 (1972).