



US00D888267S

(12) **United States Design Patent**
Salomon et al.

(10) **Patent No.:** **US D888,267 S**

(45) **Date of Patent:** **** Jun. 23, 2020**

(54) **DIAGNOSTIC INSTRUMENT**

D649,658 S 11/2011 Belfance et al.
D669,169 S 10/2012 Washington et al.
D682,441 S * 5/2013 Kim D24/216
(Continued)

(71) Applicant: **MeMed Diagnostics Ltd.**, Tirat
HaCarmel (IL)

(72) Inventors: **Noga Salomon**, Carmiel (IL); **Kfir Oved**, Hof HaCarmel (IL); **Roy Navon**, Tel-Aviv (IL); **Assaf Cohen-Dotan**, Natania (IL); **Eran Eden**, Haifa (IL); **Salit Tzaban**, Nofit (IL); **Yana Khalfin**, Haifa (IL); **Ofer Halbreich**, Tel-Aviv (IL); **Matthew Fenwick**, Mount Waverley (AU); **Adrian Charles Ian Scott-Murphy**, Surrey Hills (AU); **Matthew Hou-Pou Yeung**, Nunawading (AU); **James William Luther**, Milan (IT); **Barbara Tornaghi**, Monza (IT); **Andrea Besana**, Seveso (IT)

FOREIGN PATENT DOCUMENTS

WO WO 2019/087176 5/2019

OTHER PUBLICATIONS

The platform: MeMed Key™, posted at www.me-med.com, no posting date, online, URL:https://www.me-med.com/ (Year: 2019).*
(Continued)

Primary Examiner — Lilyana Bekic
Assistant Examiner — Mary Shannon Malley

(73) Assignee: **MeMed Diagnostics Ltd.**, Tirat
HaCarmel (IL)

(57) **CLAIM**

The ornamental design for a diagnostic instrument, as shown and described.

(**) Term: **15 Years**

(21) Appl. No.: **29/645,126**

DESCRIPTION

(22) Filed: **Apr. 24, 2018**

This invention was made with government support under contract number HDTRA1-17-C-0011 awarded by the Defense Threat Reduction Agency and grant number W81XWH-17-1-0694 awarded by the U.S. Army Medical Research Acquisition Activity. The government has certain rights in the invention.

(51) **LOC (12) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/216**

(58) **Field of Classification Search**
USPC D24/216, 219, 223, 224, 227, 229, 230, D24/231, 232, 233, 234, 107, 186, 217, D24/220, 225, 226; D10/81, 97
CPC G01N 2035/00306; G01N 2035/00326; G01N 2035/00336; G01N 33/53; G01N 33/5302; G01N 33/569; B01L 7/52
See application file for complete search history.


FIG. 1 is a front perspective view of a diagnostic instrument showing our new design;
FIG. 2 is a front view thereof;
FIG. 3 is a right side view thereof;
FIG. 4 is a left side thereof;
FIG. 5 is a top view thereof;
FIG. 6 is a back view thereof; and,
FIG. 7 is a bottom view thereof.
The broken lines depict portions of the diagnostic instrument that do not form part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

4,576,185 A 3/1986 Proud et al.
D631,554 S 1/2011 Jackson et al.

1 Claim, 7 Drawing Sheets

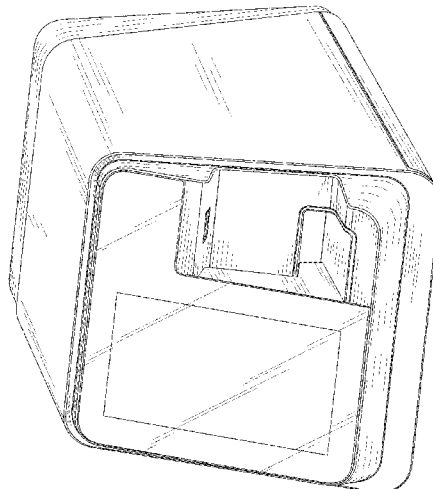

(56)

References Cited

U.S. PATENT DOCUMENTS

D704,348	S *	5/2014	Shibata	D24/216
D707,825	S	6/2014	Murai	
D718,462	S *	11/2014	Cook	D24/216
9,446,406	B2	9/2016	Gordon et al.	
D774,205	S *	12/2016	Grace	D24/169
D818,146	S *	5/2018	Tanaka	D24/216
D821,601	S *	6/2018	Henderson	D24/216
D827,859	S *	9/2018	Mathers	D24/232
D830,548	S	10/2018	Kemp	
D833,639	S	11/2018	Peltosaari et al.	
D853,873	S *	7/2019	Schueren	D10/81
D854,703	S *	7/2019	Juhlin	D24/216
2012/0227471	A1 *	9/2012	Smith	G01N 35/1011 73/61.59
2015/0250456	A1	9/2015	Olgun	
2016/0051415	A1	2/2016	Kuan et al.	
2017/0065971	A1	3/2017	Kreifels et al.	

OTHER PUBLICATIONS

Official Action Dated Nov. 26, 2019 From the US Patent and Trademark Office Re. U.S. Appl. No. 29/662,120. (13 pages).

* cited by examiner

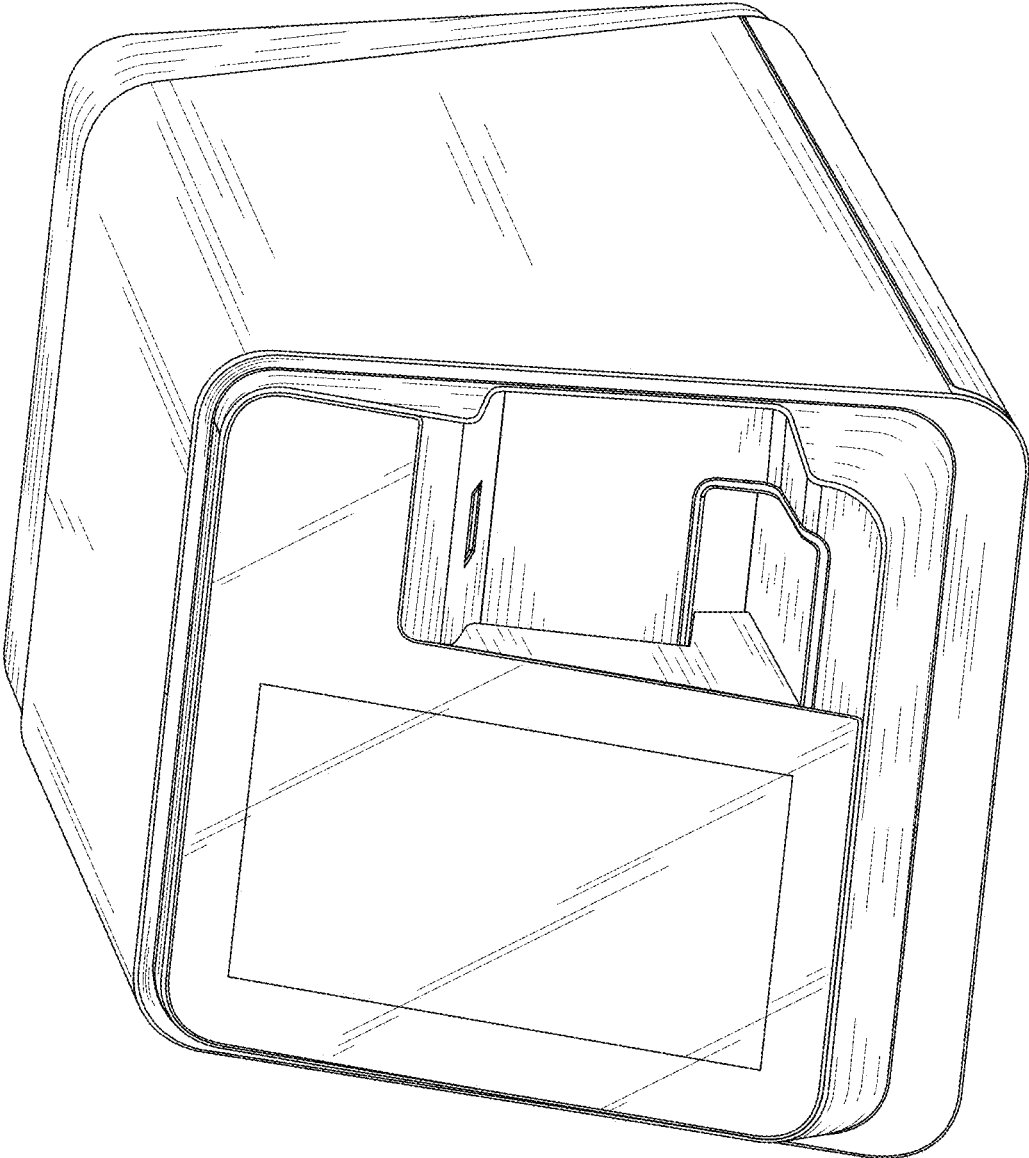


FIG. 1

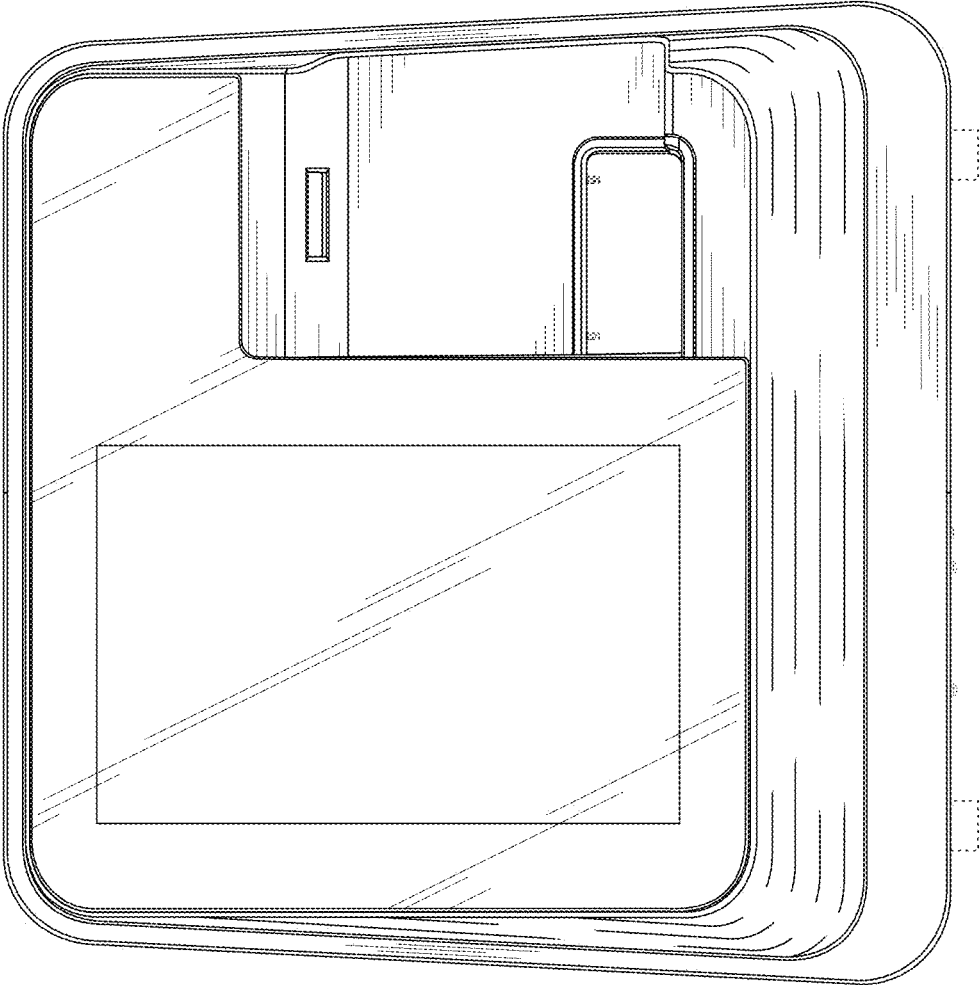


FIG. 2

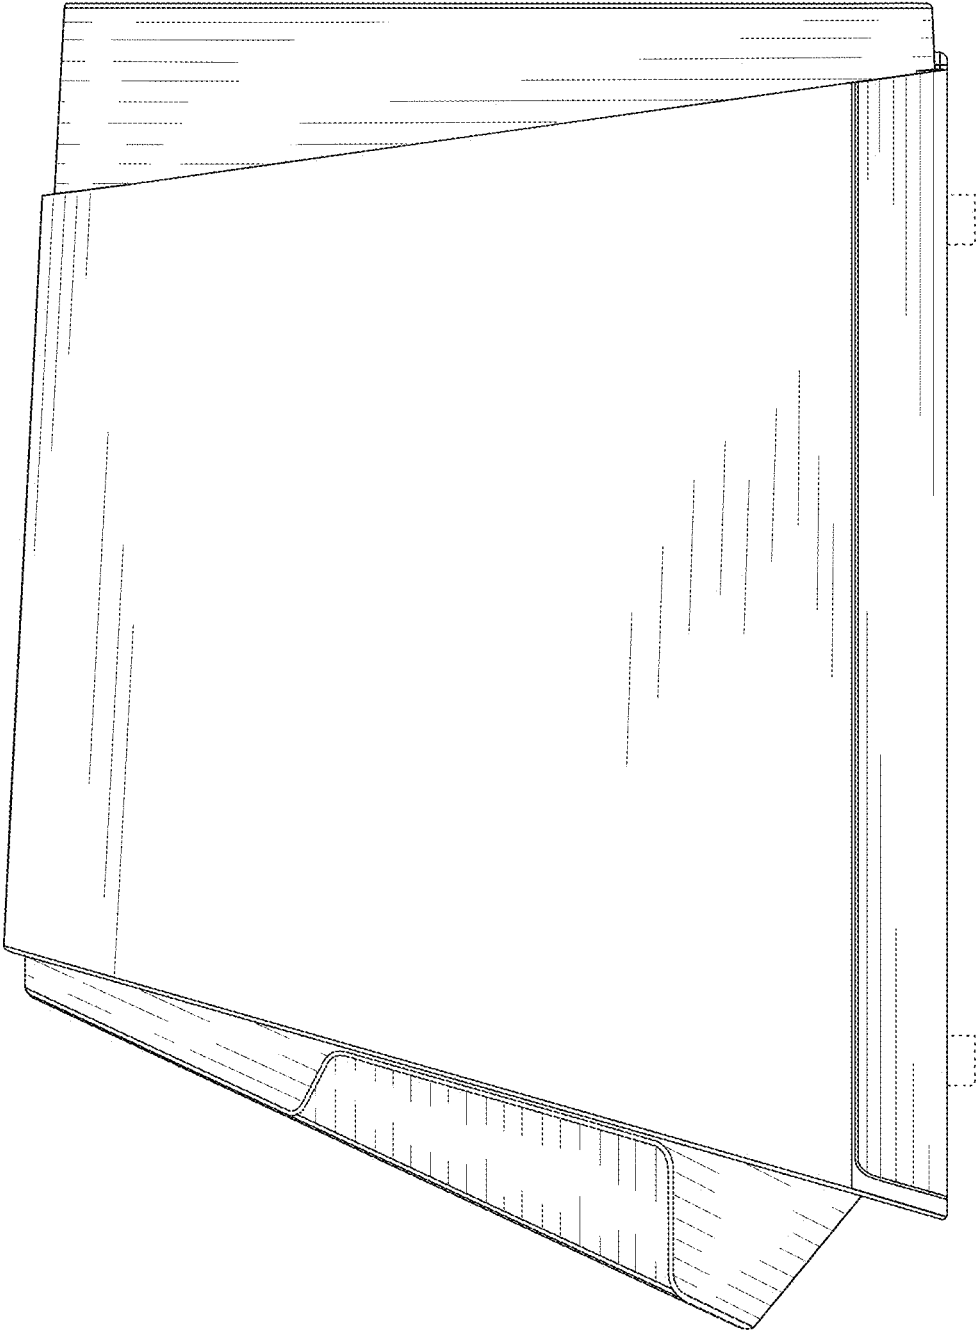


FIG. 3

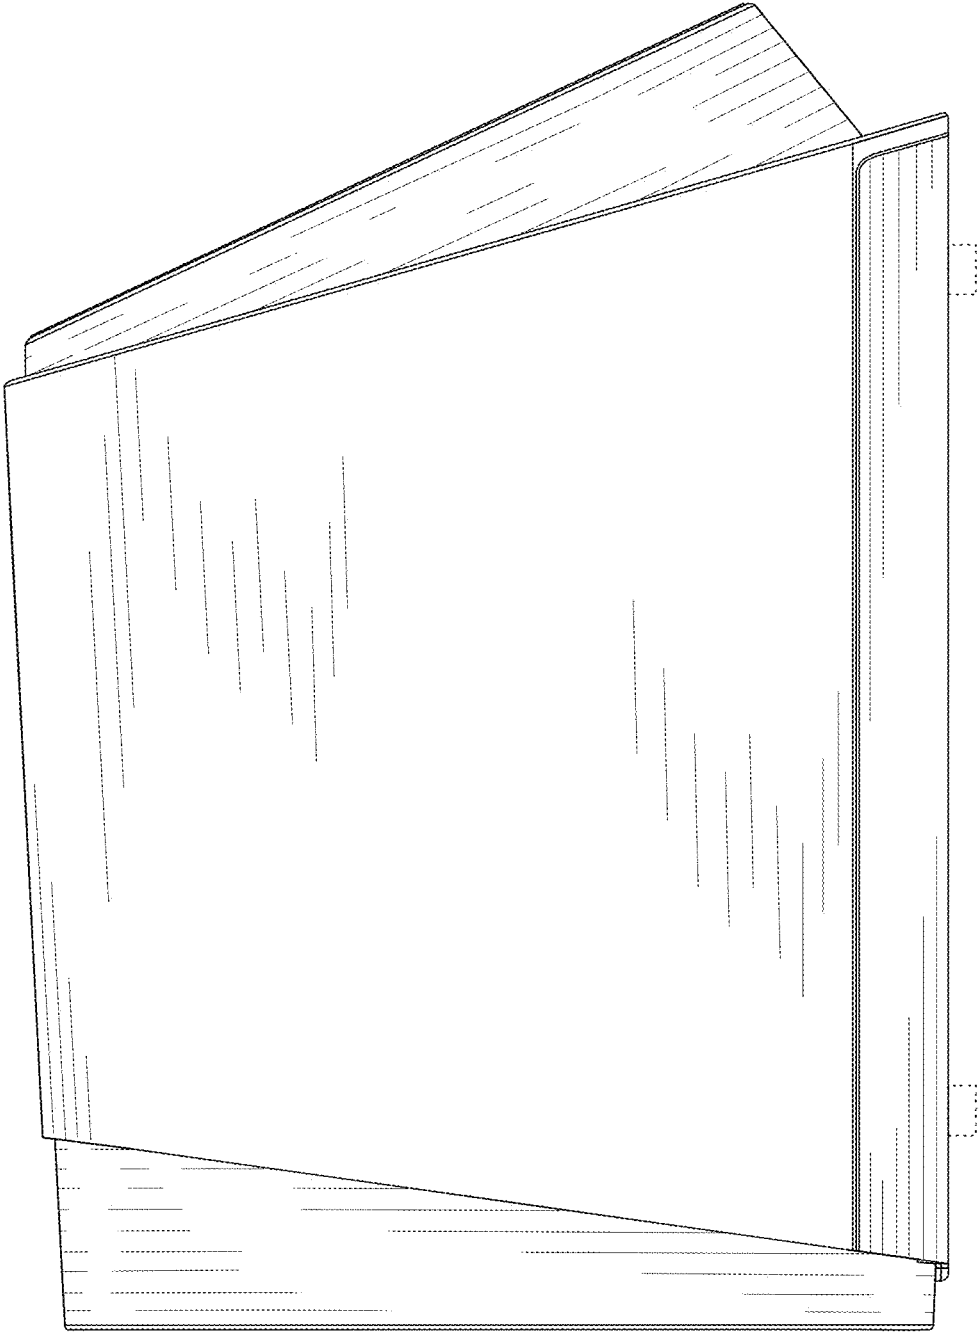


FIG. 4

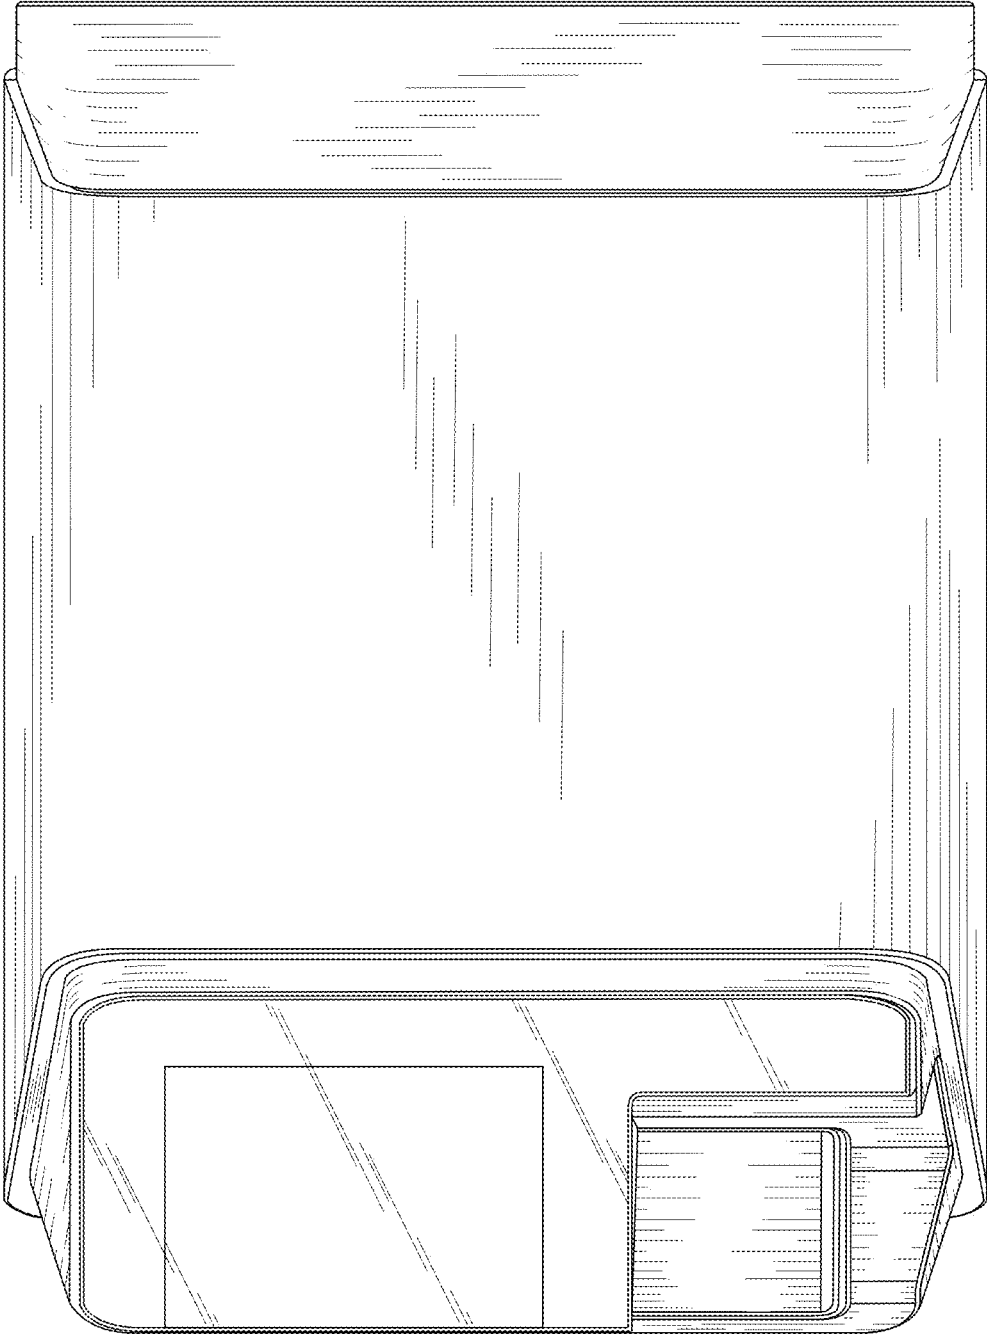


FIG. 5

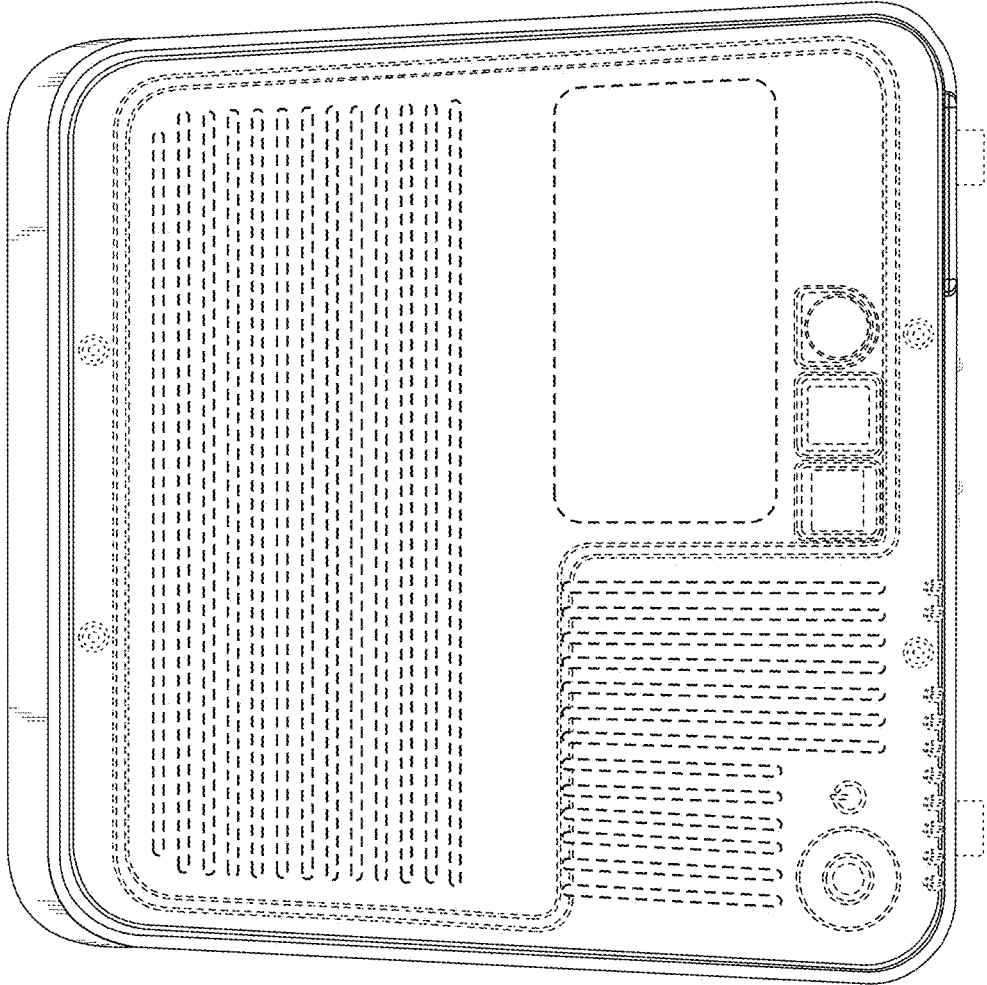


FIG. 6

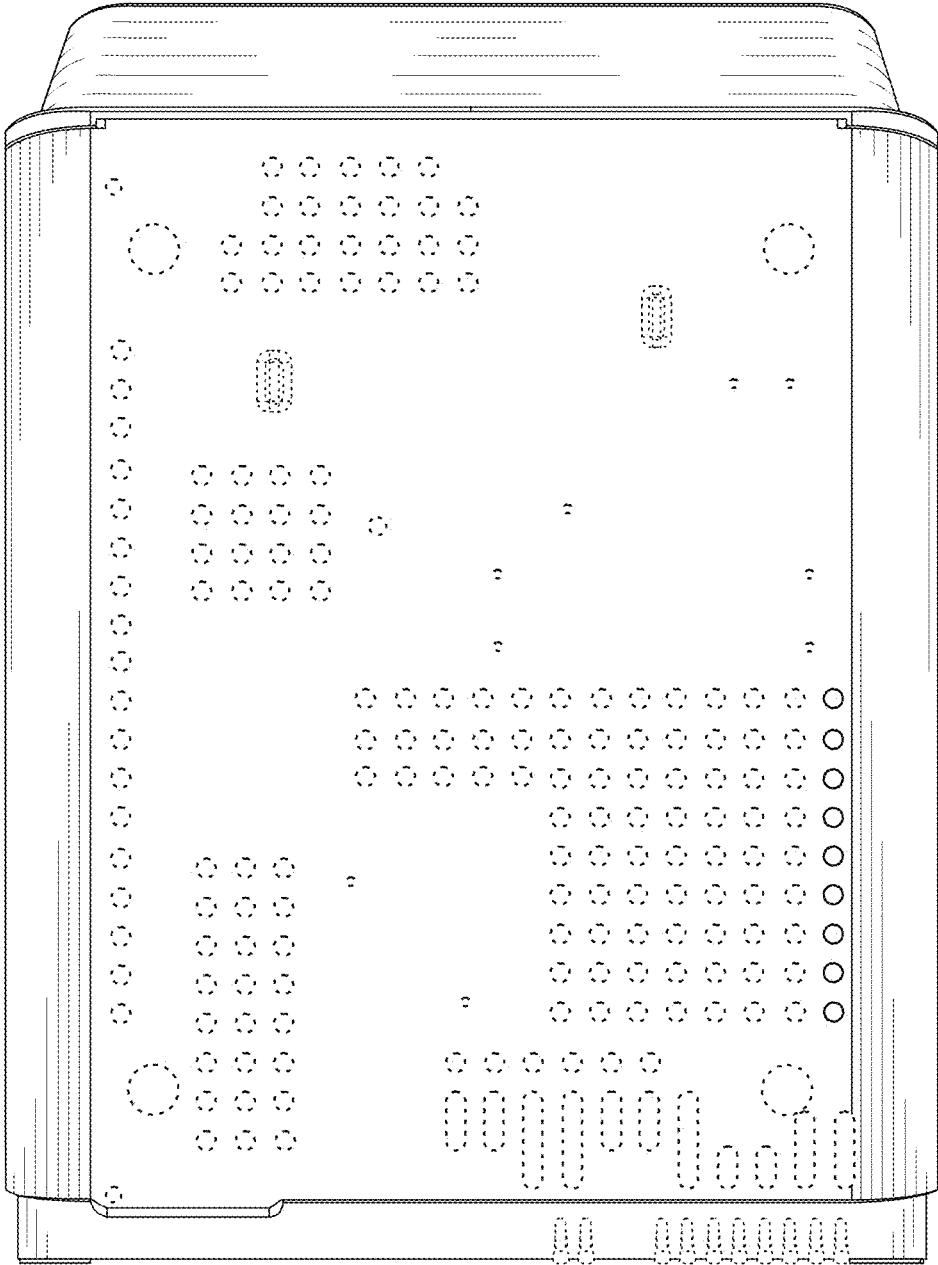


FIG. 7