




## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification <sup>6</sup> : <b>A61B 17/39</b></p>	<p><b>A1</b></p>	<p>(11) International Publication Number: <b>WO 99/62413</b></p> <p>(43) International Publication Date: 9 December 1999 (09.12.99)</p>
<p>(21) International Application Number: PCT/US98/27876</p> <p>(22) International Filing Date: 31 December 1998 (31.12.98)</p> <p>(30) Priority Data: 09/087,361 29 May 1998 (29.05.98) US</p> <p>(71) Applicant (for all designated States except US): APPLIED MEDICAL RESOURCES CORPORATION [US/US]; Suite 103, 26051 Merit Circle, Laguna Hills, CA 92653 (US).</p> <p>(72) Inventors; and (75) Inventors/Applicants (for US only): HART, Charles, C. [US/US]; 8252 Mandeville Drive, Huntington Beach, CA 92646 (US). HILAL, Nabil [US/US]; 25291 Spindlewood, Laguna Niguel, CA 92677 (US). EWERS, Richard, C. [US/US]; 7742 Alhambra, Huntington Beach, CA 92647 (US). PRAVONGVIENGKHAM, Bounsavanh [LA/US]; 450 Wilson Circle, Corona, CA 91719 (US).</p> <p>(74) Agent: MYERS, Richard, L.; Suite 103, 26051 Merit Circle, Laguna Hills, CA 92653 (US).</p>		<p>(81) Designated States: CA, JP, US, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).</p> <p><b>Published</b> <i>With international search report.</i></p>

(54) Title: IMPROVED ELECTROSURGICAL CATHETER APPARATUS AND METHOD

(57) Abstract

A catheter (10) adapted to increase the patency of a body conduit includes an elongate tube (25) having an axis extending between a proximal end, and a distal end, and a balloon (45) disposed at the distal end of the tube having properties for being expanded to a high profile state, and for being contracted to a low profile state. A sleeve (47) disposed over the balloon has a pair of ends disposed on opposing sides of a central section, the ends having a floating relationship relative to the tube with the central section disposed circumferentially of the balloon. An electrode (50) disposed outwardly of the sleeve has properties for being electro-surgically energized to incise materials defining the body conduit when the balloon is in the high profile state. The electrode can be formed of a plurality of elements stranded to increase the surface area of the electrode. The catheter can be inserted relative to a guide member (41) having a conductor which carries the electro-surgical energy from the proximal end of the tube to the electrode at the distal end of the tube. An associated method includes the step of introducing electro-surgical energy into the conductor of the guide member to energize the electrode of the catheter.

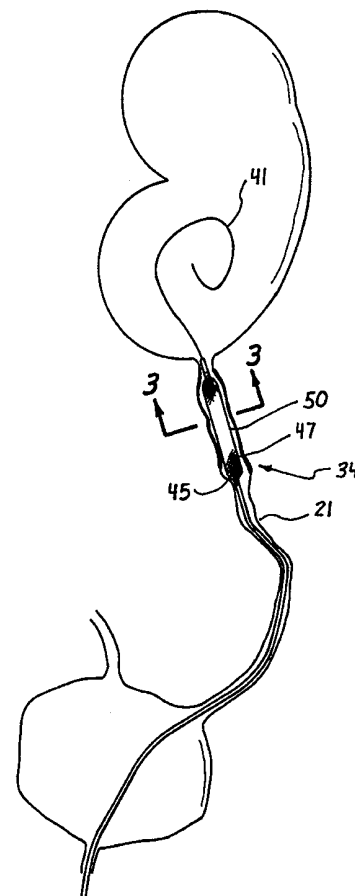

*FOR THE PURPOSES OF INFORMATION ONLY*

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

IMPROVED ELECTROSURGICAL  
CATHETER APPARATUS AND METHOD

5

Background of the Invention

Field of the Invention

This invention relates generally to surgical devices and more specifically to  
10 electro-surgical catheters adapted to incise body material defining a body conduit.

Discussion of the Prior Art

Various surgical devices have been used to electro-surgically ablate or otherwise cut  
body materials. In this type of surgery, electro-surgical energy is passed between two  
15 electrodes creating a high current density which ablates the body materials. In a typical  
monopolar system, the patient is coupled to a large grounding pad which forms one of the  
electrodes. The electro-surgical device forms the other electrode. In this system, the  
electro-surgical device provides a very low surface area and consequently a very high current  
density for ablation or cutting in proximity to the device. In a bipolar system, the two  
20 electrodes are included in the device and high current density is achieved in the small area  
between the electrodes.

These electro-surgical devices include a catheter having a balloon and an electrode  
extending over the surface of the balloon as disclosed in applicant's co-pending applications,  
Serial No. 08/241,007, filed on May 11, 1994, and entitled "Angioplasty Catheter and Method  
25 for Making Same", and Serial No. 08/216,512, filed on March 22, 1994, and entitled  
"Improved Catheter with Electro-surgical Cutter". The entirety of this disclosure is  
incorporated herein by reference. This catheter is used in a monopolar system where an  
electrode, in the form of a wire, is disposed over a radially expandable balloon of the catheter.  
As the balloon is inflated, the electrode is carried radially outwardly into proximity with the  
30 body material to be ablated or cut. Although it has always been of interest to increase the  
current density associated with the wire electrode, this has been difficult to achieve as smaller  
wire sizes necessarily result in reduced electrode strength and integrity. The balloon material  
has also been restricted to insure against over-expansion and electrode proximity. Materials  
forming non-distensible balloons have been preferred, but have made it difficult to achieve a  
35 low-profile state for insertion.

### Summary of the Invention

5 In accordance with the present invention, an electrosurgical catheter is provided with a balloon and an electrode extending axially along the outer surface of the balloon. A sleeve is disposed over the balloon and provided with ends which float along the catheter body between a low-profile state and a high-profile state for the sleeve. In the high-profile state, the sleeve has a predetermined maximum diameter which limits the radial dimension of the balloon.

10 Portions of the electrode extend through the sleeve to facilitate the electrosurgical function. The sleeve can also be provided with characteristics whereby the sleeve is biased to its low-profile state further facilitating a minimal profile for the catheter. The sleeve will typically be manufactured of a thermoplastic or thermoset material.

The sleeve can be formed from a plurality of elements which are woven, braided, or otherwise stranded to form an expandable structure. The electrode may form one of these elements in the sleeve. The electrode may also be formed from elements which are stranded to increase the surface area of the electrode without increasing its diameter. The electrode, the balloon, or the sleeve can be coated with an insulation to control the electrical relationships between these elements.

20 For example, the electrode can be formed of stranded elements which provide the electrode with an outer surface having peaks and valleys. Portions of this insulation can be removed to expose the elements in a straight or curved pattern. The electrode can be connected at each of its ends through conductors to the proximal end of the catheter thereby facilitating increased current flow to the electrode.

25 In another embodiment, the guidewire can be provided with an electrically conductive core which is exposed through insulation to energize the electrode at the distal end of the catheter. Using the guidewire as a conductor eliminates the need for an additional conductor in the catheter to energize the electrode. The conductive guidewire also facilitates operative disposition of the catheter at the surgical site.

30 In a semi-bipolar system, either the balloon or the sleeve can be used as a second electrode replacing the grounding pad in a typical monopolar system. With the wire forming one of the electrodes, the metalized balloon or sleeve forms the other electrode in a semi-bipolar system. This system provides the advantage of current density at the wire, but does not require electrical current to be conducted throughout the body of the patient. The

electrosurgical current need only flow from the active electrode with a minimal surface area to the balloon or sleeve which provide a high-surface area.

In one aspect of the invention, a catheter is adapted to increase the patency of a body conduit and comprises an elongate tube having an axis extending between a proximal end and a distal end. A balloon is disposed at the distal end of the tube and provided with properties for being expanded to a high-profile state and for being contracted to a low-profile state. A sleeve is disposed over the balloon and provided with a pair of ends which define a central section of the sleeve. The ends of the sleeve are disposed to floatingly engage the tube with the central section disposed circumferentially of the balloon. An electrode includes portions disposed outwardly of the sleeve and having properties for being electrosurgically energized to incise the body materials and increase the patency of the body conduit.

In another aspect of the invention, the electrode is formed of a plurality of elements stranded between a proximal end and a distal end to provide the electrode with an elongate configuration.

In a further aspect of the invention, the electrode has a radial cross-section which is non-circular in configuration.

In a further aspect of the invention, a guide member is adapted to facilitate insertion of a catheter into a body conduit. The guide member includes a core extending along an axis between a proximal end and a distal end, the core having properties for conducting energy. Insulation is disposed over the core with a portion of the insulation defining an exposed portion of the core at the proximal end of the guidewire and at the distal end of the guidewire.

In a further aspect of the invention, a combination includes the guide member and a catheter with an elongate shaft adapted to be moved along the guide member. An electrode disposed along the catheter is coupled to an exposed conductive core of the guide member to permit passage of energy from the proximal end of the guidewire along the core to the electrode at the distal end of the catheter.

These and other features and advantages of the invention will be more apparent with a description of preferred embodiments and reference to the associated drawings.

Description of the Drawings

Fig. 1 is a top-plan view of a patient illustrating operative placement of an  
5 electrosurgical balloon catheter in the upper pelvic junction between a kidney and a bladder of  
the patient;

Fig. 2 is an enlarged plan view with the distal end of the catheter disposed in the upper  
pelvic junction of the ureter;

Fig. 3 is a radial cross-section view taken along lines 3-3 of Fig. 2;

10 Fig. 4 is a side elevation view of the catheter with its distal end in a low-profile state;

Fig. 5 is a side elevation view similar to Fig. 4 with the distal end of the catheter  
illustrated in a high-profile state;

Fig. 6 is an enlarged radial cross-section view taken along lines 6-6 of Fig. 5;

Fig. 7 is an enlarged radial cross-section view taken along lines 7-7 of Fig. 5;

15 Fig. 8 is a perspective view of an electrode conductor of the prior art having a circular  
cross-section;

Fig. 9 is a perspective view of one embodiment of an electrode conductor of the  
present invention having a non-circular cross-section;

20 Fig. 10 is a perspective view of a further embodiment of the conductor comprising  
discrete elements stranded to form the electrode;

Fig. 11 is a perspective view of a further embodiment of the conductor wherein each  
element is comprised of separate fibers and the elements define the electrode with a generally  
hollow configuration;

25 Fig. 12 is a perspective view of a further embodiment of the electrode similar to  
Fig. 11, but having a generally solid, non-hollow configuration;

Fig. 13 is a plan view of an electrode having at least one conductor element formed in  
a spiral configuration, and a coating of insulation with portions removed to form discrete  
windows for element exposure;

Fig. 14 is an axial cross-section view taken along lines 14-14 of Fig. 13;

30 Fig. 15 is a top-plan view similar to Fig. 13 with the windows oriented in a radial  
configuration;

Fig. 16 is a top-plan view similar to Fig. 13 with the windows oriented in an axial  
configuration;

Fig. 17 is a top-plan view similar to Fig. 13 with the windows oriented in a spiral configuration;

Fig. 18 is a perspective view of a further embodiment of the electrode similar to Fig. 10 wherein multiple elements are stranded and individually energizable to control conductivity through associated windows in the insulation;

Fig. 19a is a side-elevation view illustrating the balloon partially metalized to facilitate a semi-bipolar operation and visual radial orientation of the electrode;

Fig. 19b is a cross-section view taken along lines 19b-19b of Fig. 19a;

Fig. 20a is a side-elevation view similar to Fig. 19a and illustrating the catheter rotated 45° from the orientation of Fig. 19a;

Fig. 20b is a radial cross-section view taken along lines 20b-20b of Fig. 20a;

Fig. 21a is a side-elevation view illustrating the catheter rotated 90° from the orientation of Fig. 19a;

Fig. 21b is a radial cross-section view taken along lines 21b-21b of Fig. 21a;

Fig. 22a is a side elevation view illustrating the catheter rotated 135° from the orientation of Fig. 19a;

Fig. 22b is a radial cross-section view taken along lines 22b-22b of Fig. 22a;

Fig. 23a is a side elevation view illustrating the electrode rotated 180° from the orientation of Fig. 19a;

Fig. 23b is a radial cross-section view taken along lines 23b-23b of Fig. 23a;

Fig. 24a is a side elevation view similar to Fig. 5 and illustrating an embodiment wherein the electrode is energized through two conductors;

Fig. 24b is an enlarged side-elevation view of the electrode illustrated in Fig. 24;

Fig. 25 is a side-elevation view of a semi-bipolar embodiment of the catheter;

Fig. 26 is an enlarged view of the distal end of the catheter illustrated in Fig. 25;

Fig. 27 is an assembly view of a catheter system wherein a guidewire is used to energize the electrode of the catheter;

Fig. 28 is an assembled view of the elements illustrated in Fig. 27; and

Fig. 29 is a radial cross-section view of the assembled elements of Fig. 28 illustrating the conduction of electrosurgical energy from the proximal end of the guidewire to the electrode of the catheter.

Description of Preferred Embodiments  
and Best Mode of the Invention

5           A catheter is illustrated in Figure 1 and designated generally by the reference numeral 10. The catheter 10 is illustrated to be operatively disposed in a patient 12 having a ureter 14 extending between a kidney 16 and a bladder 18. The catheter 10 is adapted to increase the patency of the ureter 14, particularly at the upper pelvic junction 21 which is commonly occluded by strictures 23.

10           The catheter 10 typically includes an elongate tube 25 having a lumen 27 extending through a hub 30 at a proximal end 32, and an electrode assembly 34 at a distal end 36. The electrode assembly 34 is electrically energized through a conductor 38 at the proximal end 32. Operative placement of the catheter 10 can be facilitated by a guide catheter or a guidewire 41.

15           Figure 2 shows an enlarged view of the upper pelvic junction 21 with the electrode assembly 34 including a balloon 45, a sheath 47 extending over the balloon 45, and an electrode 50. These elements are perhaps more easily identified in the radial cross-section view of Figure 3.

20           The side elevation views of Figures 4 and 5 illustrate the electrode assembly 34 in a low-profile state and a high-profile state, respectively. In the low-profile state of Figure 4, the catheter 10 is adapted for insertion through the bladder 18 and into the ureter 14. Once the catheter 10 is operatively disposed, the balloon 45 is expanded, for example by inflation, to a high-profile state, as illustrated in Figure 5. In the high-profile state, as illustrated in Figure 2, the balloon 45 functions to carry the electrode 50 radially outwardly into proximity with the strictures 23 to facilitate the electrosurgical effect. The balloon 45 in the high-profile state  
25           also functions to tension the walls of the ureter 14 so that the ureter 14 expands as the strictures 23 are cut by the electrode 50. Any potential for bleeding is inhibited by the tamponade effect of the inflated balloon 45.

30           The cross-section views of Figures 6 and 7 illustrate a preferred embodiment wherein the electrode 50 exists the tube 25 exteriorally of the balloon 45, but interiorly of the sheath 47. Portions of the electrode 50, designated generally by the reference numeral 52, extend through the sheath where they are exposed axially along the outer surface of the sheath 47.



The side elevation views of Figures 4 and 5 are perhaps best suited to disclose another feature of the present invention. In these figures, the balloon has ends which are fixed to the tube 25 by windings 54, 56. With the windings 54, 56 fixed to the tube, axial movement of the balloon 45 is inhibited, so that expansion of the balloon 45 is limited generally to the radial direction. By comparison, the ends of the sheath 47 are fixed to bushings 58, 61 which are separated by a central section 63 are free to float axially along the tube 25. Thus, the bushings 58 and 61 have inside diameters which are greater than the outside diameter of the tube 25. In the low-profile state illustrated in Figure 4, the bushings 58 and 61 have a maximum distance of separation as the length of the sheath 47 increases in response to radial compression of the balloon 45 and the sheath 47.

As the balloon 45 expands radially outwardly, it carries with it the central section 63 of the sheath 47. This radial expansion of the sheath 47 draws the floating bushings 58, 61 together reducing their distance of separation. In the high-profile state illustrated in Figure 5, the floating bushings 58, 61 of the sheath 47 abut the fixed windings 54, 56 of the balloon 45. At this point, the distance separating the bushings 58, 61 can no longer be reduced. With the ends of the sheath 47 limited against further proximal movement, the maximum diameter of the sheath 47 is fixed to a diameter which dictates the predetermined high-profile state of the electrode assembly 34. Note that this also fixes the maximum radial separation of the catheter tube 25 and the exposed portions 52 of the electrode 50.

Theoretically, the electrode 50 and the conductor 38 should be sized and configured to conduct the maximum amount of current through the conductor 38 to the electrode 50, and then to provide an electrode 50 of minimum surface area in order to increase the current density at the electrode 50. Of course, there are maximum size and flexibility constraints on the conductor 38, as well as strength and integrity constraints on the electrode 50 which place practical demands on these theoretical considerations. In the past, both the conductor 38 and the electrode 50 have been formed of wires having a circular cross-section as illustrated in Figure 8. Within the practical constraints noted, the round conductor 38 has been chosen with a maximum diameter and the round electrode 50 has been chosen with a minimum diameter. In U.S. Patent No. 5,628,746, Applicant discloses and claims a concept for providing a relatively large electrode wire with surface insulation that is removed to expose only a very small area of the electrode. This has had the same effect of providing a high-current density, but has enabled use of a relatively large electrode to do so. As a result, electrodes as large as the associated conductors have been used in the past. When the practical constraints on the

conductor have been maximized, embodiments providing for a relatively large electrode tapering to a relatively small conductor have been used.

Against this background of evolution, it has now been found that electrical energy passing through a conductor at radio frequencies tends to flow along the outer surface of the conductor. This is referred to as the "skin effect." Taking this phenomena into account, the conductor 38 and electrode 50 of the present invention can be provided with a generally non-circular shape in axial cross-section. This shape can take the form illustrated in Figure 9, for example, or can naturally result from a stranded conductor 38, as illustrated in Figure 10. In this embodiment, the conductor 38 electrode 50 include at least two elongate elements 70, 72 which are stranded, such as woven, braided, or twisted, along an axis 75 from the proximal end of the conductor 38 through to the distal end of the electrode 50. These elements 70, 72 may have a circular cross-section, as illustrated in Figure 10, or may also be provided with a non-circular cross-section maximizing their individual surface areas.

Another embodiment illustrated in Figure 11 provides an even further increase in the surface area of the conductor 38 and electrode 50. In this embodiment, each of the elements 70, 72 is formed of a plurality of fibers 74. These fibers 74 are twisted together to form the individual elements 70, 72, which are further twisted together to form the conductor 38 and electrode 50. In the Figure 11 embodiment, the resulting conductor 38 and electrode 50 have a generally hollow configuration so that none of the elements, such as the elements 70 and 72, extend along the axis of the conductor 38. By comparison, the conductor 38 and electrode 50 illustrated in Figure 12 include a further element 76 which extends along the axis 75, with the remaining elements 70, 72 twisted around the core element 76.

From these embodiments illustrated in Figures 9-12, it will be apparent that an increased surface area can be achieved generally with any non-circular cross-section. In Figure 9, the conductor 38 is solid and the outer surface is sculptured to provide the increased surface area. In the embodiment of Figure 10, multiple elements are stranded to provide the increased surface area. The cross-section of these individual elements can also be non-circular. Importantly, there can be two or more elements, such as the elements 70, 72, in this embodiment. The more elements, the greater the surface area. This is more apparent from the Figure 11 embodiment which includes six elements, such as the elements 70, 72. To further increase the surface area, each of these elements is formed from individual fibers which can also be provided with other than round cross-sections. Whether the cross-section of the

connector 38 is hollow, as illustrated in Figure 11, or generally solid, as illustrated in Figure 12, it is apparent that the surface area of the conductor 38 is greatly increased over the generally cylindrical circular cross-section associated with the conductors and electrodes of the prior art.

5 Turning now to the electrode 50 illustrated in Figure 13, it will be apparent that the conductor 38 with a spiraled configuration can offer significant advantages when covered with an insulation 81. When this insulation is removed, individual windows 83 are formed and exposed portions 86 of the convolutions 85 are individually exposed. This is perhaps best illustrated in the axial cross-section view of Figure 14 where the insulation 81 is removed in  
10 an area designated generally by the reference numeral 87. From this view it can be seen that the outer surface of the convolutions 85 forms peaks 89 alternating with valleys 91. When the insulation is removed from the area 87, it tends to remain in the valleys 91 so that only the peaks 89 and the convolutions 85 are exposed. This produces the individual windows 83 and the discreet, exposed convolutions 85 of the conductor 38, as illustrated in Figure 13.

15 It should be noted that with this window configuration, the exposed area of the conductor 38 can be even further reduced, greatly increasing the current density of the electrode 50. In the past, the entire conductor was exposed within the area of the removed insulation 87. In the window embodiment, as illustrated in Figure 13, the much smaller area of exposure can provide a substantial increase in current density.

20 From these views, it can be appreciated that the particular surface configuration associated with the conductor 38, and the pattern for removing the insulation 81, can provide the windows 83 and the exposed portions 86 of the conductor 38 with different spatial relationships. For example, in Figure 15, the windows 83 and exposed portions 86 have a curved, radial relationship. In Figure 16, the windows 83 and exposed portions 86 have a  
25 generally straight, axial relationship. Finally, in Figure 17, the windows 83 and exposed portions 86 are curved with a spiral relationship.

A further embodiment of the invention is illustrated in Figure 18 wherein the conductor 38 is formed of multiple elements as taught generally with reference to Figures 10, 11. These elements 70, 72 are individually provided with an insulation coating 101 Figure 18,  
30 which enables them to be individually and separately energized or controlled. While this control may provide for variations in the magnitude of energy, it will typically be a matter of timing that energy at each window 83. Thus, the individual and discreet windows 83 and the

insulation 81 can be separately, and perhaps progressively, energized to further maximize the current density as the elements 70, 72 are selectively energized at the associated windows 83.

A further embodiment of the invention is illustrated in Figures 19a-23a and their associated cross-sectional views in Figures 19b-23b. In this embodiment, the balloon 45 is provided with a metal coating 105, but only along a portion of its radial surface. For example, in the views illustrated, the metal coating 105 extends only 180° around the circumference of the balloon 45. This greatly aids in the radial orientation of the balloon 45 and, of course, facilitates operative disposition of the electrode 50. Radiopaque markers 107 can also be provided to further enhance axial location of the catheter 10.

Viewing the catheter 10 fluoroscopically will present a side-elevation view such as those associated with Figures 19a-23a. From these fluoroscopic observations, the surgeon will attempt to rotate the catheter 10 along its axis in order to accurately place the electrode 50 in the desired radial disposition. By providing the balloon 45 with the metalized coating 105, a sharp line of demarcation 109 is now apparent along the entire length of the balloon 45. If the surgeon requires an upper placement of the electrode 50, the catheter 10 can merely be turned on its axis until the fluoroscopic view of Figure 19a is achieved. Different fluoroscopic views can be sought to achieve other preferred positions for the electrode 50. For example, progressive 45° turns in a clockwise direction are illustrated in the side-elevation views of Figures 19a-23a.

It should be apparent from these views that the metalized coating 105 greatly facilitates operative disposition of the electrode 50. Although a semi-cylindrical placement of the coating 105 is illustrated in this embodiment, many other shapes of the coating 105 can also be relied on to facilitate radial placement of the electrode 50. Fluoroscopically, the embodiment illustrated in Figures 19a-23a provides the longest line of demarcation 109 and perhaps the greatest visual indication of electrode orientation. It should also be noted that the metalized coating, such as the coating 105 on the balloon 45, can also be applied to the sheath 47 individually or in combination with the balloon 45.

As previously discussed, it is desirable to maximum the magnitude of radio frequency current which can be delivered to the electrode 50. In the past, the electrode 50 has been provided with a proximal end 110 and a distal end 112. The proximal end 112 has been coupled to the connector 38 in order to energize the electrode 50. More typically, the metal core of the electrode 50 has been formed integral with the conductor 38 as a mere extension of

the conductor 38. The distal end 112 of the electrode 50 has been terminated in the tube 25 of the catheter 10.

In accordance with the embodiment Figure 24, a second conductor 114 is provided which extends through the hub 30 at the proximal end 32, and is coupled to the distal end 112 of the electrode 50. The second conductor 114 provides a further path for the transmission of electrical current to the electrode 50. The resulting increase in current which can be transmitted provides a commensurate increase in current density at the electrode 50.

A semi-bipolar embodiment of the catheter 10 is illustrated in Figure 25. In this embodiment, either or both the balloon 45 and the sheath 47 have a metallic outer surface 118 which provides a large area of contact with the body material, such as the strictures 23 (Figure 1), which define the body conduit. In this embodiment, the conductor 38 is connected to the electrode 50 in the manner previously discussed. A second conductor 121, also emanating from the hub 30, is connected to the metallic surface 118. With the electrosurgical signal introduced across the conductors 38 and 121, the catheter 10 tends to function in a bipolar mode with current passing from the relatively small surface area of the electrode 50 to the relatively high surface area of the metallic surface 118. This configuration is bipolar in that both of the poles of the electrosurgical circuit are carried by the catheter 10. The configuration is monopolar to the extent that one of the poles presents a surface area so large that the current density at this pole has no effect upon the tissue of the patient. This embodiment is referred to herein as semi-bipolar.

In order to facilitate insertion of the catheter 10, it is always of interest to minimize the cross-sectional area of the tube 25. This is accomplished in a preferred embodiment illustrated in Figures 27-29, where the tube 25 has but a single lumen 27 (Figure 3). This lumen 27, which can be used to inflate the balloon 45, is primarily sized and configured to receive the guidewire 41.

The guidewire 41 in this case is especially constructed with a non-conductive distal portion 125 coupled at a junction 127 to a conductive proximal portion 130. The conductive proximal portion 130 is covered generally centrally with insulation 132 leaving exposed a distal patch 134 near the junction 127, and a proximal patch 136 at the proximal end of the guidewire 41.

At the proximal end of the catheter 10, the hub 30 can be provided with a threaded male fitting 138 which is adapted to receive the guidewire 41. A complimentary cap 141 includes a female fitting 143, adapted to receive the fitting 138, and a tube 145 which extends

proximally axially from the fitting 143. A conductor 147 is molded into a closed end 149 of the tube 145.

In operation, the guidewire 41 is inserted into the body conduit, such as the ureter 14, in a manner well-known in the art. The catheter 10 is then threaded over the proximal end of the guidewire 41 and pushed distally toward its operative position until the proximal end of the guidewire 41 is exposed at the hub 30. At this point, the cap assembly 141 is moved over the proximal end of the guidewire 41 until the proximal patch 136 achieves electrical conductivity with the conductor 147. Holding the hub 30 in one hand, and moving the cap assembly 141 forces the guidewire 41 distally relative to the catheter, but also brings the female fitting 143 into an abutting relationship with the male fitting 138. At this point, the cap assembly 141 can be tightened to the male fitting 138 to hold the catheter 10 and guidewire 41 in a fixed axial relationship. This relationship is facilitated by a radial seal 152 in the embodiment of Figure 29.

At the distal end of the catheter 10, the electrode 50 is provided with a proximal end 110 that is foreshortened, but exposed within the lumen 27 in proximity to the sheath 47. The exact location of the proximal end 110 of the electrode 50 is predetermined relative to the hub 30. This known distance can be used to locate the distal patch 134 of the conductor 130 on the guidewire 41 so that complete assembly of the guidewire 41 and catheter 10, as illustrated in Figure 29, brings the proximal end 110 of the electrode 50 into electrical contact with the distal conductive patch 134. With these structural relationships, electrosurgical energy applied to the conductor 147 at the proximal end of the cap assembly 141 will pass through the conductor proximal portion 130 to the conductive patch 134. This energy will then be transferred to the distal end 110 and into the electrode 50.

In this manner, the guidewire 41 can be used to energize the electrode 50, thereby eliminating the need for any energizing conductor such as the conductor 38 (Figure 5). It will be noted that, with the guidewire 41 thus configured, there are no conductive elements of the guidewire 41 which extend beyond the distal end of the catheter 10. Also, although the insulation 132 over the conductor portion 130 is provided in a preferred embodiment, this may be eliminated in another embodiment since the conductor 130 is effectively insulated by the tube 25 of the catheter 10. A further advantage associated with this system relates to the axial placement of the catheter 10. Once the guidewire 41 is axially oriented with the junction 127 disposed at a predetermined position, location of the catheter 10 and associated electrode 50 is fixed along the length of the guidewire 41. Not only is the catheter 10 fixed to

the guidewire 41 at this preferred location, but the electrode 50 is only energized at this predetermined location along the guidewire 41.

It will be understood that many other modifications can be made to the various disclosed embodiments without departing from the spirit and scope of the concept. For  
5 example, various sizes of the surgical device are contemplated as well as various types of constructions and materials. It will also be apparent that many modifications can be made to the configuration of parts as well as their interaction. For these reasons, the above description should not be construed as limiting the invention, but should be interpreted as merely exemplary of preferred embodiments. Those skilled in the art will envision other  
10 modifications within the scope and spirit of the present invention as defined by the following claims.

## CLAIMS

1. A catheter adapted to increase the patency of a body conduit, comprising:
  - an elongate tube having an axis extending between a proximal end and a distal end;
  - a balloon disposed at the distal end of the tube and having properties for being expanded to a high-profile state and for being deflated to a low-profile state;
  - 5 a sleeve being disposed over the balloon and having a pair of ends disposed on opposing sides of a central section;
  - the ends of the sleeve disposed to floatingly engage the tube with the central section of the sleeve disposed circumferentially of the balloon;
  - 10 the sleeve having properties for radially compressing the balloon when the balloon is in the low-profile state; and
  - an electrode having portions disposed outwardly of the sleeve, the electrode having properties for being electrosurgically energized to incise materials defining the body conduit when the balloon is in the high-profile state.
  
2. The catheter recited in Claim 1 wherein the sleeve has non-distendable properties for maintaining the balloon in its high-profile state at a predetermined diameter.
  
3. The catheter recited in Claim 1 wherein the tube in proximity to the balloon has a first outer diameter and the ends of the sleeve have a fixed diameter greater than the first outer diameter of the tube to facilitate axial flotation of the sleeve ends relative to the tube.
  
4. The catheter recited in Claim 2:
  - wherein the sleeve ends are free to float relative to each other between positions displaced by an axial distance of separation; and
  - the predetermined diameter of the balloon in the high-profile state is dependent
  - 5 upon the axial distance of separation of the sleeve ends.
  
5. The catheter recited in Claim 4, wherein:
  - the balloon has balloon ends fixed to the tube at axially spaced locations; and



the axial distance of separation of the sleeve ends as dependent upon the axially spaced location of the balloon ends.

6. The catheter recited in Claim 1 wherein the sleeve is formed of discreet elements interwoven to form a fabric.

7. The catheter recited in Claim 1 wherein the sleeve includes at least one of a thermoplastic and a thermoset material.

8. The catheter recited in Claim 6 wherein the electrode is interwoven into the sleeve.

9. The catheter recited in Claim 6 wherein the electrode forms one of the elements in the woven fabric of the sleeve.

10. The catheter recited in Claim 1, further comprising:  
a coating disposed between the electrode and the sleeve and having properties for insulating the sleeve against the electrode.

11. A catheter adapted to increase the patency of a body conduit, comprising:  
an elongate tube having an axis extending between a proximal end and a distal end;  
a balloon disposed at the distal end of the tube and having properties for being  
5 expanded from a low-profile state to a high-profile state;  
an electrode disposed outwardly of the balloon and having properties for being electrosurgically energized to incise the material forming the body conduit; and  
the electrode being formed of a plurality of elements stranded to form the electrode.

12. The catheter recited in Claim 11 wherein each of the stranded elements includes multiple fibers.

13. The catheter recited in Claim 11 wherein the stranded electrode has an outer surface including peaks and valleys, and the catheter further comprises:

an insulation disposed over the stranded electrode; and

the insulation including portions defining a plurality of windows each exposing  
5 an associated one of the peaks of the stranded electrode in a predetermined cutting pattern.

14. The catheter recited in Claim 13 wherein the predetermined pattern is one of an axial line, a radial line, and a spiral line.

15. The catheter recited in Claim 11 wherein the electrode has a proximal end and a distal end, and the catheter further comprises:

a first conductor disposed within the tube and providing electrical conductivity  
between the proximal end of the tube, and one of the proximal end and the distal end of the  
5 electrode.

16. The catheter recited in Claim 15 further comprising:

a second conductor disposed within the tube and providing electrical  
conductivity between the proximal end of the tube and the other of the proximal end and the  
distal end of the electrode.

17. The catheter recited in Claim 16 wherein one of the first conductor and the second conductor is a guidewire.

18. The catheter recited in Claim 11 further comprising:

a spring coupled to the electrode to bias the electrode toward a tensioned state.

19. A surgical electrode for ablating body material of a patient, the electrode having an axis extending between a first end and a second end of the electrode, and being adapted for movement toward the body material in a direction generally transverse to the axis of the electrode to ablate the body material, the electrode having in radial cross-section a non-  
5 circular configuration.

20. The surgical electrode recited in Claim 19 wherein the electrode has a maximum radial dimension (MRD), and an outer perimeter greater than the product of (and MRD).
21. The surgical electrode recited in Claim 19, further comprising:  
a first element having an elongate configuration and extending generally between the first end and the second end of the electrode;  
a second element having an elongate configuration and extending generally  
5 between the first end and the second end of the electrode; and  
the first element being intertwined with the second element to provide the electrode with the non-circular cross-section.
22. The surgical electrode recited in Claim 21 wherein the electrode is free of any elements extending along the axis of the electrode.
23. The electrode recited in Claim 21 wherein at least one of the first element and the second element in radial cross-section has the general shape of a circle.
24. The surgical electrode recited in Claim 23, wherein:  
the first element has in radial cross-section the general shape of a first circle with a first diameter;  
the second element has in radial cross-section the general shape of a second  
5 circle with a second diameter; and  
the first diameter of the first circle is generally equal to the second diameter of the second circle.
25. The surgical electrode recited in Claim 19 wherein the electrode is adapted to be energized by a radio frequency current to ablate the body material of the patient.
26. A guidewire having an outer surface and being adapted to facilitate insertion of a catheter into a body conduit, comprising:  
a core extending along an axis between a proximal end and a distal end, the core having properties for conducting energy;

5 a sleeve disposed over the core and defining a major portion of the outer surface of the guidewire, the sleeve having properties for insulating the body conduit from the core; and

portions of the sleeve defining a patch wherein a portion of the core is exposed, the exposed portion of the core defining a minor portion of the outer surface of the guidewire.

27. The guidewire recited in Claim 26 wherein the catheter is adapted to be positioned with the exposed portion of the core extending into proximity with a surgical site.

28. The guidewire recited in Claim 27 wherein the catheter is adapted to be positioned with the distal end of the core in proximity to the surgical site and the exposed portions are in proximity to the distal end of the core.

29. The guidewire recited in Claim 26 wherein the sleeve forms a coating of insulation on the core of the guidewire.

30. The guidewire recited in Claim 26 wherein the energy is electrical energy at electrosurgical frequencies.

31. A combination including:  
a guide member adapted to be disposed in a body conduit;  
a core included in the guide member and having properties for conducting energy;

5 insulation included in the guide member and forming a cover extending over the core, portions of the insulation defining a window to expose portions of the core of the guide member;

a catheter including an elongate tube sized and configured to be moved along the guide member; and

10 an electrode disposed along the catheter, the electrode being coupled to the core of the guide member through the window defined by the insulation to permit conduction of the energy from the core of the guide member through the window to the electrode.

32. The combination recited in Claim 31 wherein the energy is electrosurgical energy.

33. The combination recited in Claim 31, wherein:  
the guide member is a guidewire;  
the tube of the catheter defines an internal lumen sized and configured to receive the guidewire;

5 the portions of the core of the guidewire are exposed to the lumen of the catheter when the guidewire is operatively disposed; and

the electrode extends into the lumen to contact the portions of the core of the guidewire.


34. A method for energizing an electrode at a distal end of an electrosurgical catheter operatively disposed in a body conduit, comprising the steps of:

inserting into the body conduit a guide member having an elongate configuration and a conductor extending along at least a portion of the length of the guide member;


5 inserting the catheter into the body conduit relative to the guide member;  
during the inserting step electrically contacting the conductor of the guidewire with the electrode of the catheter; and

10 introducing electrosurgical energy into the conductor of the guidewire to energize the electrode of the catheter in the body conduit.


*Fig. 1*

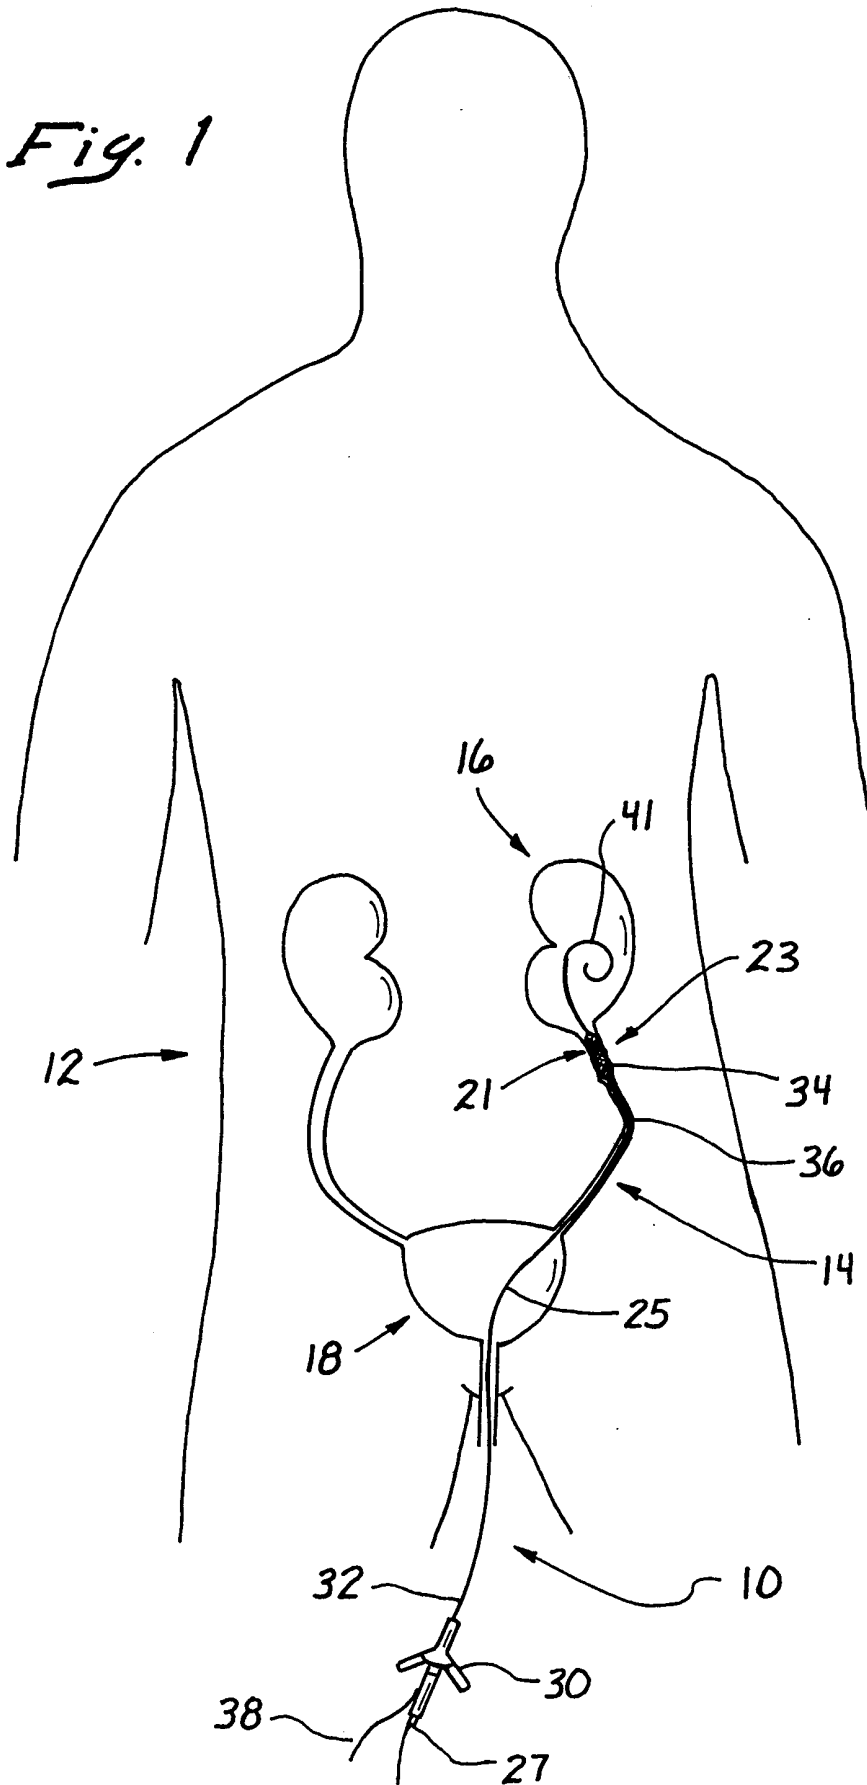

*Fig. 2*

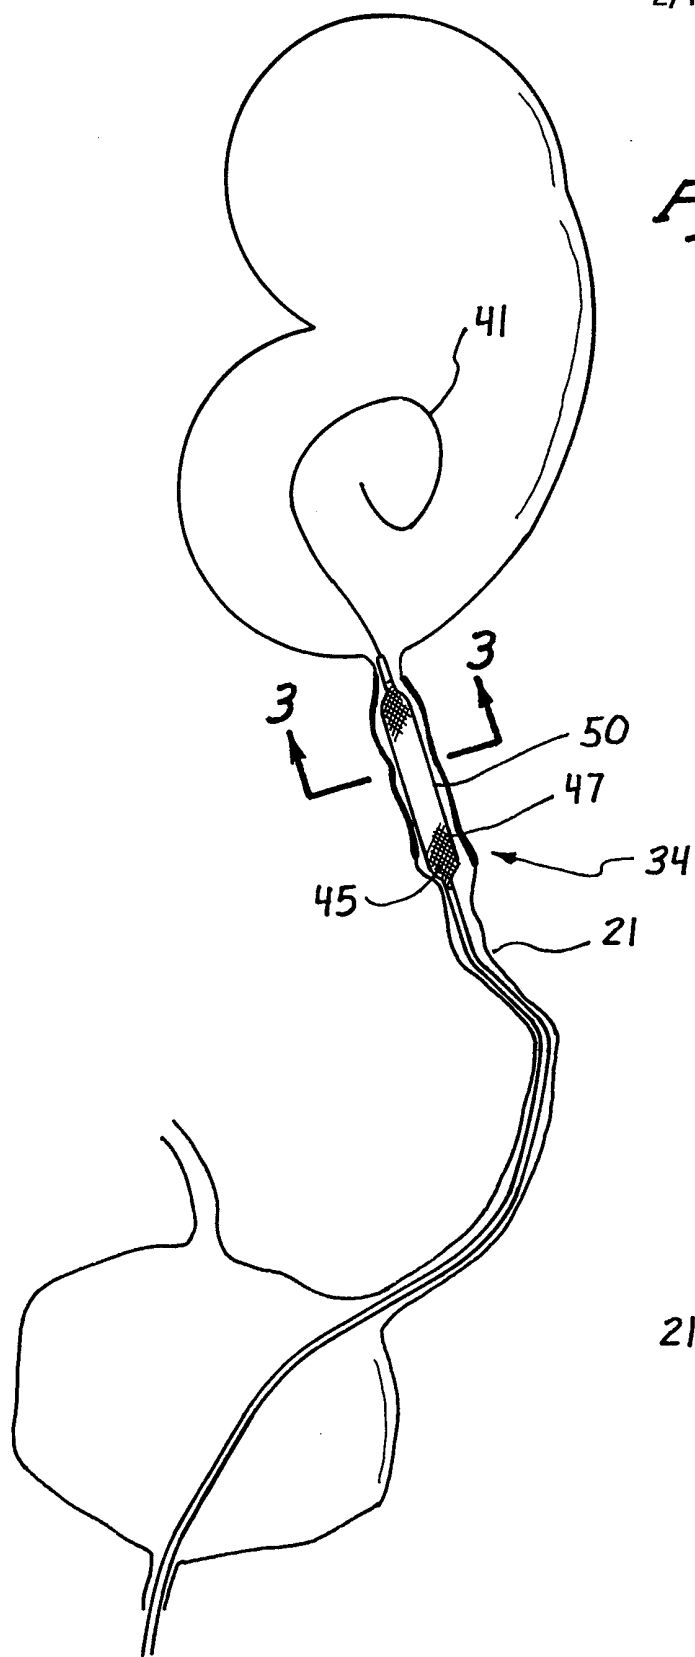

*Fig. 3*

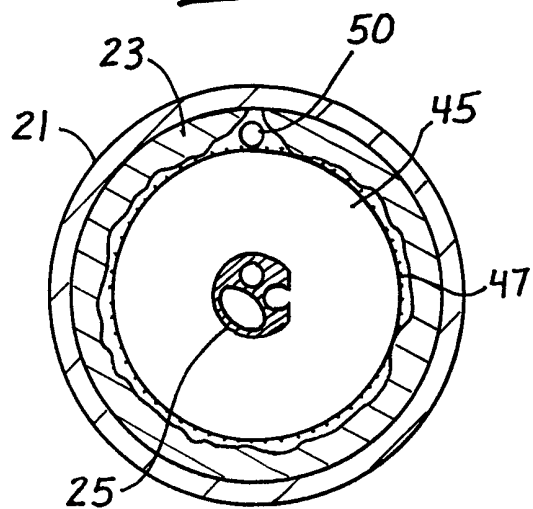

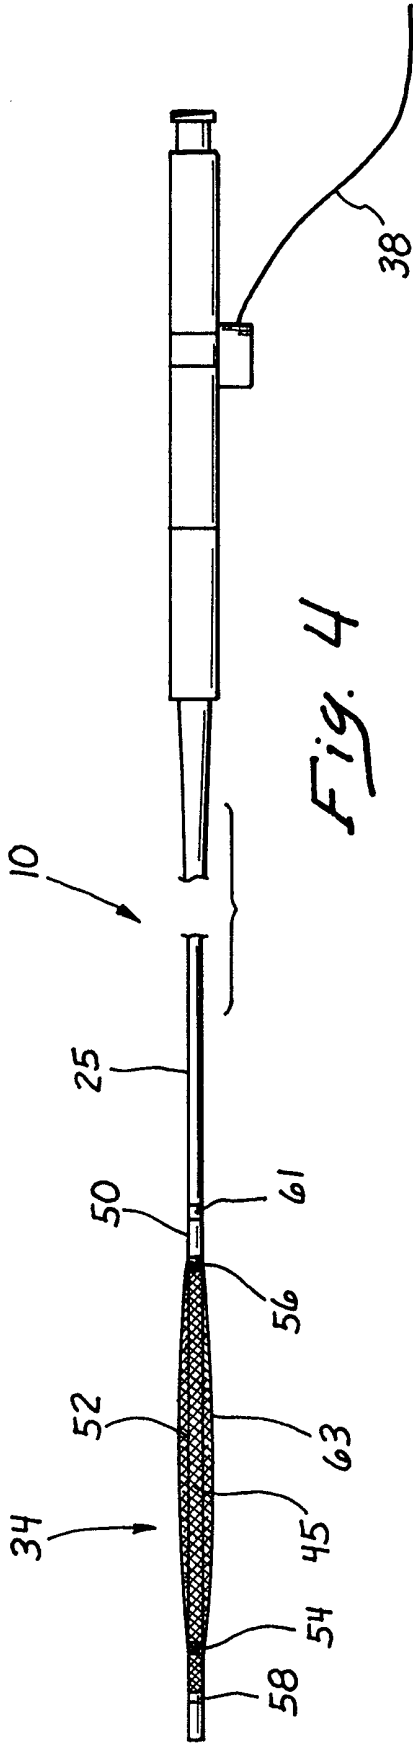


Fig. 4



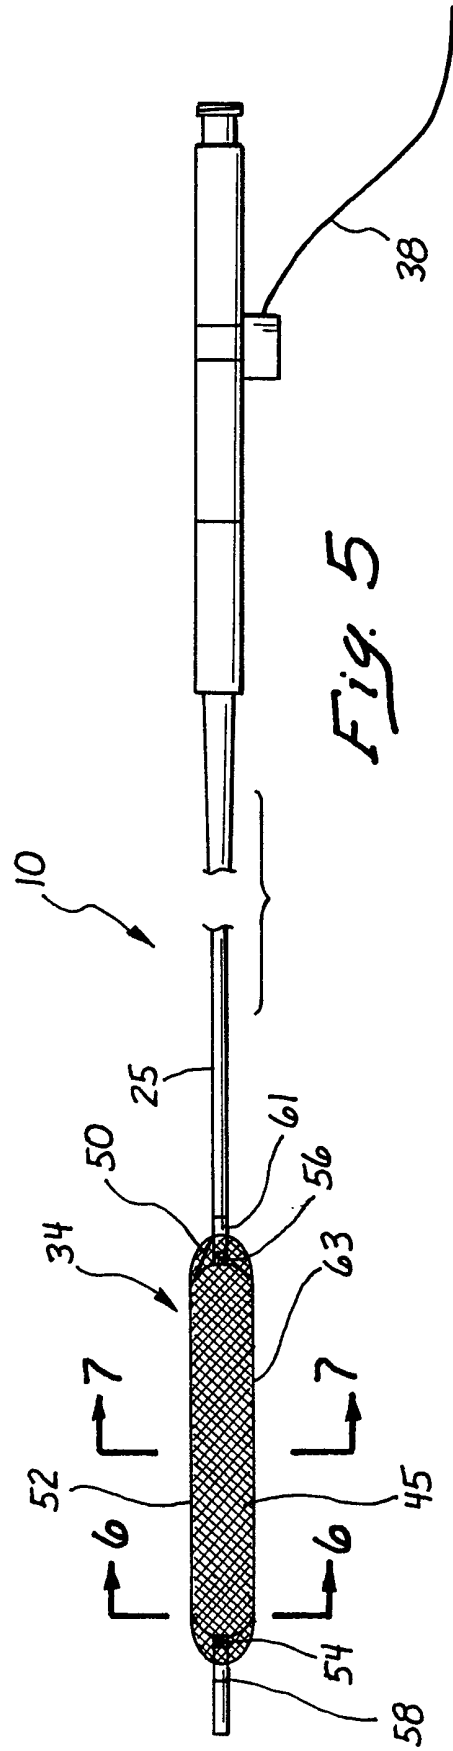


Fig. 5




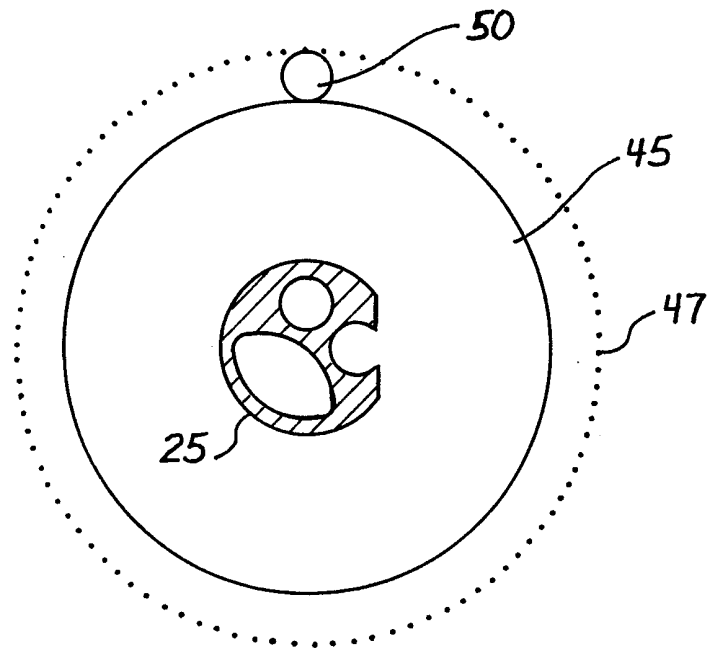

*Fig. 6*

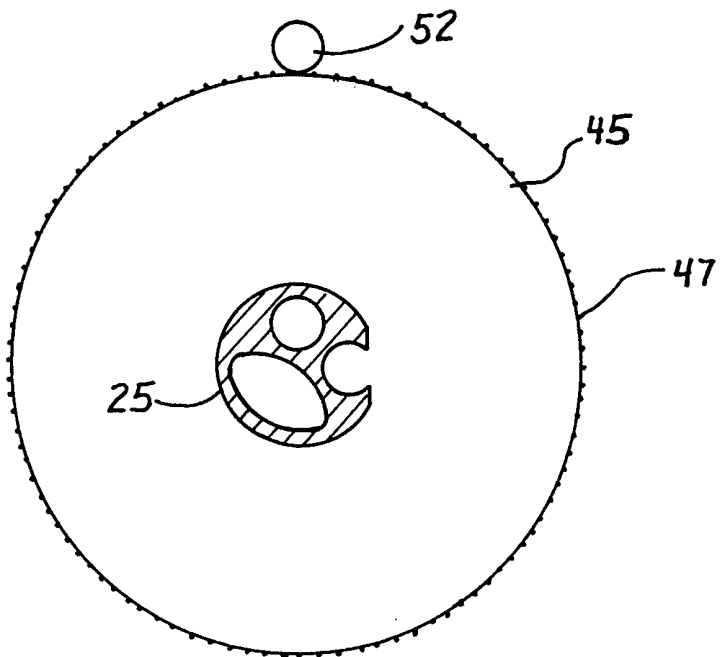


*Fig. 7*




*Fig. 8*




*Fig. 9*

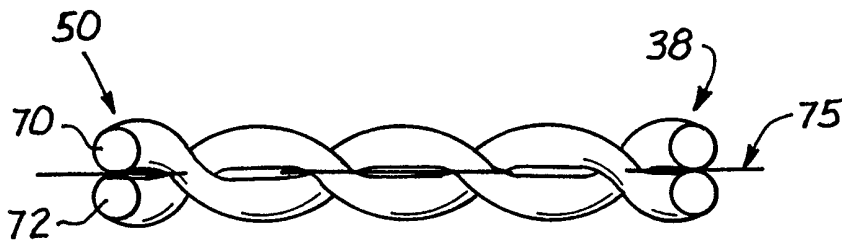




*Fig. 10*

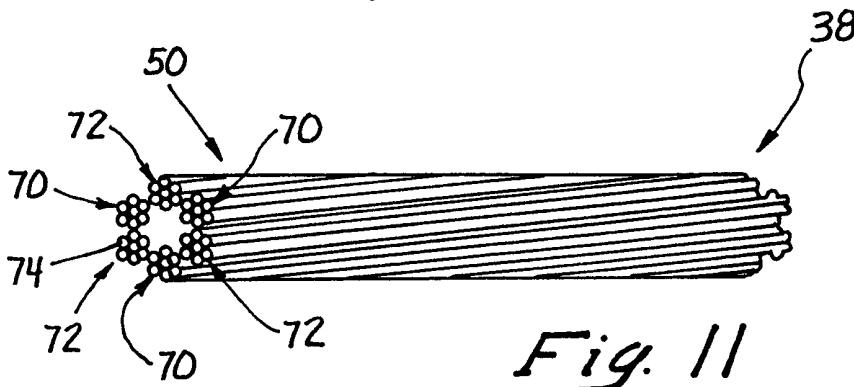


*Fig. 11*

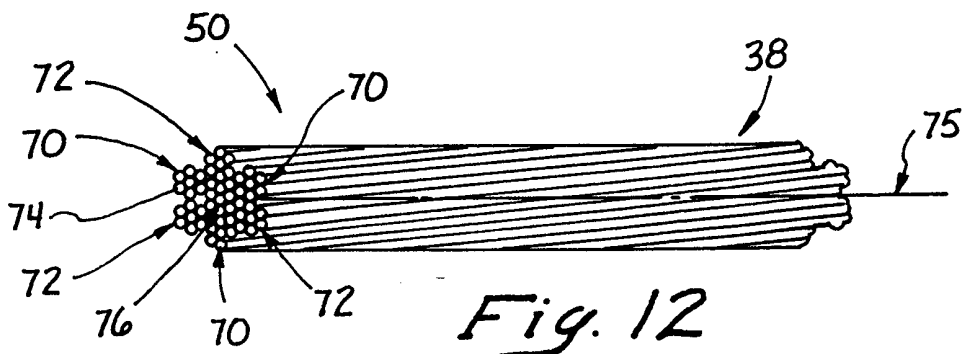


*Fig. 12*

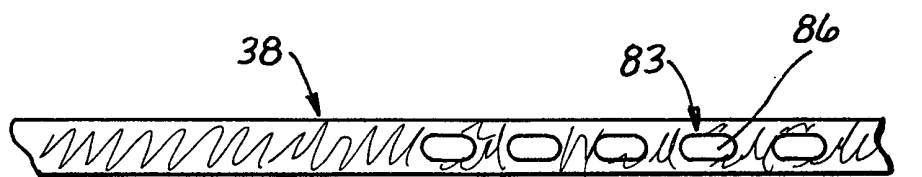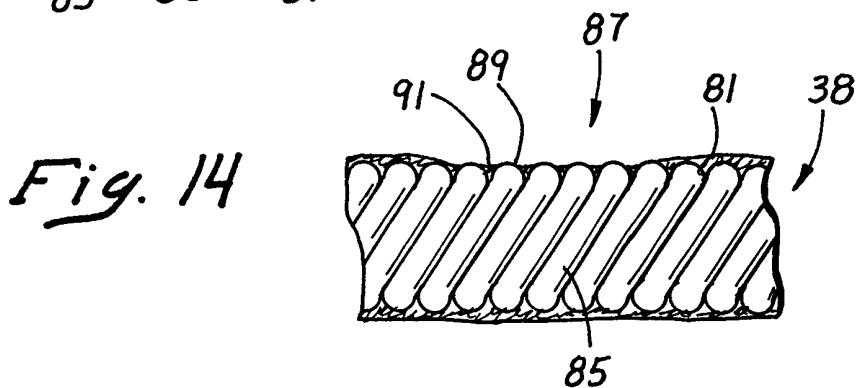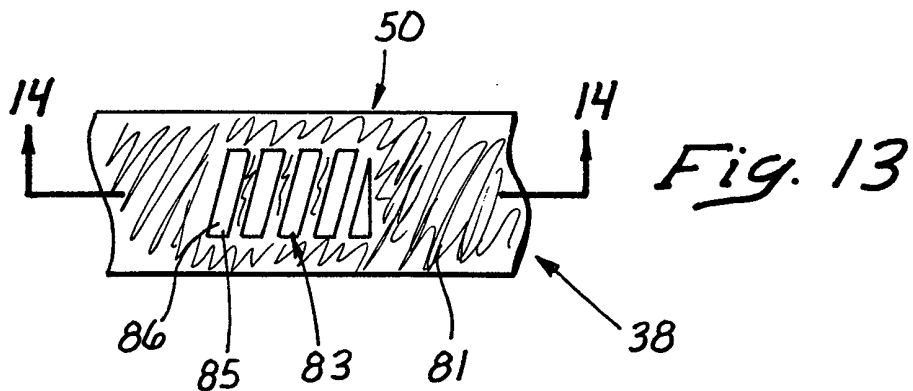


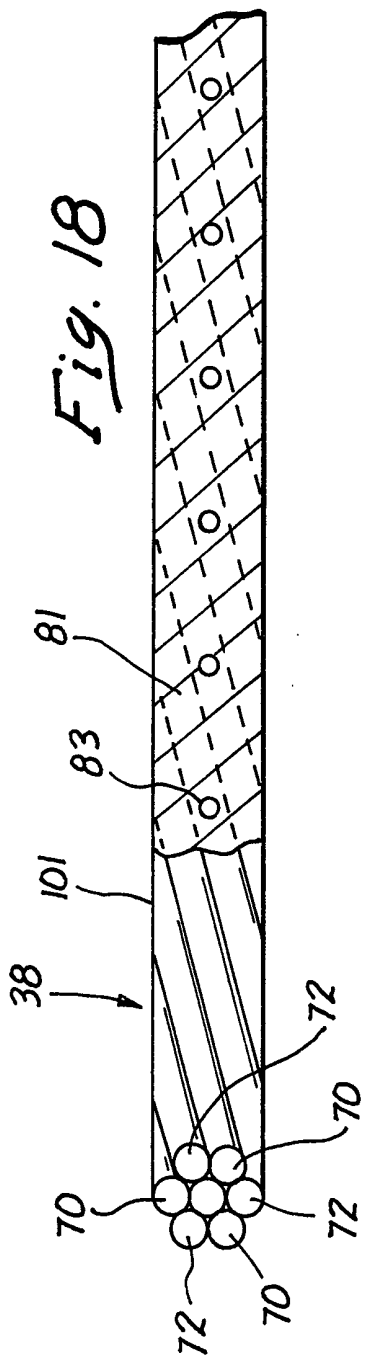


*Fig. 18*

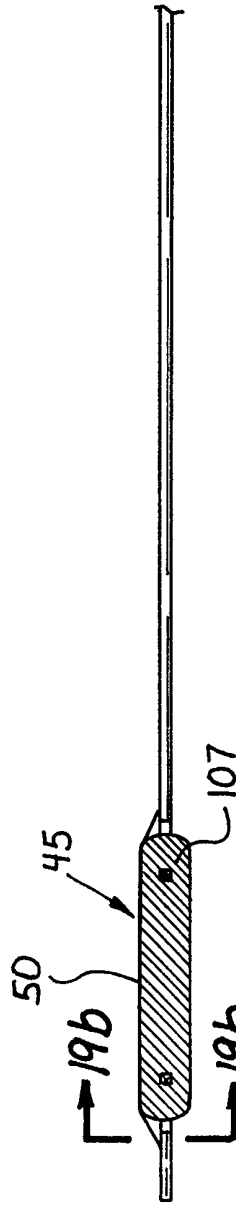

*Fig. 19a*




*Fig. 19b*

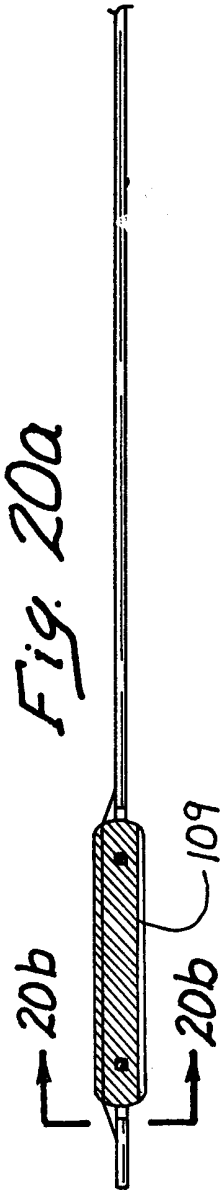


*Fig. 20a*

*Fig. 20b*




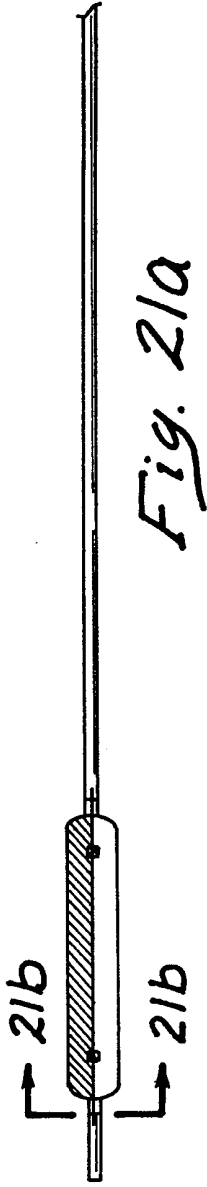

*Fig. 21a*

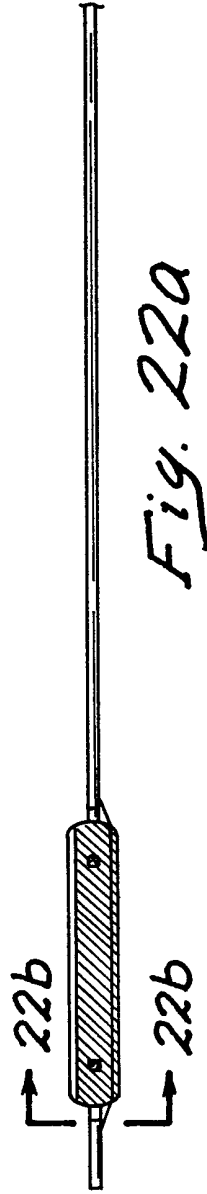

*Fig. 22a*

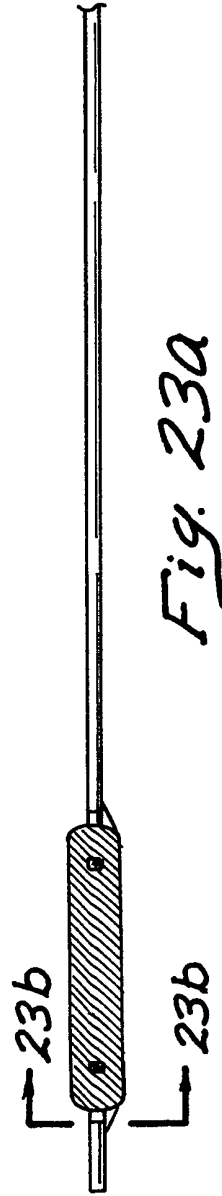

*Fig. 23a*




*Fig. 21b*




*Fig. 22b*




*Fig. 23b*

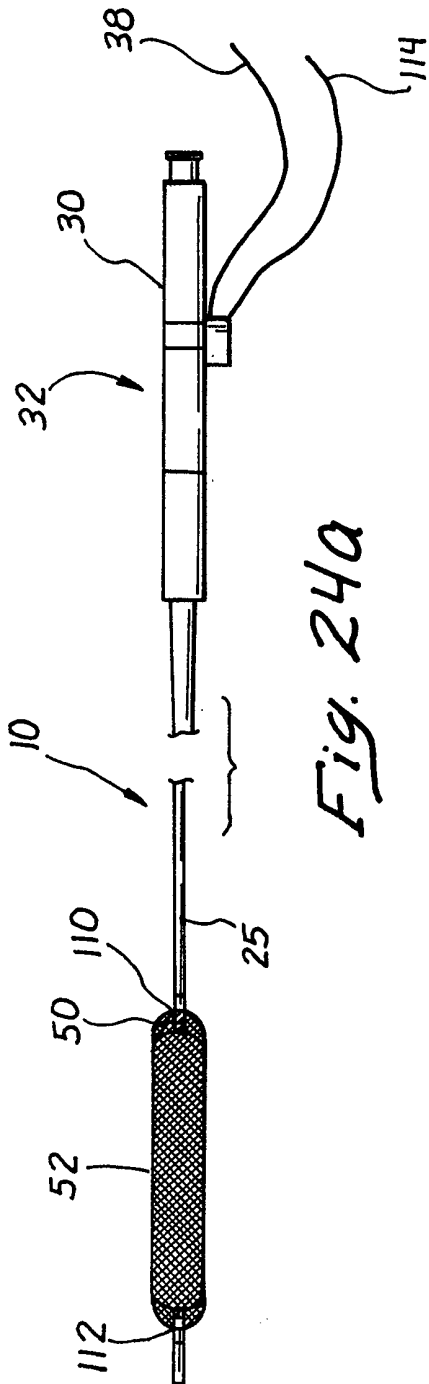


*Fig. 24a*

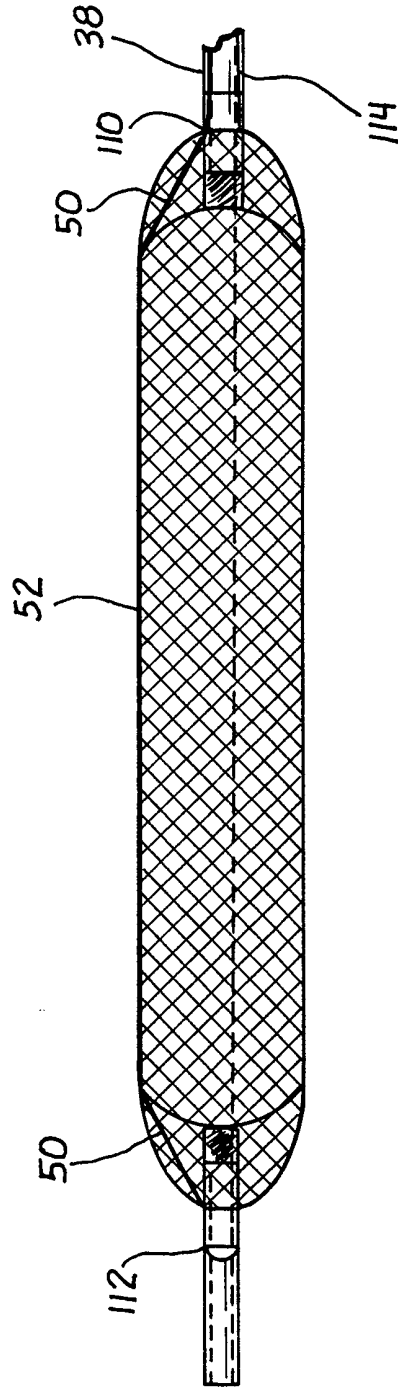

*Fig. 24b*

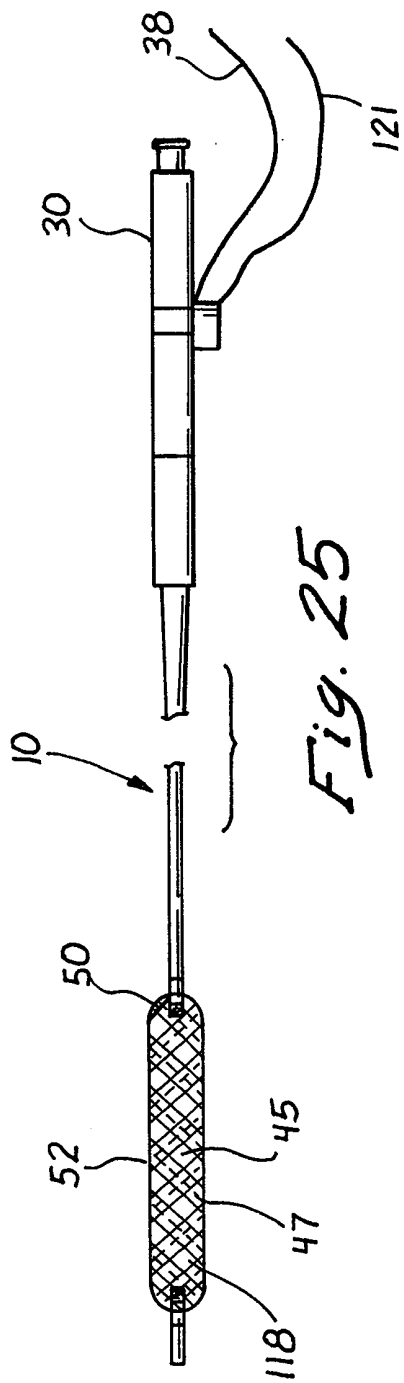

*Fig. 25*

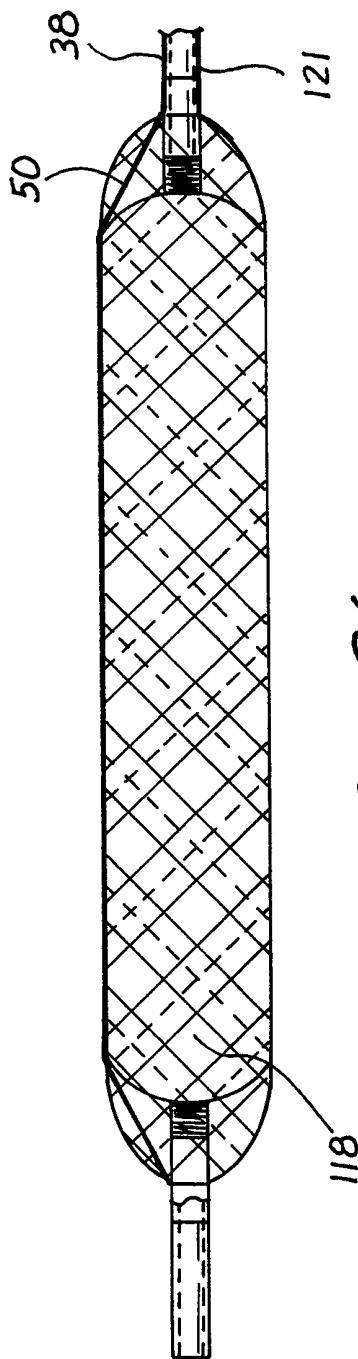

*Fig. 26*

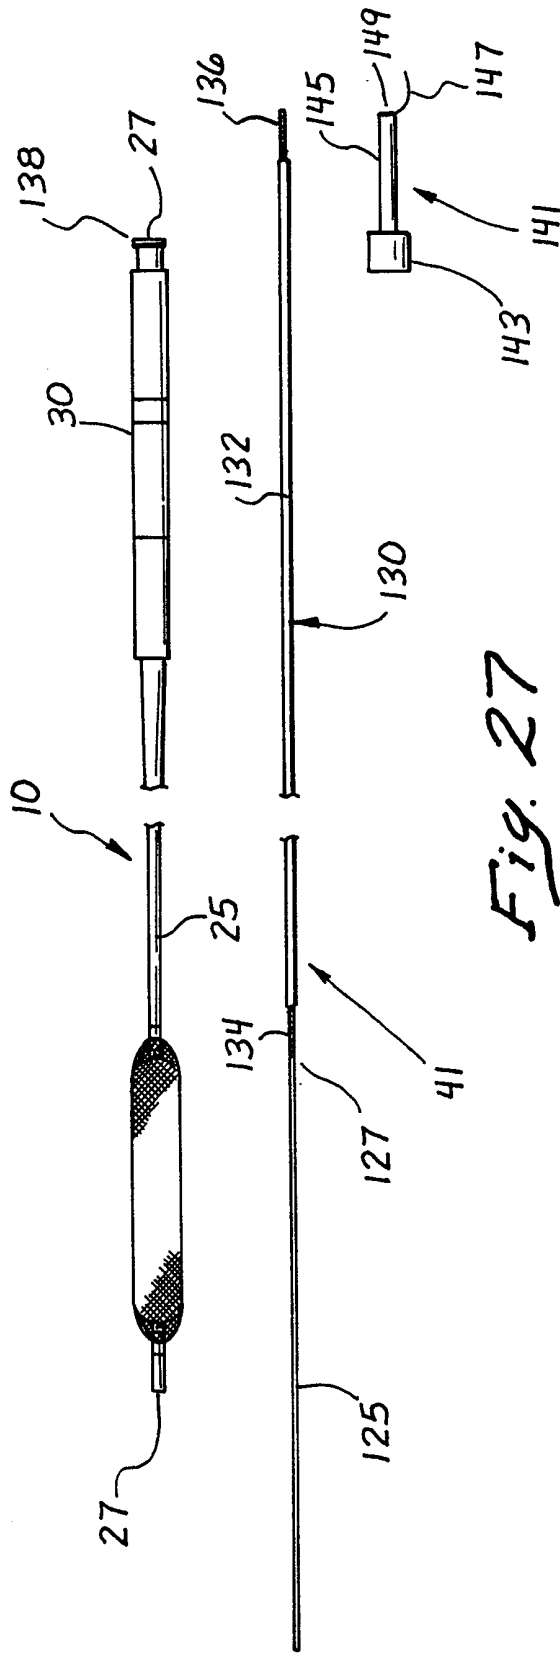


Fig. 27




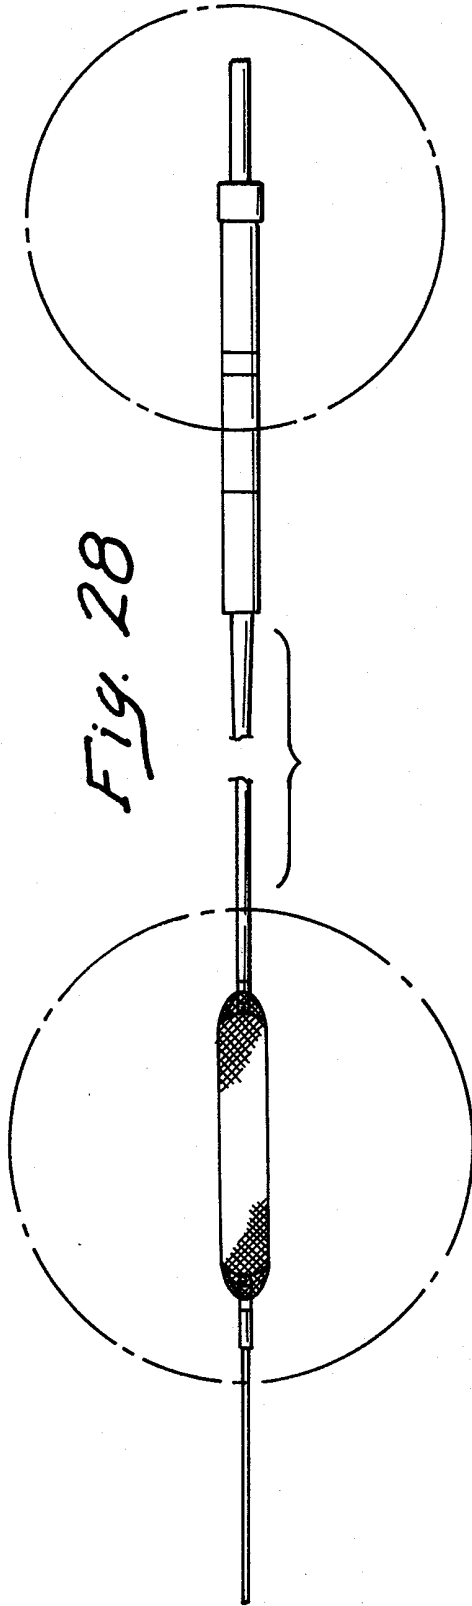


Fig. 29

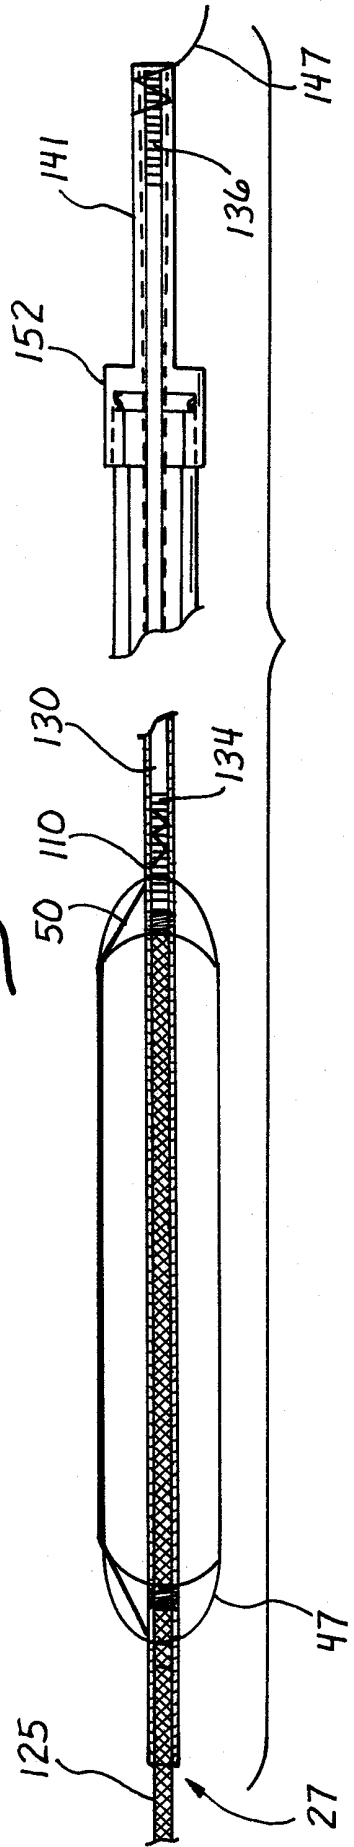

INTERNATIONAL SEARCH REPORT

International application No.  
PCT/US98/27876

**A. CLASSIFICATION OF SUBJECT MATTER**  
 IPC(6) :A61B 17/39  
 US CL :600/585; 606/41, 45, 49; 607/99  
 According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**  
 Minimum documentation searched (classification system followed by classification symbols)  
 U.S. : 600/585; 606/41, 45, 49; 607/99

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 5,682,885 A (LITTMANN et al) 04 November 1997, col. 7 lines 5-58.	26-34
X ---P Y	US 5,779,698 A (CLAYMAN et al) 14 July 1998, entire document.	19, 20, 25 ----- 11-18, 21-24
Y,P	US 5,846,238 A (JACKSON et al) 08 December 1998, col. 10 lines 40-56.	11-18, 21-24
X --- A	DE 35 16830 A (HUBMANN et al) 13 November 1986, entire document.	19, 20, 25 ----- 1-10

Further documents are listed in the continuation of Box C.  See patent family annex.

* Special categories of cited documents:	"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A" document defining the general state of the art which is not considered to be of particular relevance	"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"E" earlier document published on or after the international filing date	"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	"&" document member of the same patent family
"O" document referring to an oral disclosure, use, exhibition or other means	
"P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search 24 FEBRUARY 1999	Date of mailing of the international search report <b>30 MAR 1999</b>
---	--

Name and mailing address of the ISA/US Commissioner of Patents and Trademarks Box PCT Washington, D.C. 20231 Facsimile No. (703) 305-3230	Authorized officer <i>Lee S. Cohen</i> LEE S. COHEN Telephone No. (703) 308-2998
---	---