

US00D708759S

(12) **United States Design Patent**
Heyman et al.

(10) **Patent No.:** **US D708,759 S**
(45) **Date of Patent:** **** Jul. 8, 2014**

(54) **RETINOPATHY INSTRUMENT TRAY**
(71) Applicants: **Arnold M. Heyman**, Los Angeles, CA
(US); **Adam F. Weston**, Woodland Hills,
CA (US)
(72) Inventors: **Arnold M. Heyman**, Los Angeles, CA
(US); **Adam F. Weston**, Woodland Hills,
CA (US)

D565,743 S * 4/2008 Phillips et al. D24/229
D571,478 S * 6/2008 Horacek D24/217
D596,311 S * 7/2009 Antons D24/227
D608,015 S * 1/2010 Sandel D24/227
D608,456 S * 1/2010 Sandel D24/227
D618,821 S * 6/2010 Larsen D24/227
D631,558 S * 1/2011 Harmston et al. D24/229
D646,796 S * 10/2011 Walter D24/227
D647,628 S * 10/2011 Helfteren D24/229
D650,912 S * 12/2011 Tomes et al. D24/227
D662,218 S * 6/2012 Pittman D24/227

(73) Assignee: **Neotech Products, Inc.**, Valencia, CA
(US)

* cited by examiner

(**) Term: **14 Years**

Primary Examiner — T. Chase Nelson

Assistant Examiner — Mark Cavanna

(21) Appl. No.: **29/463,205**

(74) *Attorney, Agent, or Firm* — William W. Haefliger

(22) Filed: **Oct. 29, 2013**

(57) **CLAIM**

The ornamental design for a retinopathy instrument tray, as shown and described.

(51) **LOC (10) Cl.** **24-01**

(52) **U.S. Cl.**
USPC **D24/229**

DESCRIPTION

(58) **Field of Classification Search**
USPC D24/185, 216–232, 127–128;
D3/203.1–203.8, 304;
D6/406.1–406.3, 406.6; D9/341, 345,
D9/347, 348, 415, 418, 419, 430, 732;
422/58, 99, 102, 104, 297, 400,
422/560–564, 509, 942; 206/461–471, 526,
206/528, 531, 534–539; 211/85.13, 126.14,
211/174

FIG. 1 is a frontal elevation view showing the retinopathy instrument tray;
FIG. 2 is a right side elevation view of the FIG. 1 retinopathy instrument tray, the left side elevation being the same;
FIG. 3 is a lower edge elevation view of the FIG. 1 retinopathy instrument tray, the top edge elevation being the same;
FIG. 4 is a rear elevation view of the FIG. 1 tray;
FIG. 5 is a section view taken on lines 5-5 of FIG. 1;
FIG. 6 is a section view taken on lines 6-6 of FIG. 1;
FIG. 7 is a section view taken on lines 7-7 of FIG. 1;
FIG. 8 is a section view taken on lines 8-8 of FIG. 1;
FIG. 9 is a section view taken on lines 9-9 of FIG. 1;
FIG. 10 is a section view taken on lines 10-10 of FIG. 1; and,
FIG. 11 is a section view taken on lines 11-11 of FIG. 1.

See application file for complete search history.

The broken lines are included for the purpose of illustrating portions of the retinopathy instrument tray that form no part of the claimed design.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D334,973 S * 4/1993 Valentine et al. D24/227
D337,830 S * 7/1993 Coyne et al. D24/229
D387,177 S * 12/1997 Davis D24/227
D402,767 S * 12/1998 Davis et al. D24/229
D438,634 S * 3/2001 Merry D24/227
D442,697 S * 5/2001 Hajianpour D24/229

1 Claim, 3 Drawing Sheets


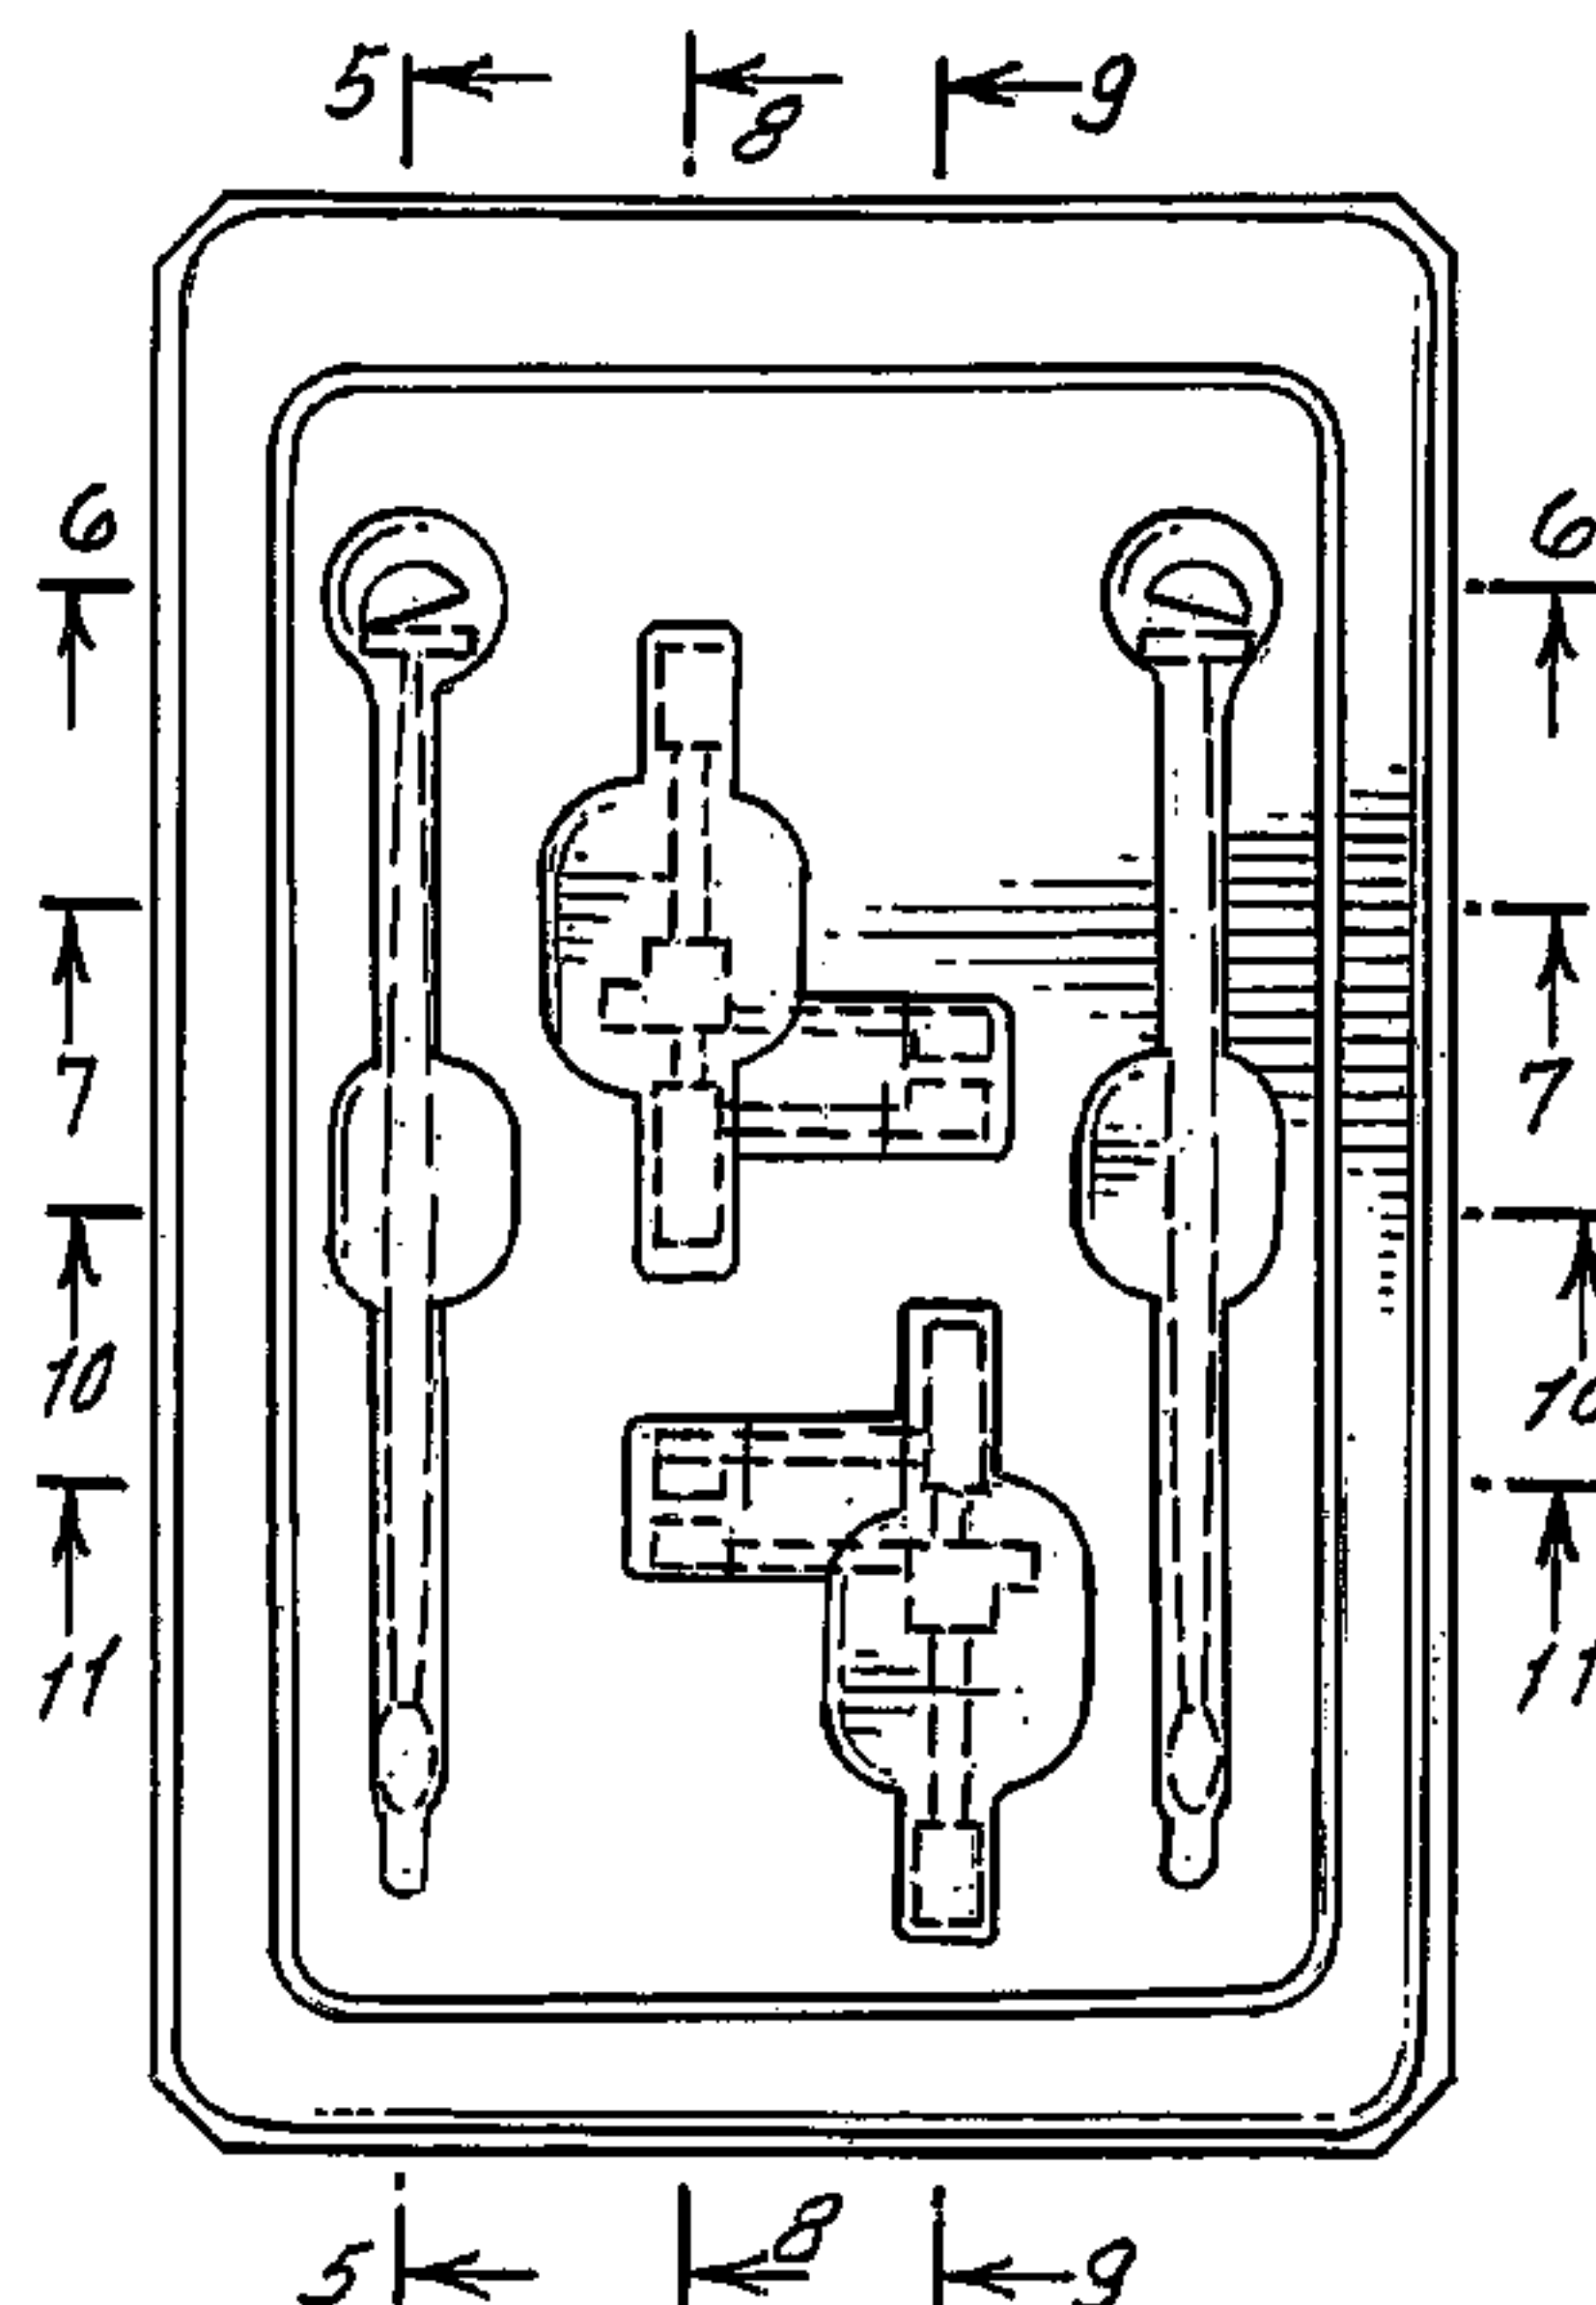


FIG. 1

5 ← 8 ← 9

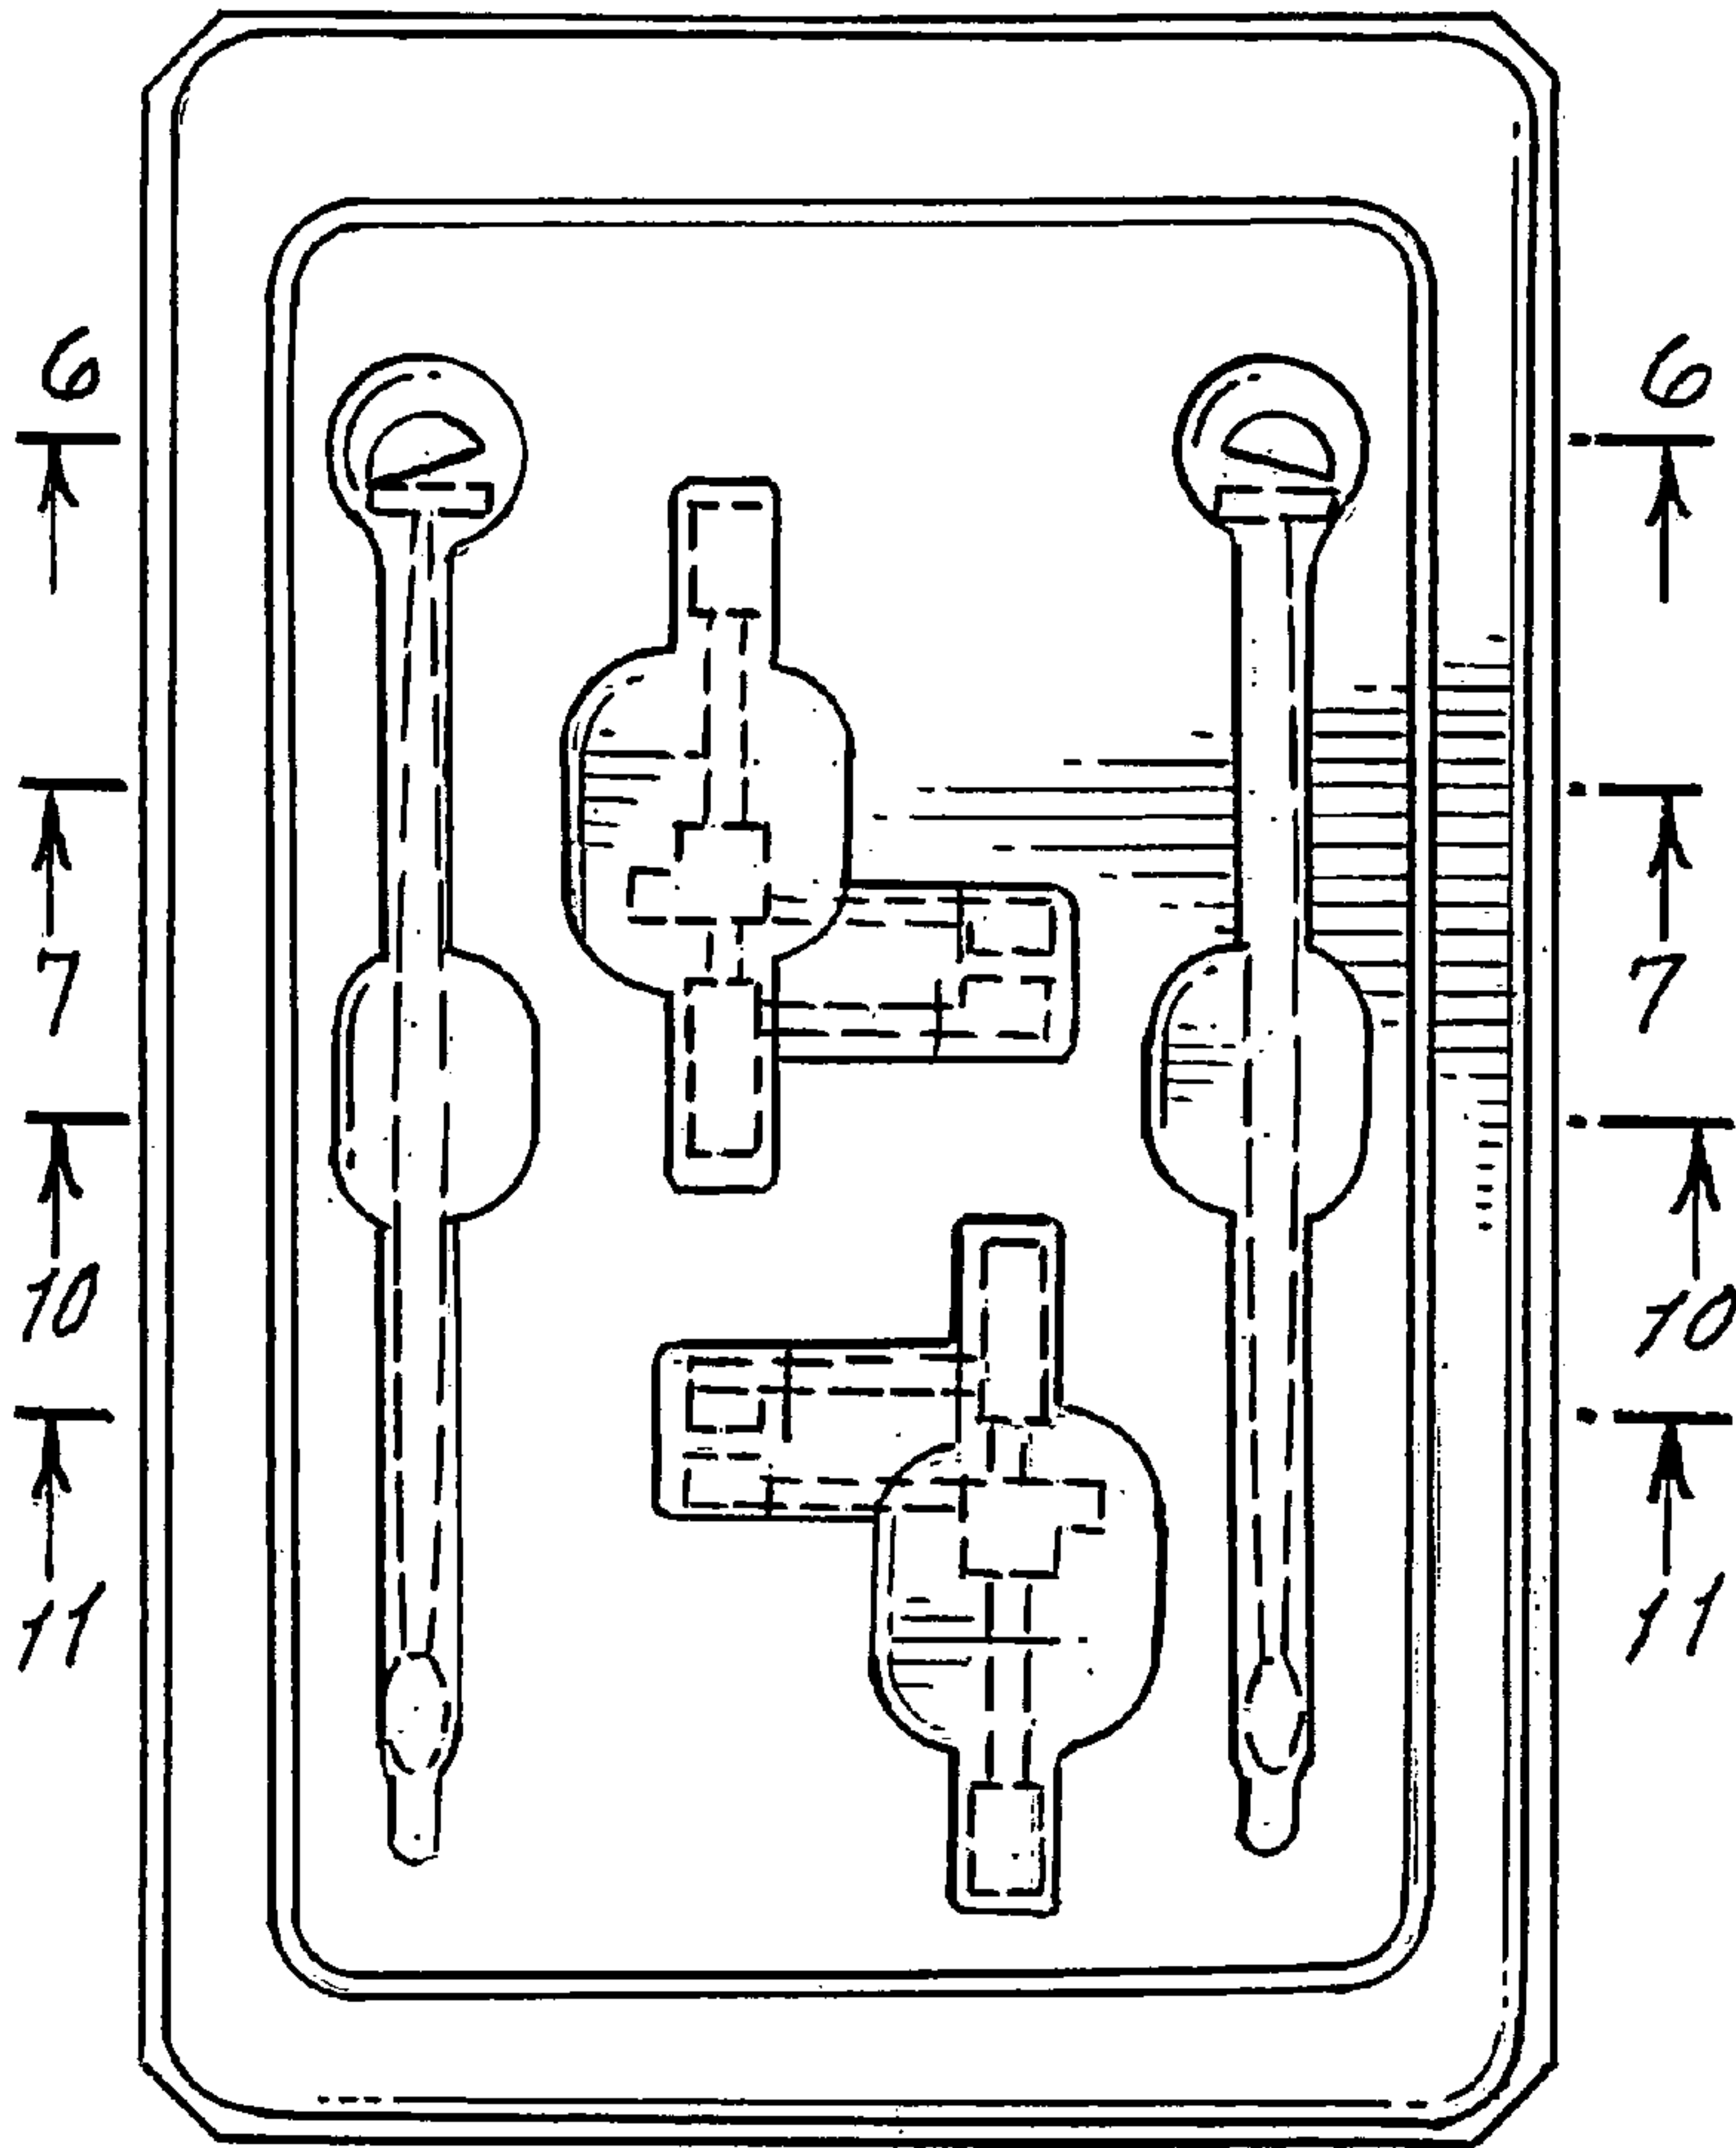

5 ← 8 ← 9

FIG. 2

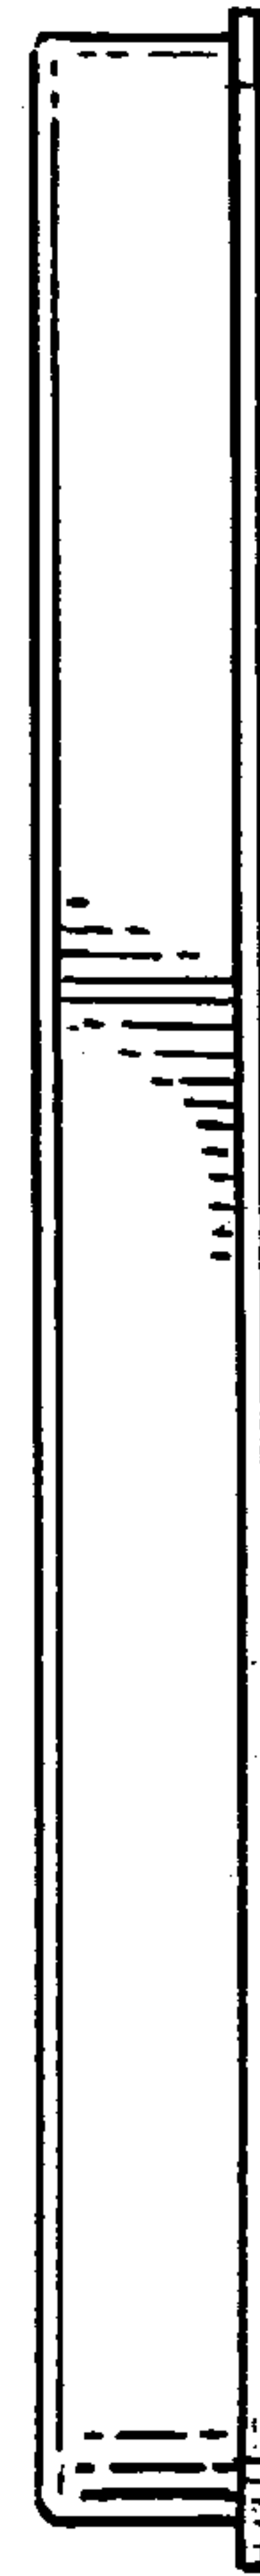


FIG. 3



FIG. 4

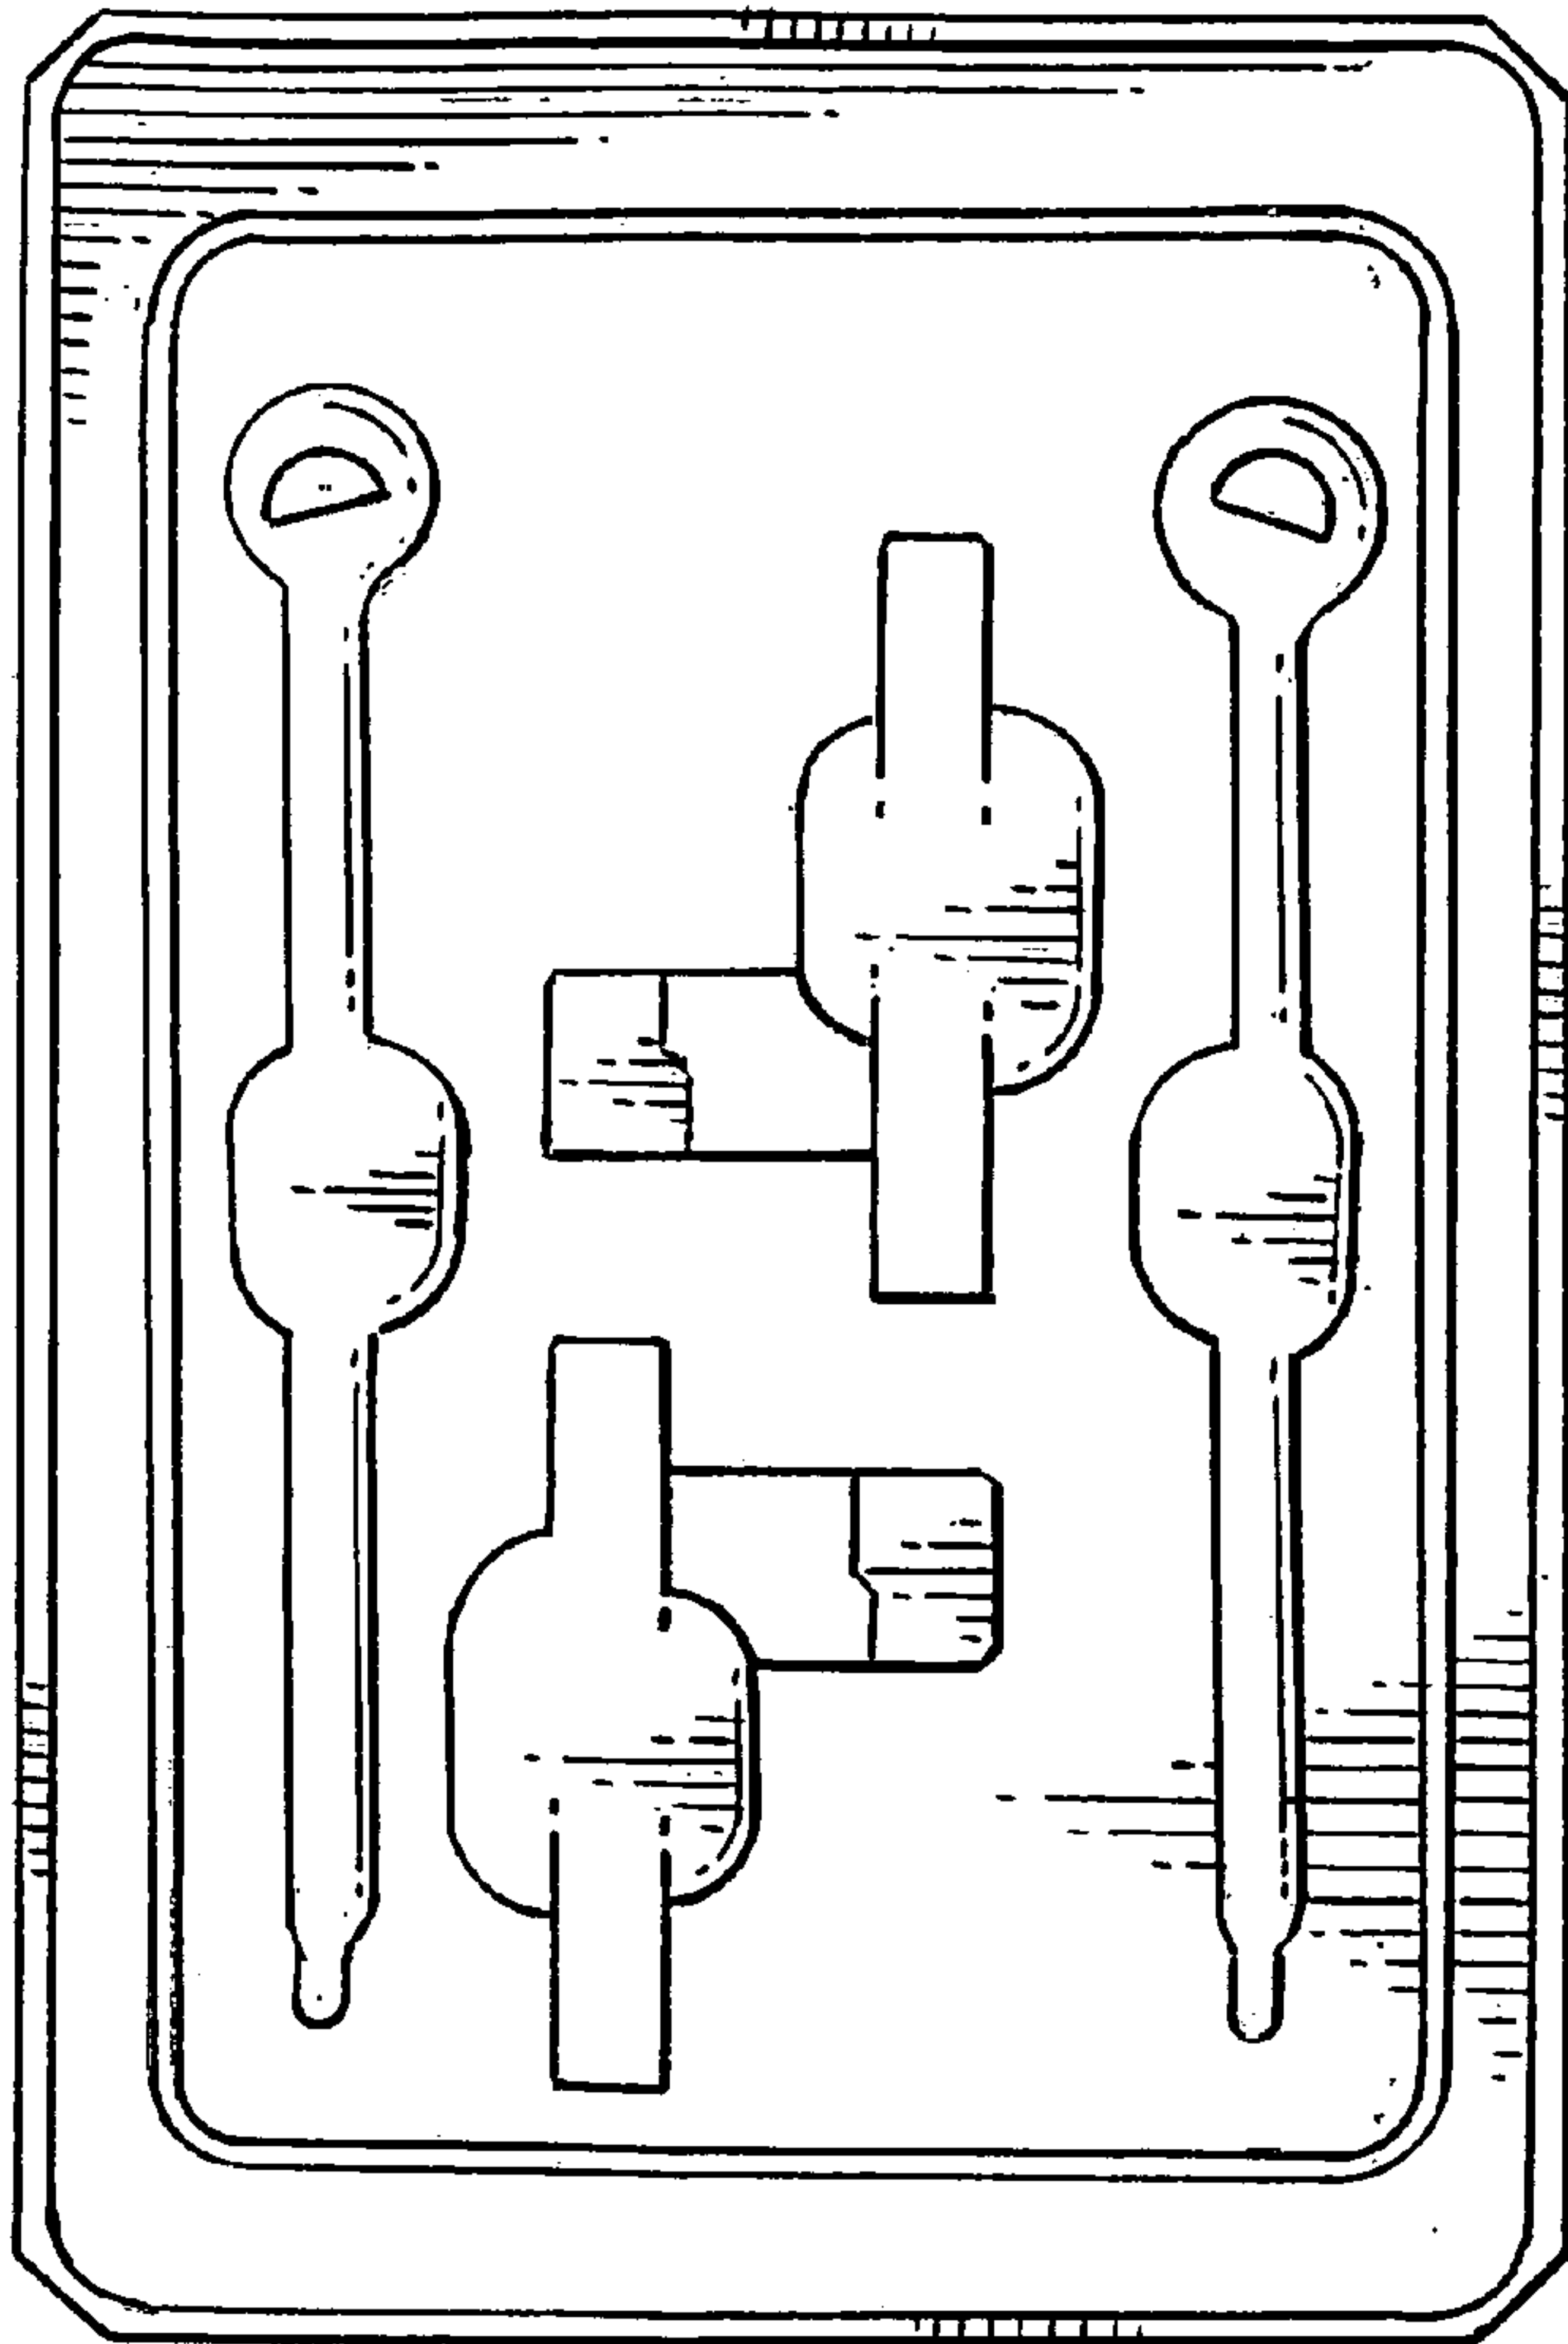


FIG. 5

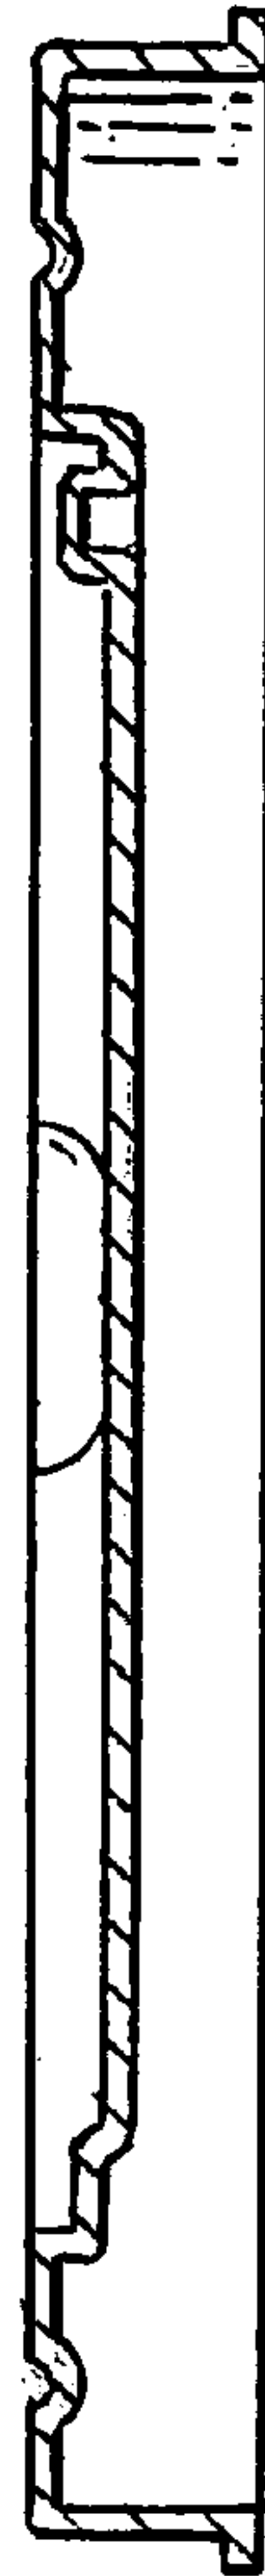


FIG. 6

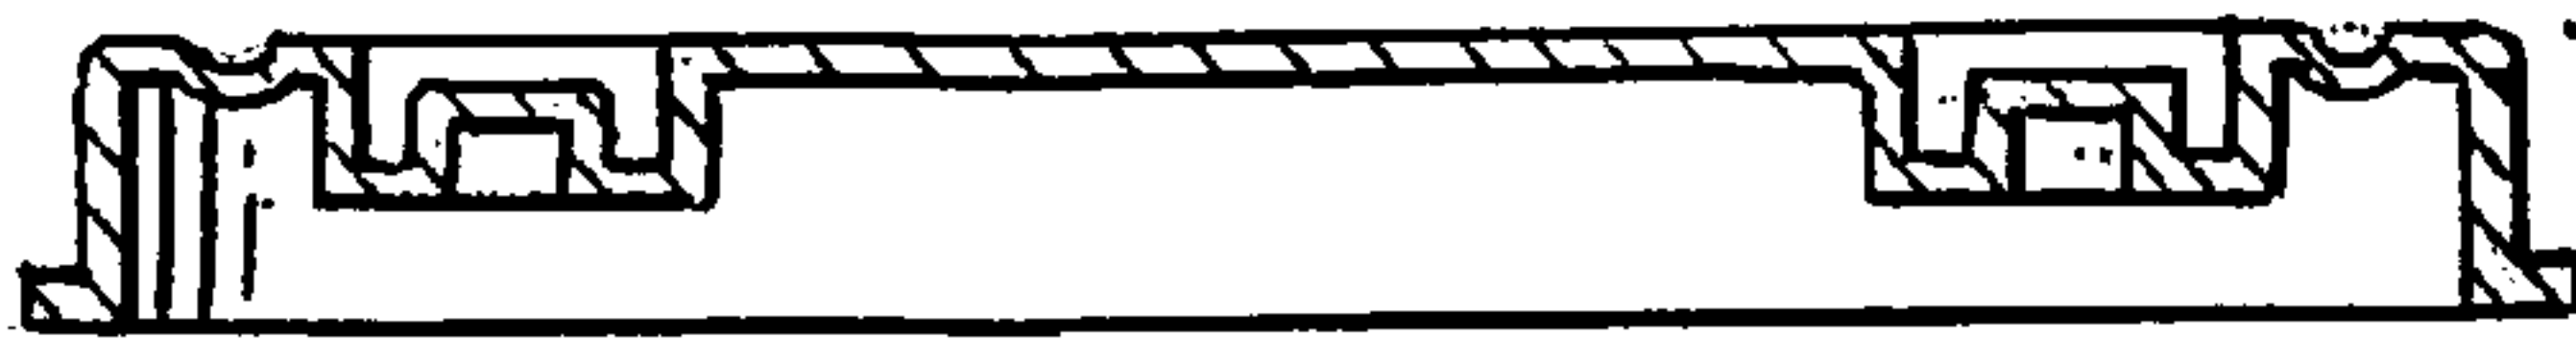


FIG. 7



FIG. 8

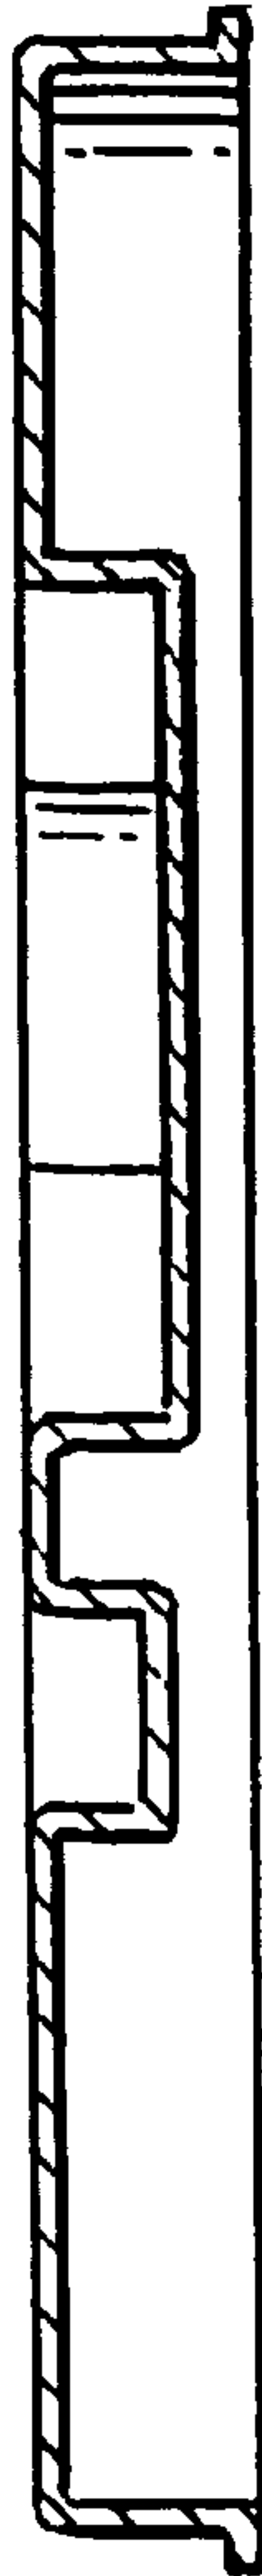


FIG. 9

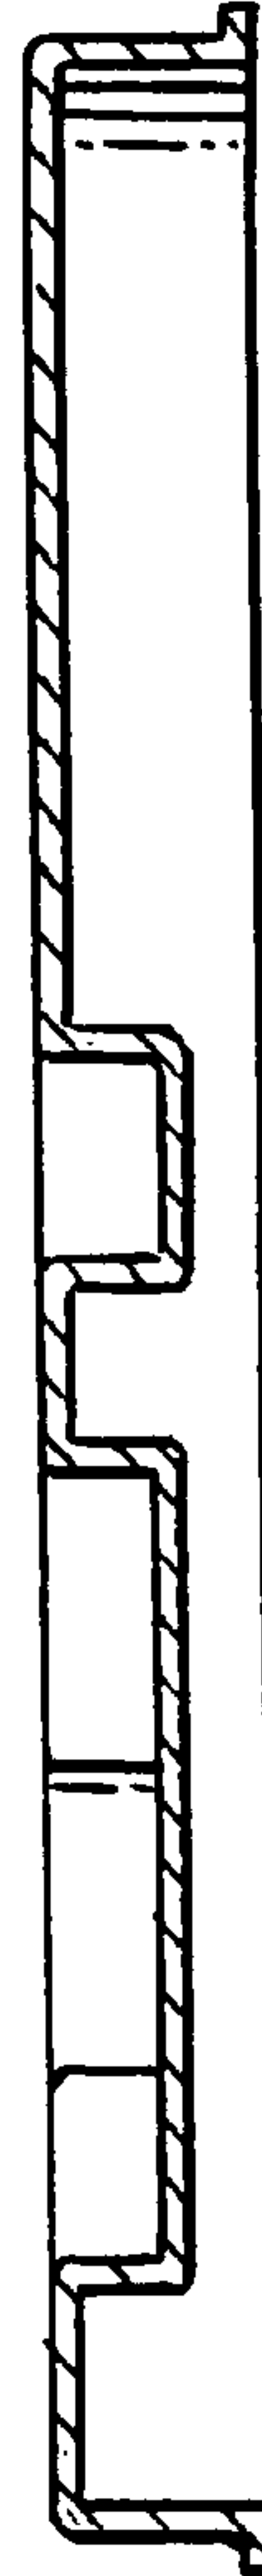


FIG. 10

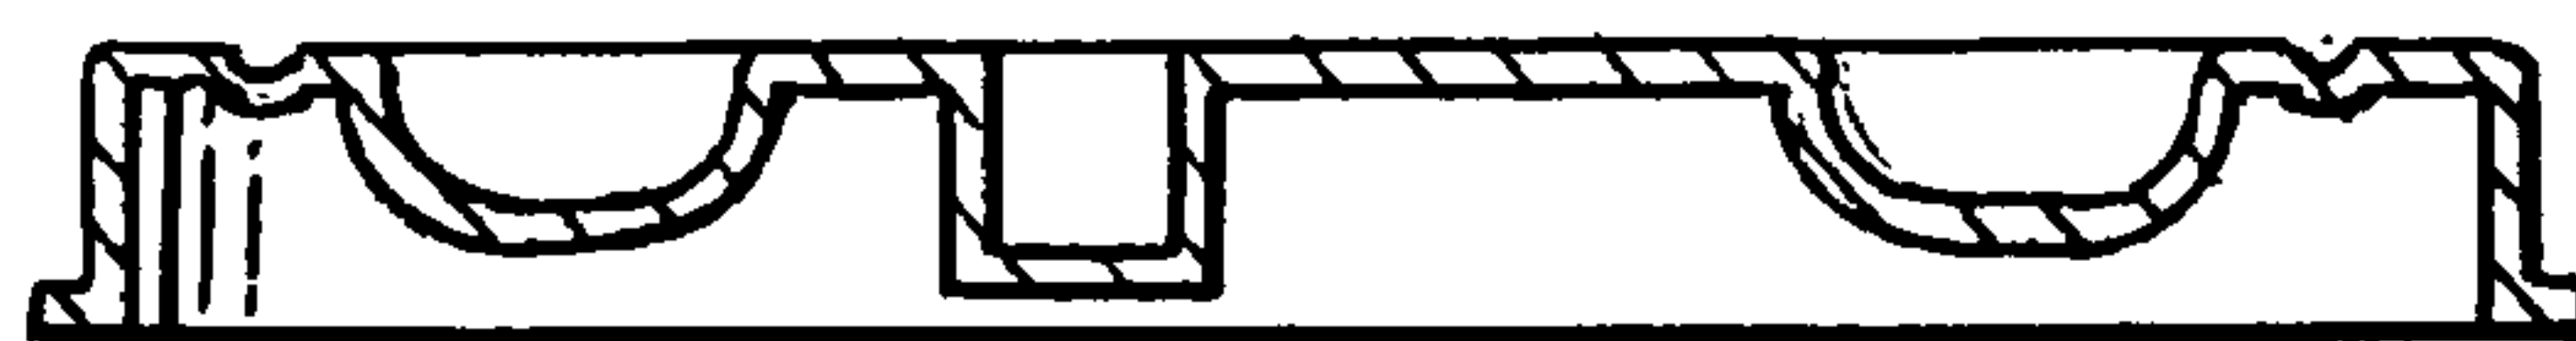


FIG. 11

