



- (51) **International Patent Classification:**  
A61B 19/00 (2006.01)
- (21) **International Application Number:**  
PCT/EP2010/059245
- (22) **International Filing Date:**  
30 June 2010 (30.06.2010)
- (25) **Filing Language:** English
- (26) **Publication Language:** English
- (71) **Applicant (for all designated States except US):** Brain-LAB AG [DE/DE]; Kapellenstr. 12, 85622 Feldkirchen (DE).
- (72) **Inventors; and**
- (75) **Inventors/ Applicants (for US only):** VOLLMER, Fritz [DE/DE]; Reifenstuelstr. 5, 80469 Munich (DE). HOEVEER, Manuel [DE/DE]; Feldbergstr. 40, 81125 Munich (DE).
- (74) **Agent:** SCHWABE-SAND MAIR-MARX; Stuntzstr. 16, 81677 Munich (DE).
- (81) **Designated States (unless otherwise indicated, for every kind of national protection available):** AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BR, BW, BY, BZ,

CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IS, JP, KE, KG, KM, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PE, PG, PH, PL, PT, RO, RS, RU, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.

- (84) **Designated States (unless otherwise indicated, for every kind of regional protection available):** ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

**Declarations under Rule 4.17:**

— of inventorship (Rule 4.17(iv))

**Published:**

— with international search report (Art. 21(3))

- (54) **Title:** MEDICAL IMAGE REGISTRATION USING A RIGID INNER BODY SURFACE

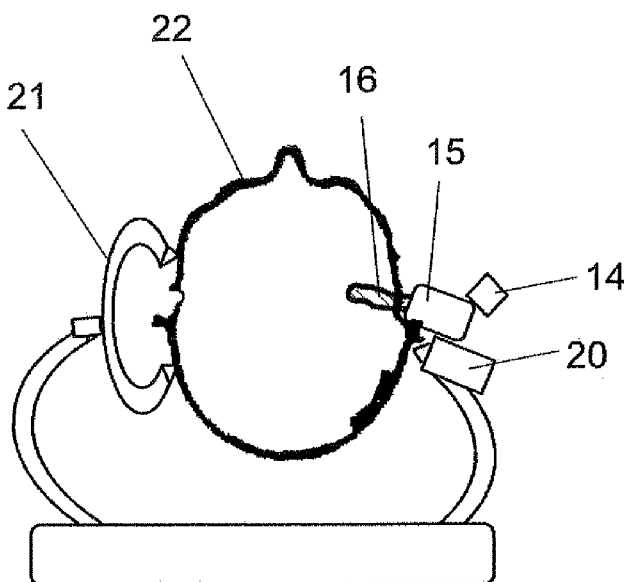


Figure 2

(57) **Abstract:** The invention relates to a medical image registration method in which an actual patient's body or portion of a patient's body (22) is positionally registered to a patient image created using a medical body-imaging technique such as MR, CT or x-ray imaging, wherein in a medical navigation system, the actual spatial position of at least a part of the body or body portion (22) is assigned to a respective position in the image of said body or body portion (22), wherein the part of the body or body portion (22) comprises a registration area in the form of the surface of a substantially rigid body structure, in particular an inner structure, made of bone or cartilage. The invention also relates to a medical image registration device which comprises a surface scanner (15) for scanning a registration area comprising the surface of a substantially rigid body structure, in particular an inner structure, made of bone or cartilage.



## **MEDICAL IMAGE REGISTRATION USING A RIGID INNER BODY SURFACE**

The present invention relates to a medical image registration method and device. In medical image registration, an actual patient's body or portion of a patient's body is positionally registered to a patient image created using a medical body-imaging technique such as for example MR, CT or x-ray imaging. In most cases, a medical navigation system is used to assign the actual spatial position of at least a part of the body or body portion to a respective position in the image of said body or body portion.

in accordance with the prior art, registration devices are imaged together with the body or body portion, and the images of said registration devices are then used to register the patient to the image of the patient by assigning the images to their actual spatial positions or equivalents. Once such registration method is for example described in DE 196 39 615 A1.

A registration device which is embodied as a dental-based stereotactic localiser is known from US 2004/0015176 A1, and a surgical face mask which is used as a registration device is disclosed in US 2003/0131852 A1.

While registration on the basis of body landmarks (eye canthus, nasion) alone is error-prone when used on its own (due for example to skin movement), registration methods using the registration devices described above are often complicated because the devices have to be fixed on the patient during the imaging step and it is necessary to ensure that they are situated at the same location during the actual registration step. This necessitates either invasive procedures or at least an uncomfortable rigid fixation. Such registration devices are also difficult to keep sterilised, expensive and in many cases difficult to handle.

It is the object of the present invention to provide an image registration method and device which overcome the disadvantages of the prior art. In particular, the intention is to provide an easy-to-use registration method and device which nonetheless still offer optimum registration accuracy. This object is achieved by a medical image registration method in accordance with claim 1 and a medical image registration device in accordance with claim 10. The sub-claims define advantageous embodiments of the invention.

In accordance with the method of the present invention, the part of the body or body portion (which is used for registration) comprises a registration area in the form of the surface of a substantially rigid body structure, in particular an inner structure, made of bone or cartilage. In other words, the present invention moves from using a device fixed on the body or body portion to using a specific part of said body or body portion, namely a part which - as recognised by the invention - is particularly qualified or suitable for this purpose. Registration devices in accordance with the prior art generate reproducible registration points or areas, whereas the present invention has recognised that such reproducible points or areas, i.e. uniquely recognisable registration points or areas, are in fact already provided by certain locations of the body or body portion itself, namely body surfaces or surface areas which have a substantially rigid body structure, in particular an inner structure, made of bone or cartilage. Using currently available surface scanning equipment, such body structures or areas can be imaged to a sufficient level of accuracy that they can be used as registration areas. On the basis of this, the present invention can render the use of separate registration devices unnecessary in many applications. All of the difficulties in handling and problems with inaccuracy associated with the use of such devices can therefore be solved by employing the method of the present invention.

The present invention also enables medical personnel to carry out automatic patient registration, in particular cranial registration, without the need for any additional registration scan, providing the rigid registration area is contained in an image data set which is already available. This is often the case, since such image data sets

have usually already been created for diagnostic purposes and are thus available for further use.

Registration in accordance with the present invention will work particularly well with CT and MR imaging methods, thus providing fast and repeatable registration, even during an operation.

In general, the registration area can comprise any sufficiently rigid inner or outer body structure surface, in particular the surface of one or more of the following body structures:

- the meatus or ear channel, or at least a part of the meatus, in particular the outer meatus;
- the palate, in particular the bony or hard palate;
- the upper inner jaw area and/or lower inner jaw area;
- the inner nose cartilage structure.

The registration area or surface can be covered by skin, membrane or mucosa but still able to be determined in terms of its shape.

Such registration areas can in particular be used within the context of cranial patient registration, i.e. within the context of operations involving a patient's head, since most of the bone and/or cartilage structures of the head and the upper jaw are always in a fixed positional relationship with respect to each other. Inner body structures are particularly useful, because they are in most cases not covered by skin, which shifts easily, and thus retain their outer form under normal circumstances.

In one embodiment of the invention, the registration area on the actual patient's body or portion of the patient's body is measured by means of a surface scanner which in particular comprises a scanner probe which can be positionally located and/or tracked. The position and orientation of the probe can then be established by a tracking system which determines the actual spatial position of at least a part of the

body or body portion. The tracking system can be a medical tracking system, such as a camera tracking system or a magnetic tracking system or the like. It can of course be used in association with the medical navigation system, in order to provide the latter with actual 3D position data.

A surface scanner as mentioned above can also comprise a surface data recording and/or processing unit which creates a positionally determined surface model of the registration area.

The method of the present invention can be performed in such a way that the registration area is measured by means of spaced interferometric measurements, in particular using a thin film interference scanner.

The method according to the present invention can also be supplemented by manually acquiring at least one additional registration landmark on the actual patient's body or body portion and including it in the assignment process by assigning it to a respective position in the image. This can serve to confirm the registration result, in particular the common angular orientation of the actual registration area and the registration area in the image.

In an alternative or additional embodiment, at least one additional registration point or landmark on a frame which is placed on the actual patient's body or body portion can be acquired and included in the assignment process by assigning it to a corresponding related position, in particular a calculated position, in the image in order to supplement the registration process or to confirm the registration result, in particular the common angular orientation of the actual registration area and the registration area in the image.

In the latter case, the registration area on the actual patient's body or body part can be measured by means of a positionally determined surface scanner which in particular comprises a scanner probe which is fixedly attached to the frame, wherein the scanner and/or the frame can be positionally located and/or tracked by a tracking

system which determines the actual spatial position of at least a part of the body or body portion.

The medical registration device in accordance with the present invention, which can be used in a registration method as described above, comprises a surface scanner for scanning a registration area comprising the surface of a substantially rigid body structure, in particular an inner structure, made of bone or cartilage. The scanner can be designed as a surface scanner, in particular an inner surface scanner, comprising a scanner probe which can be positionally located and/or tracked and in particular used for inserting into and/or scanning the surface of one or more of the following body structures:

- the meatus or ear channel, or at least a part of the meatus, in particular the outer meatus;
- the palate, in particular the bony or hard palate;
- the upper inner jaw area and/or lower inner jaw area;
- the inner nose cartilage structure.

The scanner can be embodied as an interferometric measurement scanner, in particular a thin film interference scanner.

In particular embodiments of the present invention, the registration device can be fixed to:

- a fixation support for the actual body or body portion; or
- a frame on the actual patient's body or body portion, wherein the frame is positionally acquired and included in the assignment process by assigning it to a corresponding related position, in particular a calculated position, in the image in order to supplement the registration process or to confirm the registration result, in particular the common angular orientation of the actual registration area and the registration area in the image.

The invention also relates to a program which, when it is running on a computer or is loaded onto a computer, causes the computer to perform a method such as has been described above in various embodiments. The invention also relates to a computer program storage medium which comprises such a computer program.

The invention will now be explained in more detail by referring to particular embodiments and to the attached drawings. It is to be noted that each of the features of the present invention as referred to here can be implemented separately or in any expedient combination. In the drawings:

- Figure 1               schematically shows how the surface of an ear channel (meatus) is scanned by means of a scanner probe;
- Figure 2               shows a scanning set-up including a head clamp;
- Figure 3               shows additional landmark points being acquired by means of a pointer; and
- Figures 4 and 5       show a frame being additionally used for registration purposes.

In the embodiments explained below, an automatic cranial patient registration process using special, surface-measuring earplugs will be described, wherein a three-dimensional surface measurement of the ear channel is used to automatically register the patient to a cranial data set, in particular a segmented data set. The embodiments shown are based on accurately measuring the inner surface of the (outer) meatus.

Thin film interference measurements can be used to model the surface of the ear channel, and such methods are for example described in the article "Emission reabsorption laser induced fluorescence (ERLIF) film thickness measurement" by Carlos H. Hidrovo and Douglas P. Hart (in: Measurement Science and Technology 12 (2001), pages 467 to 477). The measurement method discussed in said article can of course utilise the present invention.

As shown in the general depiction of Figure 1, the technique used in accordance with one embodiment of the present invention employs an oil-filled balloon 16 which is inserted through the outer ear 13 into the meatus 12. The balloon is filled with oil in such a way that it completely covers the inner surface of the meatus 12. An interferometric device or probe 17 which is inserted into the oil-filled balloon 16 allows an exact three-dimensional reconstruction of the balloon's shape to be created or acquired and therefore yields a three-dimensional model 18 of the outer meatus which in particular includes information about the relative position of the support 15 and the probe 17 which is fixedly attached to the support 15. In an interferometric measuring method, the probe 17 inside the balloon 16 is made of a solid material which conducts laser light and has a rigid connection to the measuring device support 15 and a reference element 14 attached to the support 15.

Other methods for mapping the three-dimensional surface of the meatus 12 can also be used, for example methods which are used for modelling hearing aids to the individual meatus of a patient.

A software can be used to reconstruct (determine) the inner surface of the meatus 12 in a given data set (for example, a diagnostic CT or MR image data set) of the patient, for example using atlas segmentation methods. Since the inner part of the meatus 12 consists of bony edges 11 and also tissue edges 10 on the outer portion, it should be possible to obtain a good MR and/or CT image. The segmented data set model (or models) and the ear measurement model can be aligned using standard three-dimensional alignment algorithms, thus yielding a transformation matrix between the measuring device and the patient data set co-ordinate system. It is this transformation matrix which serves as the basis for the registration sought.

The measuring interferometric device support 15 can be used together with a tracking or referencing element 14 mounted to it. Tracking the units simultaneously, with the reference element 14 associated with a tracking system (not shown), allows the co-ordinate systems of the patient data and the tracking system to be registered. The measuring device or its support 15 is preferably then mounted rigidly to the



reference element 14 itself. The measuring apparatus is thus rigidly fixed to the patient and the (electromagnetic or optical) reference element 14 which is tracked by a tracking system which is connected to a navigation system. Since at least the fixation or the relative position between the support 15 and the reference element 14 is known by design or calibration, the patient data can be directly referenced to the reference element co-ordinate system.

Figure 2 shows the set-up of Figure 1 when integrated with a head clamp 21, for example a Mayfield head clamp, for cranial operation purposes. The support 15 is fixed to one of the screws 20 of the head clamp 21 which in turn rigidly fixes the head. The reference element 14 (for example, an optical or magnetic tracking device) is fixed to the support 15 and the measuring device which itself has a positionally defined connection to the measuring probe 16 inside the meatus 12. Since the specific position of the measuring device and its components (the support 15 and the probe 16) is known by means of the reference element 14, the measured surface of the meatus 12 can be assigned to a unique position, location and orientation. As mentioned above, aligning said positionally determined shape to the respective shape in the image data of the patient yields a registration transformation matrix.

Measuring and tracking as described above yields the correct and accurate registration which is the aim of the present invention. Registration results can be confirmed or registration can even be supplemented, in particular with regard to the rotational orientation of the inner ear anatomy, using the embodiments of the present invention shown in Figures 3 to 5.

Figure 3 shows how additional landmark points are collected using a magnetically or optically tracked pointer instrument 26. The landmarks are points on the eye canthus or the nasion, and their positions in the patient data set can be calculated using automatic atlas segmentation algorithms. Such algorithms are known as a way of acquiring typical facial landmarks such as the nasion or the canthus of the eyes. The acquired points can then be used in the alignment procedure as additional

constraints when aligning the surface of the three-dimensional model 18 with the measured model of the meatus 12.

Figures 4 and 5 show another way of providing additional orientation data, by attaching a frame 25 to the reference element, i.e. an optical reference element 17 (Figure 4) or an electromagnetic reference element 14 (Figure 5). The frame 25 is constructed in such a way that it rigidly holds the ear measuring apparatus support 15 on one or both sides and additionally has defined points which anatomically fit into the ear 27 or onto the nasion 28. The frame is rigidly attached to the respective reference device 14, 17, and matching the three calibrated points on the ears and the nasion to landmarks - defined, for example, using atlas segmentation - allows additional constraints to be used in the registration calculation.

## Claims

1. A medical image registration method in which an actual patient's body or portion of a patient's body (22) is positionally registered to a patient image created using a medical body-imaging technique such as MR, CT or x-ray imaging, wherein in a medical navigation system, the actual spatial position of at least a part of the body or body portion (22) is assigned to a respective position in the image of said body or body portion (22), characterised in that the part of the body or body portion (22) comprises a registration area in the form of the surface of a substantially rigid body structure, in particular an inner structure, made of bone or cartilage.

2. The method according to claim 1, wherein the registration area comprises the surface of one or more of the following body structures:

- the meatus or ear channel (12), or at least a part of the meatus, in particular the outer meatus;
- the palate, in particular the bony or hard palate;
- the upper inner jaw area and/or lower inner jaw area;
- the inner nose cartilage structure.

3. The method according to claim 1 or claim 2, wherein the registration area on the actual patient's body or portion of the patient's body (22) is measured by means of a surface scanner which in particular comprises a scanner probe (15) which can be positionally located and/or tracked.

4. The method according to claim 3, wherein the position and orientation of the probe (17) can be established by a tracking system which determines the actual spatial position of at least a part of the body or body portion.

5. The method according to claim 3 or claim 4, wherein the surface scanner also comprises a surface data recording and/or processing unit which creates a positionally determined surface model of the registration area.

6. The method according to any one of claims 1 to 5, wherein the registration area is measured by means of spaced interferometric measurements, in particular using a thin film interference scanner.

7. The method according to any one of claims 1 to 6, wherein at least one additional registration landmark on the actual patient's body or body portion (22) is manually acquired and included in the assignment process by assigning it to a respective position in the image in order to supplement the registration process and/or confirm the registration result, in particular the common angular orientation of the actual registration area and the registration area in the image.

8. The method according to any one of claims 1 to 7, wherein at least one additional registration point or landmark (28) on a frame (25) which is placed on the actual patient's body or body portion is acquired and included in the assignment process by assigning it to a corresponding related position, in particular a calculated position, in the image in order to supplement the registration process or to confirm the registration result, in particular the common angular orientation of the actual registration area and the registration area in the image.

9. The method according to claim 8, wherein the registration area on the actual patient's body or body part is measured by means of a positionally determined surface scanner (15) which in particular comprises a scanner probe which is fixedly attached to the frame, wherein the scanner (15) and/or the frame (25) can be positionally located or tracked by a tracking system which determines the actual spatial position of at least a part of the body or body portion.

10. A medical image registration device by means of which an actual patient's body or portion of a patient's body (22) is positionally registered to a patient image created

using a medical body-imaging technique such as MR, CT or x-ray imaging, wherein in a medical navigation system, the actual spatial position of at least a part of the body or body portion (22) is assigned to a respective position in the image of said body or body portion (22), characterised in that the registration device comprises a surface scanner (15) for scanning a registration area comprising the surface of a substantially rigid body structure, in particular an inner structure, made of bone or cartilage.

11. The device according to claim 10, characterised in that the scanner (15) is an inner surface scanner comprising a scanner probe (17) which can be positionally located and/or tracked and in particular used for inserting into and/or scanning the surface of one or more of the following body structures:

- the meatus or ear channel (12), or at least a part of the meatus, in particular the outer meatus;
- the palate, in particular the bony or hard palate;
- the upper inner jaw area and/or lower inner jaw area;
- the inner nose cartilage structure.

12. The device according to claim 10 or claim 11, characterised in that the scanner is an interferometric measurement scanner for spaced measurements, in particular a thin film interference scanner.

13. The device according to any one of claims 10 to 12, characterised in that it is fixed to:

- a fixation support for the actual body or body portion (22); or
- a frame (25) on the actual patient's body or body portion, wherein the frame (25) is positionally acquired and included in the assignment process by assigning it to a corresponding related position, in particular a calculated position, in the image in order to supplement the registration process or to confirm the registration result, in particular the common angular orientation of the actual registration area and the registration area in the image.

14. A program which, when it is running on a computer or is loaded onto a computer, causes the computer to perform a method in accordance with any one of claims 1 to 9.

15. A computer program storage medium which comprises a computer program according to claim 14.

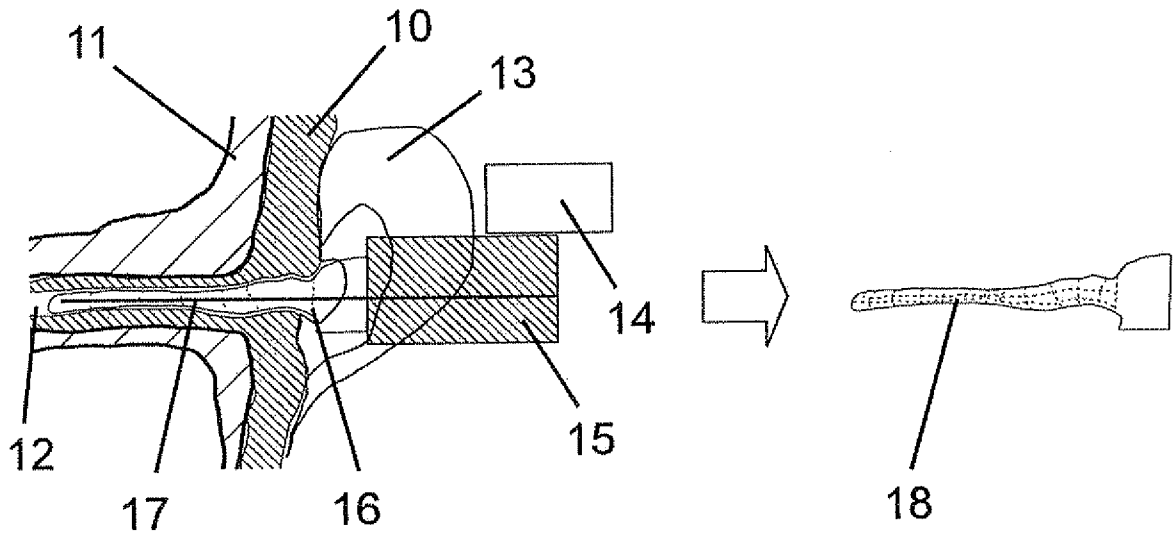


Figure 1

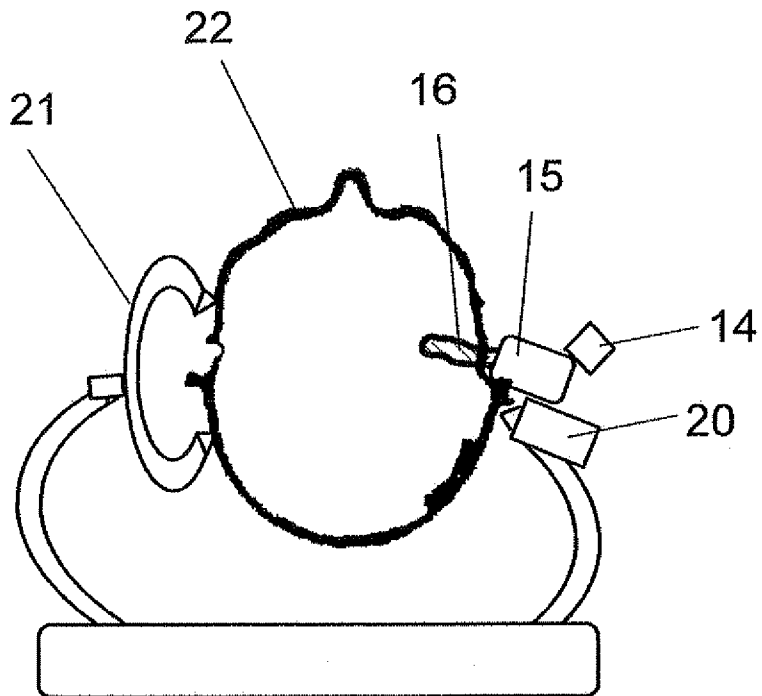


Figure 2

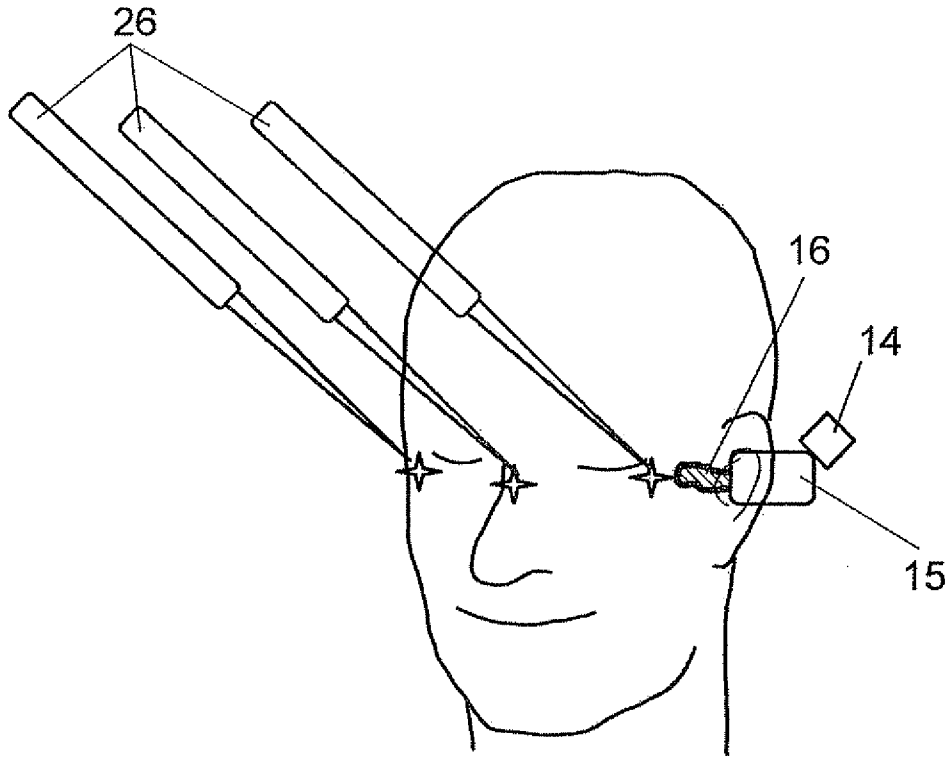


Figure 3

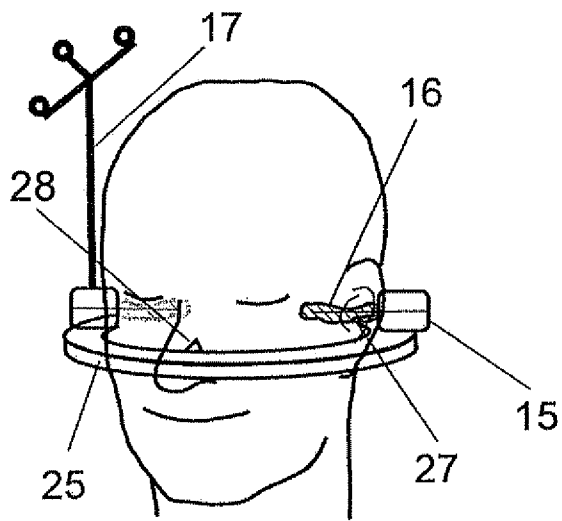


Figure 4

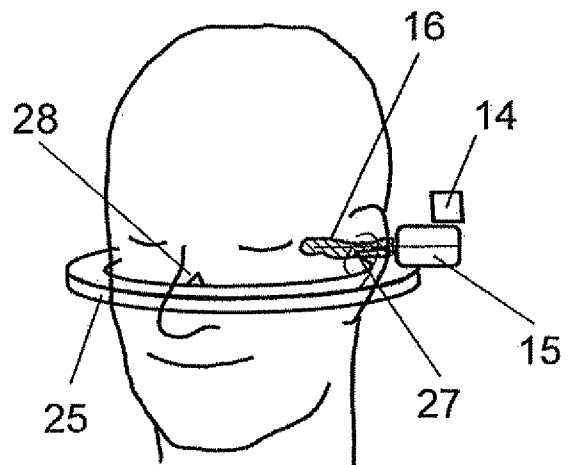


Figure 5



**INTERNATIONAL SEARCH REPORT**

International application No  
PCT/EP2010/059245

A. CLASSIFICATION OF SUBJECT MATTER  
ADD. A61B19/00

According to International Patent Classification (IPC) or to both national classification and IPC

**B. FIELDS SEARCHED**

Minimum documentation searched (classification system followed by classification symbols)  
A61B

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

**C. DOCUMENTS CONSIDERED TO BE RELEVANT**

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2010/160771 AI (GIELEN FRANS L H [NL] ET AL) 24 June 2010 (2010-06-24) paragraphs [0013] , [0060] - [0081] ; figure 2 -----	1,3-15
X	US 2006/173357 AI (VILSMEIER STEFAN [DE] ET AL) 3 August 2006 (2006-08-03) paragraphs [0005] , [0013] , [0016] , [0018] , [0037] - [0043] ; figures 1-4 -----	1-5 , 7-11 ,13, 14
X	BANKMAN I N: "Handbook of Medical Imaging - Processing and Analysis", HANDBOOK OF MEDICAL IMAGING PROCESSING AND ANALYSIS, XX, XX, 1 January 2000 (2000-01-01) , pages 623-633 , XP002322965 , pages 625-627 , item 2.2 ----- -/- -	1-3 ,5,7, 10, 14, 15

Further documents are listed in the continuation of Box C.

See patent family annex.

\* Special categories of cited documents :

- "A" document defining the general state of the art which is not considered to be of particular relevance
- "E" earlier document but published on or after the international filing date
- "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- "O" document referring to an oral disclosure, use, exhibition or other means
- "P" document published prior to the international filing date but later than the priority date claimed

- "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- "&" document member of the same patent family

Date of the actual completion of the international search

15 March 2011

Date of mailing of the international search report

24/03/2011

Name and mailing address of the ISA/  
European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040,  
Fax: (+31-70) 340-3016

Authorized officer  
  
Herberhold, C

## INTERNATIONAL SEARCH REPORT

International application No

PCT/EP2010/059245

C(Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT		
Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 6 347 240 B1 (FOLEY KEVIN T [US] ET AL) 12 February 2002 (2002-02-12)  paragraphs [0059] - [0064]; figure 6 -----	1,3-5, 7-11,14, 15
X	EP 1 219 260 A1 (BRAINLAB AG [DE]) 3 July 2002 (2002-07-03)  paragraph [0011] -----	1-3,5,7, 8,10,11, 14,15
X	W0 2004/000097 A2 (UNIV FLORIDA [US]; KIM SIYONG [US]; HELMIG RICHARD DAVID [US]) 31 December 2003 (2003-12-31) * abstract; figures 1-4 -----	1,2,14, 15
X	US 2005/222793 A1 (LLOYD CHARLES F [US] ET AL) 6 October 2005 (2005-10-06) paragraph [0025] -----	1,2,14, 15

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International application No <b>PCT/EP2010/059245</b>
--

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2010160771	A1	24-06-2010	NONE
-----			
US 2006173357	A1	03-08-2006	NONE
-----			
US 6347240	B1	12-02-2002	US 2002183610 A1 05-12-2002
			US 2006122483 A1 08-06-2006
			US 6434415 B1 13-08-2002
-----			
EP 1219260	A1	03-07-2002	AT 243473 T 15-07-2003
			DE 50002672 D1 31-07-2003
			ES 2199737 T3 01-03-2004
			US 2002077542 A1 20-06-2002
-----			
WO 2004000097	A2	31-12-2003	AU 2003251545 A1 06-01-2004
			US 2004064890 A1 08-04-2004
			US 2010151416 A1 17-06-2010
-----			
US 2005222793	A1	06-10-2005	US 2005228270 A1 13-10-2005
-----			