

(12) STANDARD PATENT
(19) AUSTRALIAN PATENT OFFICE

(11) Application No. **AU 2014274748 B2**

(54) Title
Patient-matched apparatus and methods for performing surgical procedures

(51) International Patent Classification(s)
A61B 5/05 (2006.01)

(21) Application No: **2014274748** (22) Date of Filing: **2014.06.06**

(87) WIPO No: **WO14/197844**

(30) Priority Data

(31) Number	(32) Date	(33) Country
61/845,463	2013.07.12	US
61/877,837	2013.09.13	US
61/832,583	2013.06.07	US

(43) Publication Date: **2014.12.11**

(44) Accepted Journal Date: **2018.03.01**

(71) Applicant(s)
George Frey

(72) Inventor(s)
Frey, George;Majors, Benjamin;O'Neil, Charles;Lai, Geoff;Rydin, Russ

(74) Agent / Attorney
FPA Patent Attorneys Pty Ltd, Level 43 101 Collins Street, Melbourne, VIC, 3000, AU

(56) Related Art
US 20110319745 A1
US 20120041445 A1



- (51) International Patent Classification: *A61B 5/05* (2006.01)
- (21) International Application Number: PCT/US2014/041379
- (22) International Filing Date: 6 June 2014 (06.06.2014)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:

61/832,583	7 June 2013 (07.06.2013)	US
61/845,463	12 July 2013 (12.07.2013)	US
61/877,837	13 September 2013 (13.09.2013)	US
- (72) Inventor; and
- (71) Applicant : **FREY, George** [US/US]; 2 Sunrise Drive, Englewood, CO 80113 (US).
- (72) Inventors: **MAJORS, Benjamin**; 1110 E. 4th Ave., Denver, CO 80218 (US). **O'NEIL, Charles**; 4695 W. Mineral Drive, #823, Littleton, CO 80128 (US). **LAI, Geoff**; 8391 W. Virginia Ave., Lakewood, CO 80226 (US). **RYDIN, Russ**; 1407 Laurenwood Way, Highlands Ranch, CO 80129 (US).
- (74) Agent: **WALSWORTH, Ian, R.**; SHERIDAN ROSS P.C., 1560 Broadway, Suite 1200, Denver, CO 80202 (US).
- (81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AO, AT, AU, AZ, BA, BB, BG, BH, BN, BR, BW, BY, BZ, CA, CH, CL, CN, CO, CR, CU, CZ, DE, DK, DM, DO, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, GT, HN, HR, HU, ID, IL, IN, IR, IS, JP, KE, KG, KN, KP, KR, KZ, LA, LC, LK, LR, LS, LT, LU, LY, MA, MD, ME, MG, MK, MN, MW, MX, MY, MZ, NA, NG, NI, NO, NZ, OM, PA, PE, PG, PH, PL, PT, QA, RO, RS, RU, RW, SA, SC, SD, SE, SG, SK, SL, SM, ST, SV, SY, TH, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, ZA, ZM, ZW.
- (84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LR, LS, MW, MZ, NA, RW, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, RU, TJ, TM), European (AL, AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HR, HU, IE, IS, IT, LT, LU, LV, MC, MK, MT, NL, NO, PL, PT, RO, RS, SE, SI, SK, SM, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, KM, ML, MR, NE, SN, TD, TG).

[Continued on next page]

(54) Title: PATIENT-MATCHED APPARATUS AND METHODS FOR PERFORMING SURGICAL PROCEDURES

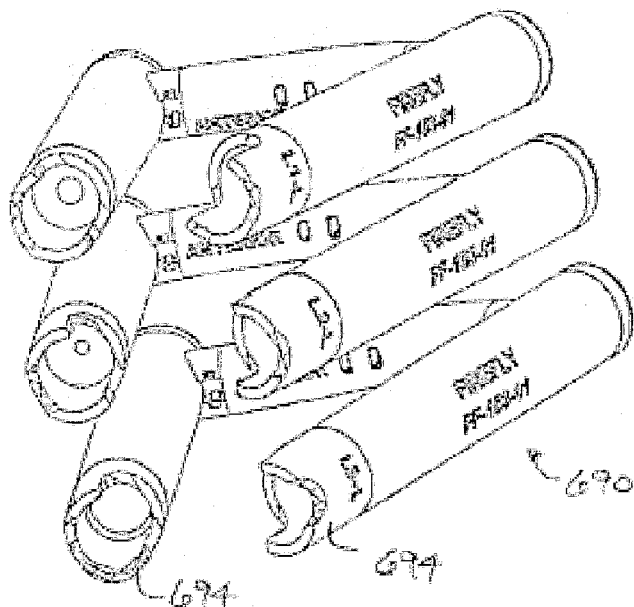


FIG. 73

(57) Abstract: A system and method for developing customized apparatus for use in one or more surgical procedures is disclosed. The system and method incorporates a patient's unique anatomical features or morphology. According to a preferred embodiment, the customized apparatus comprises a plurality of complementary surfaces. Thus, each apparatus may be matched and oriented around the patient's own anatomy, and may further provide any desired axial alignments or insertional trajectories. In an alternate embodiment, the apparatus may further be aligned and/or matched with at least one other apparatus used during the surgical procedure.



Published:

— with international search report (Art. 21(3))

— before the expiration of the time limit for amending the claims and to be republished in the event of receipt of amendments (Rule 48.2(h))

**PATIENT-MATCHED APPARATUS AND METHODS
FOR PERFORMING SURGICAL PROCEDURES**

5 **FIELD OF THE INVENTION**

The present disclosure relates to the field of medical devices and is generally directed toward apparatus configurable for use with a specific patient in a surgical setting based on the patient's unique anatomical features, and methods of manufacturing and using the same.

10 **CROSS-REFERENCE TO RELATED APPLICATIONS**

This application is a continuation-in-part of U.S. Patent Application No. 13/841,069, filed March 15, 2013. This application also claims the priority to U.S. Provisional Patent Application Nos. 61/832,583 filed June 7, 2013, 61/845,463 filed July 12, 2013 and 61/877,837 filed September 13, 2013. These applications are all
15 incorporated by reference herein in their entireties.

BACKGROUND OF THE INVENTION

Given the complexities of surgical procedures and the various tools, instruments, implants and other devices used in the procedures, as well as the varying anatomical differentiation between patients who receive those tools, instruments, implants and
20 devices, it is often challenging to create a surgery plan that accounts for the unique and sometimes irregular anatomical features of a particular patient. For example, the implantation of pedicle screws in a vertebral body (as an adjunct or stand-alone stabilization mechanism) is well accepted amongst surgeons who treat various spine pathologies, and although the performance of various pedicle screw constructs have
25 become predictable, there are still multiple challenges with the placement and insertion of the pedicle screws or other bone anchors. The challenges occur when a surgeon is unable to reference boney landmarks due to previous surgery or when the patient's anatomy is irregular in shape.

Surgeons now have the ability to readily convert magnetic resonance imaging
30 (MRI) data or computed tomography (CT) data into a data set readable by computer-aided design (CAD) program and/or finite element modeling (FEM) program, which then may be used to create, for example, a custom implant based on the dynamic nature of the anatomical structures the custom implant is designed to associate with. This data, while currently used by surgeons in surgery planning, is largely unused for creating a

customized set of instruments or other surgical devices that are designed to complement the patient's unique anatomy.

The prior art fails to teach a system for creating a suite of surgical apparatus based on the data set derived from the MRI or CT scan. For example, the use of the patient-specific data set for a vertebral body may allow a surgeon to accommodate for subtle variations in the position and orientation of a plate or other bone anchor to avoid particular boney anatomy or irregularities in the positioning and alignment of the adjoining vertebral bodies. As another example, the use of these data sets may also assist a surgeon in selecting a desired trajectory for an implantable device so as to avoid, for example, crossing the pedicle wall and violating the spinal canal during an actual procedure. The use of the data sets permit the surgeon to avoid these types of mistakes by creating customized tools and instruments, which may comprise orientation, end-stops or other safety related features to avoid over-torque and over-insertion of any implantable devices. The data sets also permit the surgeon to create a patient-contacting surface that is oriented to match one or more of the anatomical features represented by the data set, and thereby quickly and efficiently locate and place the patient-contacting surface(s) in the appropriate location and orientation.

It would therefore be advantageous to provide apparatus suitable for use with a surgical procedure that is adapted and/or configured and/or capable of conforming to a plurality of anatomical features of a particular patient and/or to one or more additional apparatus to assist the surgeon in completing the surgical procedure(s) safely and efficiently, and that otherwise significantly reduces, if not eliminates, the problems and risks noted above. Other advantages over the prior art will become known upon review of the Summary and Detailed Description of the Invention and the appended claims.

Reference to any prior art in the specification is not an acknowledgment or suggestion that this prior art forms part of the common general knowledge in any jurisdiction or that this prior art could reasonably be expected to be understood, regarded as relevant, and/or combined with other pieces of prior art by a skilled person in the art.

SUMMARY OF THE INVENTION

A novel system and method is described herein for developing customized apparatus for use in one or more surgical procedures. The system and method according to this embodiment uses a patient's unique morphology, which may be derived from capturing MRI data or CT or

other data to derive one or more "Patient Matched" apparatus, which comprises complementary surfaces based on a plurality of data points from the MRI or CT data. Each "Patient Matched" apparatus is matched and oriented around the patient's own anatomy, the desired insertional trajectories (which may be verified in a pre-operative setting using 3D CAD software, such as the software disclosed in WO 2008027549, which is incorporated by reference herein in its entirety), and according to one embodiment described herein, other apparatus used during the surgical procedure.

In a first aspect, the present invention provides a surgical device for use in a minimally invasive surgical procedure, comprising: two or more guides each having a proximal and a distal end, the distal ends each comprising patient-contacting surfaces configured to anatomically mate with and are determined from corresponding subcutaneous anatomical features of a patient; a coupling member selectively attachable to the proximal ends of a plurality of the two or more guides, thereby forming a medial portion of the surgical device; wherein the proximal ends of the two or more guides extend outside of the patient and wherein the coupling member is configured to be selectively attached to at least a first guide and a second guide outside of the patient; wherein the distal ends of the at least a first and second guides of the surgical device are configured to contact the corresponding subcutaneous anatomical features to ensure proper alignment and placement of the surgical device; and wherein the two or more guides, when coupled with the coupling member, are oriented in a pre-determined direction.

Also disclosed herein is a surgical device formed by anatomical data for a specific patient, comprising: a medial body of the surgical device, the medial body having a proximal and a distal end; at least one patient-specific element selectively coupled to the distal end of the medial body and configured to be positioned on a patient-specific subcutaneous anatomical feature corresponding to the patient-specific element; the medial body further comprising a central bore configured to receive at least one insert; the at least one insert selectively positioned within the medial body of the surgical device, the at least one insert comprising an aperture for receiving an instrument or implant; wherein the aperture of the at least one insert is customized to receive an instrument or advance an implant by a predetermined distance.

In a second aspect, the present invention provides an orthopedic device for use in a minimally invasive surgical procedure, comprising: a first patient-specific element configured to at least one patient-specific surface determined from a patient's anatomy and which anatomically

conforms to at least a first subcutaneous anatomic feature of a specific patient; a second patient-specific element configured to at least one second patient-specific surface determined from a patient's anatomy and which anatomically conforms to at least a second subcutaneous anatomic feature of a specific patient; and an arcuate bridge coupling the first and second patient-specific elements, the arcuate bridge configured to be selectively engaged with the first and second patient-specific elements at a location beyond the patient's anatomy.

By way of providing additional background, context, the following are incorporated by reference in their entireties for the express purpose of explaining the nature of minimal access, less invasive, or minimally invasive surgery ("MIS") procedures and to further describe the various tools and other apparatus commonly associated therewith: U.S. Pat. No. 6,309,395 to Smith et al; U.S. Pat. No. 6,142,998 to Smith et al; U.S. Pat. No. 7,014,640 to Kemppanien et al; U.S. Pat. No. 7,406,775 to Funk, et al; U.S. Pat. No. 7,387,643 to Michelson; U.S. Pat. No. 7,341,590 to Ferree; U.S. Pat. No. 7,288,093 to Michelson; U.S. Pat. No. 7,207,992 to Ritland; U.S. Pat. No. 7,077,864 Byrd III, et al; U.S. Pat. No. 7,025,769 to Ferree; U.S. Pat. No. 6,719,795 to Cornwall, et al; U.S. Pat. No. 6,364,880 to Michelson; U.S. Pat. No. 6,328,738 to Suddaby; U.S. Pat. No. 6,290,724 to Marino; U.S. Pat. No. 6,113,602 to Sand; U.S. Pat. No. 6,030,401 to Marino; U.S. Pat. No. 5,865,846 to Bryan, et al; U.S. Pat. No. 5,569,246 to Ojima, et al; U.S. Pat. No. 5,527,312 to Ray; and U.S. Pat. Appl. No. 2008/0255564 to Michelson.

Various surgical procedures may be performed through introduction of rods or plates, screws or other devices into adjacent boney anatomy to join various portions of, for example, a vertebra to a corresponding portion on an adjacent vertebra. MIS procedures are often performed in the sacroiliac, lumbar, thoracic, or cervical spine regions of a patient. MIS procedures performed in this area are often designed to stop and/or eliminate all motion in the spinal segment by destruction of some or all of the joints in that segment and further utilizing bone graft material and/or rigid implantable fixation devices for securing the adjacent vertebrae. By eliminating movement, back pain and further degenerative disc disease may be reduced or avoided. Fusion requires tools for accessing the vertebrae, such as surgical cannulae for MIS procedures, and other tools for implanting the desired implant, bioactive material, etc. Such procedures often require introduction of additional tools to prepare a site for implantation. These tools may include drills, drill guides, debridement tools, irrigation devices, vises, clamps, cannula, and other insertion/retraction tools.

Spinal and other surgeries may be performed by a number of different MIS procedures, as opposed to conventional surgical procedures and methods, which typically

require cutting of muscles, removal of bone, and retraction of other natural elements. During a MIS procedure, a less destructive approach to the patient anatomy is carried out by using retractor tubes or portals, which take advantage of anatomy and current technology to limit the damage to intervening structures.

5 In a typical MIS procedure on the spine, skeletal landmarks are established fluoroscopically and a small incision is made over the landmark(s). According to various methods known in the prior art, a series of dilators are applied until one or more cannula is placed over the anatomic structure. In some procedures, a microscope is then placed over the operative site to provide illumination and magnification with a three dimensional view
10 of the anatomical site to ensure that the surgeon is able to accurately locate the desired patient anatomy and properly position and orient any tool, instrument or other surgical device used during the MIS procedure. The microscope, however, is an expensive and unwieldy device requiring uncomfortable gyrations of the surgeon's back and neck in order to gain the necessary view, and is also a nuisance to drape (a large, sterile plastic bag
15 has to be placed over the eight foot tall structure). The use of adequate illumination is also difficult to direct due to the size of the microscope.

A significant danger of performing MIS operations, and in particular accessing an intervertebral space during a MIS surgery on the spine, is that of inadvertently contacting or damaging the para-spinal nerves, including the exiting nerve roots, traversing nerves
20 and the nerves of the cauda equina. The exact location of these para-spinal nerves cannot be precisely determined prior to the commencement of surgery, and therefore are dependent on a surgeon's ability to visually locate the same after the initial incision is made. Moreover, intervertebral spaces in the spine have other sensitive nerves disposed at locations which are not entirely predictable prior to insertion of the surgical tool into the
25 intervertebral area. Accordingly, the danger of pinching or damaging spinal nerves when accessing an intervertebral space has proven to be quite limiting to the methods and devices used during minimally invasive spinal surgery. In addition, as cannula are received through the patient's back, such as when performing minimally invasive spinal surgery, minor blood vessels are ruptured, thereby blocking the surgeon's vision inside the
30 intervertebral region after the cannula has been inserted. Other anatomical features at a particular patient may also obstruct the surgeon's view or make it difficult to provide illumination within the cannula. Therefore, one particular shortcoming that is addressed by the present disclosure is to provide devices which are patient-matched to facilitate proper

location and orientation without use of microscopes or other equipment and that otherwise eliminate the problems associated with prior art MIS procedures.

The customized and integrated matching aspects of this presently disclosed system provides an advantage over the prior art, in particular by providing a plurality of
5 interlocking and/or matching points for each apparatus, which in turn reduces the likelihood of misalignment, misplacement and subsequent mistake during the surgical procedure(s).

Accordingly, one aspect of the present disclosure is to provide a method for preparing a customized surgical device or instrument, which in a preferred embodiment
10 comprises the following steps:

obtaining data associated with a patient's anatomy;

converting the data obtained to a 3-dimensional data set(s);

determining at least one trajectory or path for facilitating a surgical procedure to be performed on the patient;

15 determining at least one surface associated with the patient's anatomy;

generating a 3-dimensional representation of the customized surgical device or instrument, which incorporates the at least one trajectory of path and a matching surface to the at least one surface associated with the patient's anatomy; and

20 fabricating the customized surgical device or instrument using the 3-dimensional representation.

According to another aspect of the present disclosure, a system and method for facilitating a surgical procedure(s) comprises the following steps:

Obtaining data associated with the patient's anatomy by way of a MRI or CT scan;

Converting the MRI or CT scan data to a 3-Dimensional data set(s)

25 Determining one or more axes or planes of orientation of a device to be constructed for use in facilitating the surgical procedure(s) to be performed on the patient;

Modeling the device for use in facilitating the surgical procedure(s) using the determined axes and accounting for any other constraints derived from the converted data set(s);

30 Generating a prototype of the modeled device by, for example, use of rapid prototyping machinery; and

Preparing the prototype for use during the surgical procedure(s).

According to this aspect described above, the method step of accounting for any other constraints derived from the converted data set(s) may comprise adjusting the size of the modeled device to accommodate the space limitations on the surgeon, orienting elements of the modeled device to avoid certain anatomical features, creating one or more surfaces that may conveniently be operatively associated with one or more instruments and/or tools used in the surgical procedure(s), etc.

According to yet another aspect of the present disclosure, the system and method includes use of data obtained from a radiographic imaging machine, a fluoroscopy, an ultrasonic machine or a nuclear medicine scanning device.

In another aspect, the patient-matching features may be confirmed by one or more additional process, such as fluoroscopy or other processes known to those of skill in the art.

In one aspect of the present disclosure, the method comprises the use of bone density data obtained through a CT scan of the patient anatomy for use in planning the trajectory of a surgical guide and corresponding fixation device or instrument, such as a cutting/routing/drilling instrument intended to penetrate the boney anatomy. This data may be used in other manners contemplated and described herein to assist the surgeon in planning, visualizing or otherwise preparing for the surgical procedure for the patient.

In yet another alternative embodiment, the data obtained from one of the scanning devices described above may be supplemented or merged with data from a bone density scanner to fabricate a device that is designed to remain in the patient after the surgical procedure is completed. It is to be expressly understood that data from a bone density scanner is not necessary to practice the inventions described herein, but may supplement the data and assist a surgeon or other medical professional in determining the proper location, trajectory, orientation or alignment of the various apparatus described herein.

According to yet another aspect of the present disclosure, data may be supplemented or merged with data from a bone density scanner to achieve further control over the orientation of any desired axes, particularly where the surgical procedure involves insertion of one or more implantable devices.

According to yet another embodiment, the data obtained from the patient permits the apparatus to be manufactured with defined pathways through the apparatus, which are operatively associated with at least one tool, instrument, or implant, and which permit the at least one tool, instrument or implant to be inserted in the defined pathways in a

consistent and reproducible manner. Examples of devices that are implanted or remain in the patient include anchoring devices such as screws, pins, clips, hooks, etc., and implantable devices such as spacers, replacement joints, replacement systems, cages, etc..

According to yet another aspect of the present disclosure, a preconfigured surgical
5 template is disclosed, which comprises one or more guides for receiving at least one tool. According to this embodiment, the one or more guides further comprise patient-contacting surfaces formed to be substantially congruent with the anatomical features of a patient. The preconfigured surgical template is configured such that the patient-contacting surfaces are configured to contact the plurality of anatomical features in a mating engagement, to
10 ensure proper alignment and mounting of the guide or template, and the guides of the preconfigured surgical template are oriented in a direction selected prior to manufacturing of the preconfigured surgical template to achieve desired positioning, aligning or advancing of a tool within the one or more guides.

According to yet another aspect of the present disclosure, a method for creating a
15 template for use in a surgical operation is disclosed, comprising the steps of:

collecting data from the patient corresponding to the patient's unique anatomy;

creating a model of the template from the data collected, the model comprising a plurality of matching surfaces to the patient's unique anatomy;

providing data associated with model to fabrication machinery;

20 rapidly generating the template to comprise the plurality of matching surfaces and further comprising at least one additional matching surface corresponding to at least one tool or instrument used in the surgical operation; and

generating a permanent device based on the template for use in the surgical operation.

25 In one embodiment of the present disclosure the model is a digital model. In another embodiment of the present disclosure the model is a physical model.

According to yet another aspect of the present disclosure, a system for performing a surgical procedure on a patient is disclosed, comprising:

a surgical guide;

30 the surgical guide comprising a plurality of surfaces determined from data scanned from the patient, the plurality of surfaces configured to match the patient's boney anatomy;

the surgical guide further comprising at least one trajectory or path determined from the patient's boney anatomy for facilitating the surgical procedure;

the surgical guide further comprising at least one sleeve, the sleeve comprised of a conductive material and having a first end and a second end;

an instrument comprising at least a first portion comprised of a conductive material and adapted to be received within the at least one sleeve by inserting the at least a first
5 portion in the first end of the at least one sleeve and contact the conductive material of the at least one sleeve;

wherein the at least a first portion of the instrument is adapted to pass through the at least one sleeve and exit the second end of the at least one sleeve; and

wherein the surgical guide may be subject to an electrical current for providing
10 intra-operative monitoring (IOM) of the instrument during contact with the surgical guide and with the patient anatomy.

Further aspects of the present disclosure are directed to the system described above and further comprising a surgical guide which is subject to an electrical current by providing at least one electrode on the conductive material of the surgical guide and
15 providing electrical current to the at least one electrode.

Further aspects of the present disclosure provide a method for manufacturing a surgical guide at an off-site manufacturing location, an on-site manufacturing location, a clinic, a surgery center, a surgeon's offices, a public hospital or at a private hospital.

Still further aspects of the present disclosure include a surgical guide manufactured
20 using one of the methods described herein, wherein the guide is manufactured by a process selected from the group consisting of a rapid prototyping machine, a stereolithography (SLA) machine, a selective laser sintering (SLS) machine, a selective heat sintering (SHM) machine, a fused deposition modeling (FDM) machine, a direct metal laser sintering (DMLS) machine, a powder bed printing (PP) machine, a digital light processing
25 (DLP) machine, an inkjet photo resin machine, and an electron beam melting (EBM) machine.

Incorporated by reference in their entireties are the following U.S. patents and patent applications directed generally to methods and apparatus related to surgical procedures, thus providing written description support for various aspects of the present
30 disclosure. The U.S. patents and pending applications incorporated by reference are as follows: U.S. Pat. Nos. 7,957,824, 7,844,356 and 7,658,610, and U.S. Pat. Pub. Nos. 2010/0217336, 2009/0138020, 2009/0087276 and 2008/0114370.

One having skill in the art will appreciate that embodiments of the present disclosure may have various sizes. The sizes of the various elements of embodiments of the present disclosure may be sized based on various factors including, for example, the anatomy of the patient, the person or other device operating with or otherwise using the apparatus, the surgical site location, physical features of the devices and instruments used with the devices described herein, including, for example, width, length and thickness, and the size of the surgical apparatus.

Embodiments of the present disclosure present several advantages over the prior art including, for example, the speed and efficacy of the procedure, the minimally invasive aspects of the procedure, the disposability of the prototype devices, the ability to introduce customized implements or tools to the surgical site with minimal risk and damage to the surrounding tissue, lower risk of infection, more optimally placed and/or oriented guides and implantable devices, a more stable and controlled method of placing and inserting of apparatus associated with the surgical procedure further reducing the likelihood of the apparatus becoming misaligned or dislodged, and fewer and/or less expensive tools and instruments in a surgical site, among other advantages. For example, the embodiments reduce the number and need for multiple trays, instruments and different size devices used in a particular surgery, thereby reducing the cost of the equipment necessary to complete the surgery. The embodiments also reduce the cumulative radiation exposure to both the surgeon and medical professionals in the operating environment and the patient.

One having skill in the art will appreciate that embodiments of the present disclosure may be constructed of materials known to provide, or predictably manufactured to provide the various aspects of the present disclosure. These materials may include, for example, stainless steel, titanium alloy, aluminum alloy, chromium alloy, and other metals or metal alloys. These materials may also include, for example, PEEK, carbon fiber, ABS plastic, polyurethane, polyethylene, photo-polymers, resins, particularly fiber-encased resinous materials rubber, latex, synthetic rubber, synthetic materials, polymers, and natural materials.

One having skill in the art will appreciate that embodiments of the present disclosure may be used in conjunction devices that employ automated or semi-automated manipulation. Embodiments of the present disclosure may be designed such that the apparatus may be formed and verified, for example, remotely by an operator, remotely by an operator through a computer controller, by an operator using proportioning devices,

programmatically by a computer controller, by servo-controlled mechanisms, by hydraulically-driven mechanisms, by pneumatically-driven mechanisms or by piezoelectric actuators. It is expressly understood for purposes of this disclosure that other types of machinery other than rapid prototyping machinery may be employed in the systems and methods described herein, for example, by computerized numerical control (CNC) machinery.

The Summary of the Invention is neither intended nor should it be construed as being representative of the full extent and scope of the present disclosure. The present disclosure is set forth in various levels of detail in the Summary of the Invention as well as in the attached drawings and the Detailed Description of the Invention and no limitation as to the scope of the present disclosure is intended by either the inclusion or non-inclusion of elements, components, etc. in this Summary of the Invention. Additional aspects of the present disclosure will become more readily apparent from the Detailed Description, particularly when taken together with the drawings.

The above-described benefits, embodiments, and/or characterizations are not necessarily complete or exhaustive, and in particular, as to the patentable subject matter disclosed herein. Other benefits, embodiments, and/or characterizations of the present disclosure are possible utilizing, alone or in combination, as set forth above and/or described in the accompanying figures and/or in the description herein below. However, the claims set forth herein below define the invention.

BRIEF DESCRIPTION OF THE DRAWINGS

The accompanying drawings, which are incorporated in and constitute a part of the specification, illustrate embodiments of the disclosure and together with the general description of the disclosure given above and the detailed description of the drawings given below, serve to explain the principles of the disclosures.

It should be understood that the drawings are not necessarily to scale. In certain instances, details that are not necessary for an understanding of the disclosure or that render other details difficult to perceive may have been omitted. It should be understood, of course, that the disclosure is not necessarily limited to the particular embodiments illustrated herein.

In the drawings:

Fig. 1 is a perspective view of a three-dimensional model of a unique grouping of anatomical features from which a set of data points may be derived according to one embodiment of the present disclosure;

Fig. 2 is a flow chart diagram showing the various steps of performing a method of manufacturing and using an apparatus for facilitating a surgical procedure according to one embodiment of the present disclosure;

Fig. 3 is a side elevation view of a particular apparatus for facilitating a surgical procedure according to one embodiment of the present disclosure;

Fig. 4 is rear elevation view of the apparatus shown in Figure 3;

Fig. 5 is a top plan view of the apparatus shown in Figure 3, relative to a unique grouping of anatomical features, and according to one embodiment of the present disclosure;

Fig. 6 is a perspective view of the apparatus and unique grouping of anatomical features shown in Figure 5;

Fig. 7 is another perspective view of the apparatus shown in Figure 3 demonstrating the customized patient-matching surfaces of the apparatus;

Fig. 8 is a perspective view of an apparatus according to an alternative embodiment of the present disclosure;

Fig. 9 is a perspective view of an apparatus according to yet another alternative embodiment of the present disclosure.

Fig. 10 is another perspective view of the apparatus shown in Figure 3 along with a custom fabricated instrument for use during a particular surgical procedure;

Figs. 11A-B are perspective views of an apparatus according to another alternative embodiment of the present disclosure;

Fig. 12 is a perspective view of the apparatus shown in Figures 11A-B in an assembled state;

Fig. 13 is a perspective view of an apparatus according to yet another alternative embodiment of the present disclosure;

Fig. 14 is a perspective view of an apparatus according to yet another alternative embodiment of the present disclosure;

Fig. 15 is a perspective view according to yet another alternative embodiment of the present disclosure;

Fig. 16 is a different perspective view of the apparatus shown in Figure 15;

Fig. 17 is an exploded perspective view of the apparatus shown in Figure 15.

Figs. 18-19 are perspective views according to yet another alternative embodiment of the present disclosure;

5 Figs. 20-21 are perspective views according to yet another alternative embodiment of the present disclosure;

Fig. 22 is a perspective view according to yet another alternative embodiment of the present disclosure;

Fig 23 is a perspective view according to yet another alternative embodiment of the present disclosure;

10 Fig. 24 is a perspective view according to yet another alternative embodiment of the present disclosure;

Fig. 25 is a perspective view according to yet another alternative embodiment of the present disclosure;

15 Fig. 26A is a perspective view according to yet another alternative embodiment of the present disclosure;

Fig. 26B is a perspective view according to the embodiment shown in Figure 26A;

Fig. 27A is a front elevation view according to yet another alternative embodiment of the present disclosure;

Fig. 27B is a perspective view according to the embodiment shown in Figure 27A;

20 Fig. 28 is an elevation view according to yet another alternative embodiment of the present disclosure;

Fig. 29A is a perspective view according to yet another alternative embodiment of the present disclosure;

25 Fig. 29B is a perspective view according to yet another alternative embodiment of the present disclosure;

Fig. 30 is a perspective view according to yet another alternative embodiment of the present disclosure;

Fig. 31 is a perspective view according to yet another alternative embodiment of the present disclosure;

30 Fig. 32A is a perspective view according to yet another alternative embodiment of the present disclosure;

Fig. 32B is a perspective view according to the embodiment shown in Figure 32A;

Fig. 33A is a perspective view according to yet another alternative embodiment of the present disclosure;

Fig. 33B is a perspective view according to the embodiment shown in Figure 33A;

Fig. 33C is another perspective view according to the embodiment shown in Figure
5 33A depicted with the cutting guide of Figure 32A;

Fig. 34A is a perspective view according to yet another alternative embodiment of the present disclosure;

Fig. 34B is a perspective view according to yet another alternative embodiment of the present disclosure;

10 Fig. 35 is a top plan view according to yet another alternative embodiment of the present disclosure;

Fig. 36 is a detailed view of the device according to the embodiment shown in Figure 35;

15 Fig. 37 is another top plan view of the device according to the embodiment shown in Figure 35;

Fig. 38 is a top plan view according to yet another alternative embodiment of the present disclosure;

Fig. 39 is another top plan view of the device according to the embodiment shown in Figure 38;

20 Figs. 40A-D are additional top plan views of the devices according to the embodiments shown in Figures 35-39;

Fig. 41 includes side elevation views of devices according to another alternative embodiment of the present disclosure;

25 Figs. 42A-B are top plan views of a device according to another alternative embodiment of the present disclosure;

Figs. 43A-B are additional top plan views of a device according to yet another alternative embodiment of the present disclosure;

Fig. 44A-B are perspective views of the devices shown in Figures 43A-B;

30 Fig. 45 includes side elevation views of drill sleeve devices according to another alternative embodiment of the present disclosure;

Fig. 46 is a front elevation view according to another alternative embodiment of the present disclosure;

Figs. 47A-D are views of an assembly tray and arrangement device according to another alternative embodiment of the present disclosure;

Figs. 48A-C are views of a device for providing patient-specific contacting surfaces and trajectories in a patient's cervical spine;

5 Figs. 49A-C are views of another device for providing patient-specific contacting surfaces and trajectories in a patient's cervical spine;

Figs. 50A-D and 51A-C are views of yet another device for providing patient-specific contacting surfaces and trajectories in a patient's cervical spine;

10 Figs. 52A-C are views of yet another device for providing patient-specific contacting surfaces and trajectories in a patient's cervical spine;

Figs. 53A-E are views of an unassembled and assembled device for providing patient-specific contacting surfaces and trajectories in a patient's cervical spine;

Figs. 54A-C are views of a device for providing patient-specific contacting surfaces and trajectories along with an instrument for positioning the same;

15 Figs. 55A-C are views of yet another device for providing patient-specific contacting surfaces and trajectories in a patient's cervical spine;

Figs. 56A-D are views of yet another device for providing patient-specific contacting surfaces and trajectories in a patient's cervical spine;

20 Fig. 57 is a side elevation view of a patient-specific insert for use with the devices shown in Figures 48A-56D referenced above;

Figs. 58A-C are views of a modeling device for creating a patient-specific or generic guide with predetermined trajectories;

Figs. 59A-D are views of yet another embodiment of a guide for use in a patient's cervical spine;

25 Figs. 60A-C are additional views of a guide for use in a patient's cervical spine;

Figs. 61A-C show views of yet another embodiment of a guide for use in a patient's cervical spine;

Figs. 62A-E show views of yet another embodiment of a guide for use in a patient's cervical spine;

30 Figs. 63A-H show various views of additional embodiments of a guide and related apparatus for use in a patient's cervical spine;

Figs. 64-66 are views of a device having custom inserts for inserting guide wires;

Fig. 67 is the device shown in Figures 64-66 with the inserts removed;

Fig. 68 shows Figure 67 with the device removed but with the wires remaining;
and

Figs. 69-73 are various views of a device according to yet another alternate embodiment of the present disclosure for use in a MIS procedure;

5 Fig. 74 is a perspective view of the device shown in Figs. 69-73 further comprising one or more optional alignment/depth/position control elements;

Fig. 75 is an alternate embodiment of the device shown in Figs. 69-73;

Figs. 76A-C are views of an alternative embodiment of a device further comprising one or more optional alignment/depth/position control elements;

10 Figs. 77A-G are views of another alternative embodiment of a device further comprising one or more optional alignment/depth/position control elements;

Figs. 78A-B are views of another alternative embodiment of a device further comprising one or more optional alignment/depth/position control elements;

15 Figs. 79A-B are views of another alternative embodiment of a device further comprising one or more optional alignment/depth/position control elements;

Fig. 80 is a detailed view of the device of Figs. 79A-B;

Figs. 81A-C are various views of a MIS device according to another embodiment;

Figs. 82A-B are various views of a MIS device according to yet another embodiment;

20 Figs. 83A-D are various views of a MIS device according to yet another embodiment;

Figs. 84A-E are various views of a MIS device according to yet another embodiment;

Fig. 85 is a view of another MIS device according to an alternate embodiment;

25 Figs. 86A-C are various views of a MIS device according to yet another embodiment;

Figs. 87A-B are various views of a MIS device according to yet another embodiment;

30 Figs. 88A-B are various views of a MIS device according to yet another embodiment;

Figs. 89A-B are various views of a MIS device according to yet another embodiment;

Figs. 90A-C are various views of a MIS device according to yet another embodiment;

Figs. 91A-D are various views of a MIS device according to yet another embodiment;

5 Figs. 92A-D are various views of a MIS device according to yet another embodiment;

Figs. 93A-D are various views of templates which may be contoured using methods described herein for create a patient-specific device;

10 Figs. 94A-C are various views of one embodiment of the present disclosure, which includes a plurality of patient-specific guides;

Figs. 95A-C are side elevation views of a connection mechanism according to one embodiment of the present disclosure;

Figs. 96A-C are side perspective views of a connection mechanism according to another embodiment of the present disclosure;

15 Figs. 97A-C are side perspective views of a connection mechanism according to yet another embodiment of the present disclosure;

Figs. 98A-C are side perspective views of an insert and guide sleeve according to one embodiment of the present disclosure;

20 Figs. 99A-G show various views of a system for aligning a guide according to one of the various embodiments described herein;

Figs. 100A-D are side perspective views of an insert according to one embodiment of the present disclosure; and

Figs 101A-D are various views of a patient-specific guide according to yet another alternative embodiment of the present disclosure.

25 **DETAILED DESCRIPTION**

As shown in the appended Figures and described in further detail herein, the present disclosure relates to a novel system and method for developing a variety of customized, patient-matched apparatus for use in a diverse number of surgical procedures. The system and method uses a patient's unique morphology, which may be derived from capturing MRI data or CT data to derive one or more patient-matched apparatus, which
30 comprise complementary surfaces to those encountered during the surgical procedure(s) as derived from a set of data points. According to various embodiments described herein, the patient-matched apparatus may further comprise desired axes and/or insertional

trajectories. According to one alternate embodiment described herein, the patient-matched apparatus may be further matched with at least other apparatus used during the surgical procedure. Other features of the disclosure will become apparent after a review of the following disclosures and varying embodiments of the invention.

5 Multiple embodiments of the disclosure are depicted in Figures 1-101. Referring now to Figure 1, a perspective view of a three-dimensional model of a unique grouping of anatomical features according to one embodiment of the present disclosure is shown. Here, the model **2** is comprised of multiple vertebral bodies **4, 6** but according to other embodiments may be comprised of any anatomical grouping for a particular patient. Data
10 associated with the model **2** may be captured from a MRI or CT scan or from radiographic images of the patient's corresponding boney anatomy (or alternatively from other data sources). The data, once captured, may be converted using known software tools to a CAD program, where the data set is representative of the model **2** and may be used to provide additional data points for forming the contours, sizes, shapes and orientations of one or
15 more apparatus to be used in the surgical procedure.

According to an alternative embodiment, the data may be obtained from an ultrasonic or nuclear medicine scanning device. In yet another alternative embodiment, the data may be supplemented or merged with data from a bone density scanner to fabricate a device that is designed to remain in the patient after the surgical procedure is completed,
20 or alternatively to achieve further control over the orientation of any desired axes, particularly where the surgical procedure involves insertion of one or more implantable devices.

Figure 2 is a flow chart showing the various steps of performing a method of manufacturing an apparatus, according to various embodiments described herein, for use
25 in facilitating a surgical procedure. The method, according to a preferred embodiment, comprises the following steps:

- A) Obtaining data associated with the patient's anatomy by way of a MRI or CT scan;
- B) Converting the MRI or CT scan data to a 3-Dimensional data set(s)
- 30 C) Determining one or more axes of orientation of a device to be constructed for use in facilitating the surgical procedure(s) to be performed on the patient;

D) Modeling the device for use in facilitating the surgical procedure(s) using the determined axes and accounting for any other constraints derived from the converted data set(s);

E) Generating a prototype of the modeled device by, for example, use of rapid prototyping machinery; and

F) Preparing the prototype for use during the surgical procedure(s).

As shown in Figure 2, the method may comprise additional steps or may be repeated for additional devices used in the surgical procedure. The step of obtaining data is typically performed in a traditional manner, by subjecting the patient to a scan using MRI or CT or other suitable scanning equipment known in the art. The data is then captured by the equipment and may be converted to a 3-Dimensional data set(s) by software or other algorithmic means known in the art, such as by exporting the data into a known modeling software program that allows data to be represented, for example, in CAD format. Once this data is converted, a device may be modeled to complement the data set(s) and oriented by one or more axes determined by the surgeon either before or through observation of the data set(s) from the initial scan of the patient's anatomy.

The method step of accounting for any other constraints derived from the converted data set(s) may comprise adjusting the size of the modeled device to accommodate the space limitations on the surgeon, orienting elements of the modeled device to avoid certain anatomical features, creating one or more surfaces that may conveniently be operatively associated with one or more instruments and/or tools used in the surgical procedure(s), etc. The prototype may be generated using known rapid prototyping machinery, or alternatively by milling machinery such as a CNC milling machine. Alternatively, the initial device fabricated by this method may be in a temporary state for further consideration and or manipulation by the surgeon, and then finally constructed using one of the methodologies described herein. The steps may be repeated for complementary devices, some or all of which may include further matching surfaces for the patient's anatomy or to the previously fabricated devices (i.e., the devices fabricated may have matching surfaces for adjoining together one or more devices, as described in greater detail below).

Alternatively, the system and method described herein may facilitate the alignment of various anatomical features for a particular patient, such as, for example, multiple vertebral bodies in a patient to correct spinal deformities. For example, the data set(s) may

provide an initial location for the anatomical features, but may be further manipulated by the surgeon in a pre-operative setting to create a desired data set(s), such as a final location for the anatomical features once the surgical procedure(s) are completed. In this manner, the devices formed by the system and method described above may be used in either an
5 initial location or a final location for the anatomical features, and be matched to those specific locations and orientations for each stage of the surgical procedure. These staged devices would in turn provide the surgeon with a visual guide to determine the degree of correction achieved through the surgical procedure, as compared to the pre-operative plan. Other variations on the method of the present disclosure are described in the Summary of
10 the Invention and included in the appended claims.

Fabrication methods may comprise the use of a rapid prototyping machine, such as a stereolithography (STL) machine, selective laser sintering (SLS) machine, or a fused deposition modeling (FDM) machine, direct metal laser sintering (DMLS), electron beam melting (EBM) machine, or other additive manufacturing machine. One example of such a
15 rapid prototyping machine is commercially available from 3D Systems and known as Model SLA-250/50. The rapid prototyping machine selectively hardens a liquid, powdered or other non-hardened resin or metal into a three-dimensional structure, which can be separated from the remaining non-hardened resin, washed/sterilized and used directly as the apparatus. The prototyping machine receives the individual digital data sets and
20 produces one structure corresponding to each of the desired apparatus.

Generally, because stereolithographic machinery produces a resin, which may have less than optimal mechanical properties (which may not be generally acceptable for a particular surgical use), the prototyping machine may alternatively be used to produce a mold. After the model is prepared, a conventional pressure or vacuum molding machine
25 may be used to produce the apparatus from a more suitable material, such as stainless steel, titanium alloy, aluminum alloy, chromium alloy, PEEK, carbon fiber, or other metals or metal alloys.

According to another alternative embodiment, the system and method may comprise providing the data set(s) to a CNC machine, which in turn may be utilized to
30 manufacture a custom milled apparatus from one of the more mechanically sound materials listed above. In yet another alternative embodiment, volume manufacturing of apparatus in accordance with the embodiments described herein may also be achieved, for

example, where a particular orientation or insertion trajectory is common among a large grouping of patients.

According to one particular embodiment of the present disclosure, a system and method is provided for fabricating apparatus for use with a variety of surgical procedures associated with a patient's spine. Individuals who suffer degenerative disc disease, natural spine deformations, a herniated disc, spine injuries or other spine disorders often require surgery on the affected region to relieve the individual from pain and prevent further injury. Such spinal surgeries may involve removal of damaged joint tissue, insertion of a tissue implant and/or fixation of two or more adjacent vertebral bodies, with the surgical procedure varying depending on the nature and extent of the injury.

For patients with varying degrees of degenerative disc disease and/or nerve compression with associated lower back pain, spinal fusion surgery, or lumbar arthrodesis ("fusion") is commonly used to treat the degenerative disease. Fusion commonly involves distracting and/or decompressing one or more intervertebral spaces, followed by removing any associated facet joints or discs, and then joining or "fusing" two or more adjacent vertebra together. Fusion of vertebral bodies also commonly involves fixation of two or more adjacent vertebrae, which may be accomplished through introduction of rods or plates, and screws or other devices into a vertebral joint to join various portions of a vertebra to a corresponding portion on an adjacent vertebra.

Fusion may occur in the lumbar, thoracic or cervical spine region of a patient. Fusion requires tools for accessing the vertebrae and implanting the desired implant, any bioactive material, etc. Such procedures often require introduction of additional tools and/or instruments, including drills, drill guides, debridement tools, irrigation devices, vises, clamps, cannulae, retractors, distracters, cutting tools, cutting guides and other insertion/retraction tools and instruments. The insertion, alignment and placement of these tools, instruments and fixation devices are critical to the success of the operation. As such, providing a customized and patient-specific tool or instrument increases the likelihood that the surgical procedure will be successful.

For example, one particular apparatus formed by the system and method described above and that may be used for a particular fixation related surgery is depicted in Figures 3 and 4. According to one embodiment of the present disclosure, the apparatus may be in the form of a pedicle screw guide **10**, which is comprised of a medial body **12** and two generally elongated wings **14**, each wing **14** terminating in a generally cylindrical column

16. In a preferred embodiment each of the cylindrical columns 16 is substantially hollow to permit one or more types of devices to be inserted therethrough, as depicted in Figure 3. The medial body 12 further comprises a longitudinal cavity 20 formed about a lower surface of the medial body 12 (shown from the perspective view taken in Figure 3). Each
5 of the cylindrical columns 16 further comprise a lower, patient-contacting surface 18, 19, which in conjunction with the longitudinal cavity 20 provide a plurality of patient-specific contours for matching with a plurality of anatomical features, as described in greater detail below.

The contours and locations of the lower, patient-contacting surfaces 18, 19 and the
10 longitudinal cavity 20 are formed by use of data set(s) converted from a MRI or CT scan of the patient. The remainder of the pedicle screw guide 10 shown in Figures 3 and 4 may be formed to meet the surgeon's particular preferences. For example, the wings 14 need only be of sufficiently length to locate the two cylindrical columns 16 in the location of the corresponding patient-matched anatomical features. The wings may take on other
15 shapes, orientations, thicknesses, etc. without deviating from the novel aspects of this disclosure. Similarly, the medial body 12 need only be sized to accommodate the longitudinal cavity 20, and may comprise other extensions other than the wings 14 to aid in grasping or manipulating the pedicle screw guide 10 as desired.

Additionally, the wings 14 may be made from a semi-malleable or semi-rigid
20 material to create at least a partial interference fit when the pedicle screw guide 10 is placed on the corresponding anatomical grouping for the particular surgery. For example, a snap or interference fit may be formed by subtle deflection of the wings 14 when placing the two cylindrical columns 16 adjacent the inferior articular process, and then deflect to the desired location once the wings are positioned in their final orientation. Further
25 aspects of the disclosure in this respect are described in greater detail below.

Figure 5 is a plan view of the apparatus shown in Figure 3 relative to a unique grouping of anatomical features according to one embodiment of the present disclosure. Here, the pedicle screw guide 10 is positioned so that the medial body 12 is centrally located above the central portion of a vertebral body 4, such that the longitudinal cavity 20
30 mates with the contours of the spinous process 41 for this particular vertebral body 4. Similarly, the cylindrical columns 16 are positioned one at each medial side of the pedicle screw guide 10 so that the wings 14 span the lamina 43 of the vertebral body 4 and the cylindrical columns 16 are located proximate to the inferior articular process 44, 45. The

lower, patient-contacting surface **18, 19** of cylindrical columns **16** are formed to mate with the contours of the inferior articular process **44, 45** and behind the superior articular process **42**.

Thus, the pedicle screw guide **10** provides a plurality of mating or matching
5 locations, any one of which, if not positioned correctly, will impact the seating of the other two. In this aspect the pedicle screw guide provides a notable improvement over the prior art, which may be slightly rotated, misaligned or misplaced and still appear to the surgeon as if the device is properly seated. The redundancy and plurality of mating surfaces ensures that the pedicle screw guide **10** is both properly located and properly aligned. If
10 the pedicle screw guide **10** is not properly located or aligned, the lower, patient-contacting surfaces **18, 19** will not fit on each of the inferior articular processes **44, 45** and thereby prevent the longitudinal cavity **20** from being firmly seated on the spinous process **41**.

Figure 6 is a perspective view of the apparatus shown in Figure 5. Desired insertion trajectory lines **A, B** are shown to demonstrate that the locating of the cylindrical
15 columns **16** is in addition to the orientation of the axes for each of the cylindrical columns **16**, which may be independent relative to their seating adjacent the inferior articular process **44, 45** (i.e., the direction of the axis relative to normal may be different among the cylindrical columns **16**). The orientation of the cylindrical columns **16** is also derived from the data set(s) described above, and in one preferred embodiment is selected based on the
20 orientation that will permit a fixation device (i.e., pedicle screw) to be inserted consistent with the location of the pedicle and in a direction that avoids penetration of the fixation device from the pedicle (i.e., eliminates the possibility of the screw either extending through the pedicle or becoming inserted at an angle that causes the pedicle screw to exit the side of the pedicle).

The customized or configured patient-contacting surfaces of the apparatus shown
25 in Figures 3-6 are demonstrated by the bottom perspective view of the pedicle screw guide **10** in Figure 7. Here, the lower, patient-contacting surfaces **18, 19** may comprise dynamic contours having multiple compound radii, such that the surfaces **18, 19** are completely congruent with the corresponding anatomical features of the vertebrae. Thus, the surfaces
30 conform substantially to the surface of the vertebrae where the cylindrical columns **16** are to be located during the surgical procedure, and would not conform substantially to a different surface of the vertebrae. In this manner, the surgeon is informed immediately if the pedicle screw guide **10** is misaligned, because it will not properly seat on the vertebrae.

Figure 8 shows an apparatus according to an alternative embodiment of the present disclosure. In this embodiment, a multi-level pedicle screw guide **10'** is shown relative to several adjoining vertebral bodies **4, 6, 8**. The multi-level pedicle screw guide **10'** comprises multiple secondary wings **14'** and tertiary wings **14''**, which each have
5 corresponding cylindrical columns **16', 16''** for inserting and aligning a plurality of pedicle screws into the adjoining vertebral sections **6, 8**. It is expressly understood that multiple levels in number greater than or less than three may be achieved without departing from the spirit of the present invention.

Figure 9 shows an apparatus according to yet another alternative embodiment of
10 the present disclosure, which is comprised of multiple sections **12'', 12''', 12''''**. Similar to the embodiment shown in Figure 8, this pedicle screw guide **10''** permits alignment and insertion of pedicle screws in multiple levels **4, 6, 8** of the spine. However, the multiple sections **12'', 12''', 12''''** each have a modified medial body that comprises an engaging end and a receiving end, such that the multiple sections **12'', 12''', 12''''** may be joined as
15 shown in Figure 9. The receiving and engaging ends of each of the multiple sections **12'', 12''', 12''''** are different so that when assembled, only the proper ordering of the sections **12'', 12''', 12''''** may be achieved (i.e., section **12''** may only be joined with section **12'''**). This figure demonstrates yet another aspect of the present disclosure, in particular, the ability to mate or join specific devices adjacent to one another to further ensure alignment
20 and mating with the particular anatomical features associated with each device, as well as provide a means for applying corrective force to the vertebrae and visualize the degree of deformity correction.

Figure 10 shows an apparatus according to the embodiment of Figure 5 with a customized instrument, which may be used in concert with the apparatus during a
25 particular surgical procedure. For example, during a spinal fusion procedure such as the one described above, it is common for the surgeon to attach one or more pedicle screws to the vertebrae of the patient to achieve the desired fusion of intra-vertebral bodies. The cylindrical column **16** may have a internal diameter that corresponds with a gradually increasing external diameter of the instrument **60** such that the instrument **60** may only be
30 advanced into the cylindrical column **16** to a predetermined distance, thereby providing a hard stop and in turn providing means for preventing the pedicle screw **62** from advancing too far into the boney anatomy of the patient. According to yet another embodiment, the hollow portion of the cylindrical column **16** may have a section with a narrower internal

diameter (not shown in Figure 10), which corresponds to a end-stop fitted to the external diameter of the instrument **60** in a manner and location to prevent the instrument from over penetrating the cylindrical column **16** and thereby inserting the pedicle screw **62** beyond a safe limit.

5 Figure 11 is a perspective view of an apparatus according to yet another alternative embodiment of the present disclosure. Here, the apparatus is a pedicle screw guide **100** which further comprises a narrow bridge **112** about the medial body, which permits a collar **130** to be coupled with the modified pedicle screw guide **100**, as shown in Figure 12. The collar **130** may comprise a contoured lower surface matching the spinous process
10 of the patient (similar to the longitudinal cavity of the embodiment shown in Figure 3), and may be inserted into the pedicle screw guide **100** for matching the particular anatomical feature for the vertebrae operated on during the surgery. Thus, in this embodiment, the collar **130**, in addition to the lower patient-contacting surfaces **118**, **119** of the two cylindrical columns **116**, comprises at least one of the patient-matching
15 contours, and may be removed and replaced with other collars of differing contour as required for surgical procedures on different vertebrae. In this embodiment, the cylindrical columns **116** may further comprise one or more apertures **111** to facilitate visualization of the pedicle screw while it is being advanced into the cylindrical columns **116**.

 Figure 13 is a perspective view of an apparatus for facilitating a surgical procedure
20 according to yet another alternative embodiment of the present disclosure. In this embodiment, the apparatus formed by the system and method described above is comprised of a laminectomy cutting guide **150**. This laminectomy cutting guide further comprises at least one alignment channel **151** for inserting a guide wire or other securing element, and a cutting slot **152** for directing the path of a blade or other cutting edge. As
25 with the pedicle screw guide described in Figure 3 above, this laminectomy cutting guide **150** also comprises a lower patient-contacting surface **155** which permits the laminectomy cutting guide **150** to mate with one or more vertebral bodies. Although shown in Figure 13 as a generally rectangular prism, it is expressly understood that other geometrical shapes for the laminectomy cutting guide **150** are equally as practical, and considered within the
30 scope of the disclosure.

 Figure 14 shows yet another alternative embodiment of the present disclosure. In this embodiment the apparatus formed by the system and method described above is comprised of a tube retractor **160**, which also comprises a lower patient-contacting surface

165. This patient-contacting surface **165** may be formed in a section **164** of the tube retractor that is selectively removable from the cylindrical body **163** of the tube retractor **165**, such that the tube retractor **165** may be reused in a number of surgeries while the section **164** is reformed and coupled to the cylindrical body **163** for each patient. The tube retractor also comprises a generally hollow inner lumen **162** and at least one tab **161** for manipulating during insertion and that assists the surgeon in ensuring proper alignment of the tube retractor **160**.

Figures 15-17 demonstrate yet another alternative embodiment of the present disclosure. In this embodiment, the template may comprise a patient-matched guide **180** for facilitating the placement of one or more interbody devices, such as by way of example but not limitation, an implantable cage for introducing one or more bioactive substances or bone graft, or an artificial disc. In Figure 15 and 16, the patient-matched guide **180** is shown in one potential location relative to a unique anatomical grouping (between two adjacent vertebrae) for assisting the surgeon for placing one or more interbody devices.

In Figure 17, the patient-matched guide **180** is shown in an exploded view to demonstrate how a plurality of components may be fabricated using the system and method described above for a particular surgical procedure. These components include a patient-specific insert **182**, a guide sleeve **184** and connectors **186**, which in a finally assembled state form the patient-matched guide **180** shown in Figure 15.

Referring now in detail to Figures 18-19, another alternative embodiment of the present disclosure is shown. According to this embodiment, a surgical template **190** is depicted, which may further incorporate a plurality of fixation devices **198, 198'**, which may be used to secure the template **190** in a variety of different ways. According to this embodiment, the template **190** comprises an intermediate section **192** oriented to bridge a patient's Spinous Process, and may further comprise apertures (not shown in Figs. 18-19) for inserting one or more fixation devices **198, 198'**. The template **190** may further comprise two laterally extending portions or "wings" **194** which each terminate with a guide **196**. The description of the guides provided above in connection with other embodiments disclosed herein is hereby incorporated by reference with respect to this embodiment.

According to the embodiment shown in Figures 18-19, fixation devices **198, 198'** may be inserted through apertures (not shown) in the intermediate section **192** of the template **190** for stabilizing and securing the template **190** to the patient's Spinous Process.

According to one embodiment, the direction and orientation of a first fixation device **198** is different than the orientation and direction of a second fixation device **198'** to further improve the stability of the template **190** prior to insertion and placement of the permanent fixation devices. According to yet another embodiment, the apertures may be located in
5 different locations than depicted in Figures 18-19, and may be fewer or greater in number according to the demands of the surgery and the patient's specific boney anatomy.

Referring now in detail to Figures 20-21, yet another alternative embodiment of the present disclosure is shown. In this embodiment, the template **200** further comprises two additional contacting surfaces **205** which preferably have a hollow opening at the patient-
10 contacting end and an aperture extending therethrough for inserting a fixation device **199**, **199'**. As described above in connection with Figures 18-19, the purpose of the fixation devices **199**, **199'** is for securing the template **200** to the boney anatomy and facilitate securing permanent fixation devices (not shown) through a plurality of guides **206**.

Referring to Figure 20, the template **200** includes a boss **208** extending from a top
15 surface of the template **200** for inserting a first fixation device **199**, wherein the boss **208** is partially hollow to accommodate the shape and length of the fixation device **199**. The boss **208** extends above a laterally extending portion or "wing" **204** of the template **200** as shown in Figure 20. The boss **208** may extend more or less above the template than shown in Figure 20 to provide a hard stop against over insertion of fixation device **199**.
20 Similarly, the opposite laterally extending portion or "wing" of the template **200** also comprises a boss **208'** for inserting a second fixation device **199'**.

Incorporating the disclosure above with respect to determining and modeling patient contacting surfaces, according to this embodiment the template **200** has at least four patient-specific contacting surfaces **205**, **207**. This embodiment improves stability
25 and positioning of the template, and allows a surgeon to achieve a dynamically stable surgical template, which in turn ensures that all permanent fixation devices are being positioned and inserted in a direction and orientation pre-determined for the particular surgical demands. This is accomplished by providing the four patient contacting surfaces, which act like independent legs of a table, and being positioned at different locations (and
30 at different planes) with respect to the patient's boney anatomy to further improve the stability and positioning of the template **200**.

According to the embodiment shown in Figures 18-21, the guides and other patient contacting surfaces may be depth-specific, and may further incorporate specific internal

diameters to accommodate insertion of a temporary fixation device to a controlled depth within the patient's boney anatomy. Furthermore, the guides may have specific threaded internal surfaces to accommodate a specific fixation device and to facilitate insertion of a threaded fixation device, such as a screw. In certain embodiments, the templates could be designed for a specific patient to prevent excessive penetration of the fixation devices into the boney anatomy, or facilitate a depth-controlled first set of fixation devices to temporarily secure the templates.

According to yet another embodiment, each of the patient contacting surfaces may have an integrated blade with a patient-contacting cutting surface, integrated about at least a portion of the patient contacting surface to further set and secure the template to the boney anatomy prior to insertion of the fixation devices. The purpose of the blade is to cut through the soft tissue to achieve better template to bone contact between the template and the patient's boney anatomy. The hollow portions of the guides and other patient contacting surfaces of the template further permit soft tissue to become positioned within these hollow surfaces after the template has been set in the desired location, further securing the template to the patient's boney anatomy. The blade may be substantially cylindrical or ring shaped to match the shape of the guide, or may be oval, polygon, or other shape to match a patient contacting surface.

To add further stability to the seating and placement of the patient contacting surfaces described herein to the patient anatomy, the contacting surfaces may further comprise one or more spikes or teeth, which serve to contact and at least partially penetrate the patient anatomy to secure the device in place. In one embodiment, the spikes or teeth may be made of the same material and may be permanently attached to the patient contacting surfaces. In another embodiment, the spikes or teeth may be made of a different material, such as the ones described herein, and may further be selectively inserted onto one or more of the patient contacting surfaces as desired.

Referring now to Figure 22, yet another alternative embodiment of the present disclosure is shown. According to this embodiment, the template **220** has a plurality of patient contacting surfaces **212**, **219**, which are achieved through the use of a "floating" patient-matched component **214**, which may inserted into one of a plurality of guides **216** either before or after the first set of patient contacting surfaces **212** are positioned. The patient-matched component **214** may further comprise a longitudinal key **218** which corresponds to a slot or groove (not shown in Figure 22) in the guide **216** for facilitating

proper location (rotationally) of the patient-matched component **214** respective of the template **220**.

Thus, according to this embodiment, the template **220** may be secured in a first position by using at least two fixation devices (not shown) securing the template **220** to its desired location, and then a plurality of patient-matched components **214** may be inserted
5 into the guides **216** of the template **220** and seated about two distinct locations of the patient's boney anatomy.

Referring now to Figure 23, yet another embodiment of the present disclosure is shown, wherein a instrument **240** may be used to facilitate insertion of a template **230**
10 according to various embodiments disclosed herein. The instrument **240** is preferably comprised of a handle **242** and an extending arm **244**, the length of which may vary depending on the specific patient's anatomical features and/or surgeon preferences. At the distal end of the extending arm **244** is a tab **246**, which is formed to match a corresponding slot **236** located on one surface of the template **230**. In operation, the instrument **240** may
15 be joined with the template **230** and used to insert and position the template **230** within the patient's surgical site.

Referring now to Figure 24, another alternative embodiment of the present disclosure is shown. According to this embodiment, a template **250** may be provided which is not patient-specific (but in an alternate embodiment, may be patient-specific) and
20 further provides means of attaching a plurality of patient-specific components **254** to the template **250**. As shown in Figure 24, the components **254** may be secured to the template **250** by aligning apertures **252**, **258** and attaching one or more securing devices (not shown in Figure 24) such as a screw, pin, or other like device. Once the components **254** are secured to the template **250**, the patient contacting surfaces **262** may be used to guide and
25 position the template **250** with the integrated components **254** in the desired location. In this manner, a standard template **250** may be provided prior to obtaining any patient data, and combined with patient-specific components **254** that are formed after the patient anatomical data has been captured, thereby eliminating custom machining or fabrication of the template for a specific surgical application.

According to this embodiment the template **250** may be reusable, or in an
30 alternative embodiment may be disposable. The template **250** may be comprised of any of the materials listed herein, but in a preferred embodiment is formed of a metal, metal alloy or a polymeric-based material. According to yet another alternative embodiment, the

components **254** may snap into place or have a friction-fit connection and therefore do not require screws or other securing devices to attach to the template **250**. In yet another alternative embodiment, the template **250** may be provided in a variety of set sizes and orientations to cover variability in patient anatomy and different size vertebral bodies
5 (with respect to different levels or regions of the patient's spine).

Referring now in detail to Figure 25, another embodiment of the present disclosure is shown. In this embodiment, the template **270** has a plurality of patient contacting surfaces **276**, **278** and further comprises a plurality of clamps **272** for securing the template **270** to the Spinous Process of the patient. According to this embodiment, the
10 clamps **272** each have a patient contacting surface **274** (here designed to contact the Spinous Process about each lateral side) to secure the template to the desired location of the patient's anatomy. Each of the clamps **272** may be positioned laterally with respect to the template **270** (shown in an elevation view) and affixed to a set position with respect to the body of the template **270**. The clamps **272** may be secured in a fixed position against
15 the Spinous Process by a number of known means, including a latch mechanism, a ratcheting mechanism, a direction-specific resistance mechanism, or a selectively-releasable tightening mechanism. In this embodiment, the clamps **272** allow oppositional forces occurring in the boney anatomy to become balanced relative to the patient's template **270**. In turn, the clamping mechanism ensures and maintains the alignment of
20 the template **270** relative to the boney surfaces further ensuring accuracy with respect to insertion of permanent fixation devices. The clamps can take a variety of shapes or embodiments including pins, paddles, or any other type of opposing surfaces that apply juxtapositional stabilizing forces.

According to one embodiment, the surgical guides depicted in Figs. 24 and 25 may
25 include surfaces about the patient contacting end of the guide sleeves (see **254**, Figure 24) to conform to the soft tissue existing at the facet complex where the patient contacting end of the guide sleeve contacts the patient's vertebrae (see **278**, Figure 25). Thus, according to this embodiment, the generally cylindrical guide sleeve(s) comprise a patient contacting surface that resembles a half cylinder or partial cylinder (as shown in Figures 24 and 25)
30 to avoid contact with this soft tissue.

In one alternate embodiment, the surgical guide may further comprise one or more portions that have been cut-out or may selectively be cut-out or broken off to facilitate placement. One such surgical guide is shown in Figs. 26A and 26B. According to this

embodiment, the surgical guide comprises a plurality of patient contacting surfaces, one or more of which has been modified to facilitate clearance of the guide as it is being placed into position (see surfaces **282** on Fig. 26A). Furthermore, a surgical guide as described herein may comprise one or more clamping elements for securing the guide in a preferred
5 location, such as the clamp **284** depicted in Figures 26A and 26B.

According to yet another embodiment, the guide sleeve(s) **254** may further permit insertion of one or more inserts **288**, as shown in Figs. 27A and 27B. These inserts **288** may be sized with external diameters for mating with the interior diameter of the guide sleeve(s) **254**, and have an interior aperture running longitudinally through the insert **288**
10 for accommodating a drill bit or tap (by way of example) of varying sizes. In practice, the insert **288** may facilitate and guide a drill bit for creating a pilot hole for further insertion of a fixation device, such as a screw. According to one embodiment, inserts **288** may further comprise one or more indicia for identifying the specific insert **288** for a particular level of a patient's spine, or other indicia indicating the direction, orientation, use or
15 purpose of said insert **288**.

Referring now to Figure 28, the inserts **288** provided with the surgical guides for mating with the guide sleeves **254** may have a varying length **L**, and may be made longer or shorter depending on the geometry of the guides, the patient's anatomy, the purpose of the insert, etc. For example, if a greater depth of a particular drill is required, the insert
20 **288** may be shorter to accommodate further penetration of the drill bit into the patient's vertebrae. Likewise, the interior aperture of the insert **288** may have varying diameter depending on the precise tool or instrument that is intended to be used with the insert (as depicted in Figs. 29A and 29B). In this manner, a surgeon may insure that he or she is using the proper tool, such as a drill or tap, with each of the inserts (which may further
25 include one or more indicia to indicate the location or specific use intended for said insert) when performing a surgical procedure. Further illustration of the principles described above see Figures 29A and 29B, which depict an insert with a 4.5 millimeter aperture diameter for placement of a tap instrument and a 1/8 inch aperture diameter for use in connection with a 1/8 inch drill bit, respectively.

Referring now to Figure 30, according to one embodiment the inserts **288** described above may also include patient-specific contacting surfaces **294**, for further matching the insert **288**, in addition to the guide sleeves **254**, with the patient-specific anatomy. This allows greater stability and positioning of the insert **288**, and the guide
30

with the insert **288** included, in the proper location. In addition, for inserts **288** used in connection with a drill bit or other vibrating or oscillating tool, these patient-matching surfaces **294** on the insert **288** would also prevent the distal end of the drill bit from "walking" or moving on the surface of the vertebral body when creating the initial pilot hole, thereby reducing the risk of incorrect trajectory of a fixation device.

According to further embodiments of the present disclosure, the patient contacting surfaces, formed by one or more protrusions extending from the main body of the surgical guide described in greater detail above (and according to several embodiments disclosed herein) may comprise a sharp or semi-sharp contacting edge for penetrating and affixing to the soft tissue surrounding the patient's anatomical feature, such as a facet joint. The contacting surfaces may, according to this embodiment, comprise recessed cavities for soft tissue incursion. These recessed cavities create edges around the outside of the legs, which could be sharp or selectively sharpened to facilitate cutting through soft tissue to rest/mate with underlying bone. This is particularly important for spinal surgical procedures where the precise location of the patient contacting surface must be within a small degree of error, and must remain permanent throughout the procedure.

Referring now in detail to Figure 31, the insert may further comprise a key or notch **296** about one surface of the generally cylindrical body of the insert, which is configured to mate with a cutout or slot **298** on the guide sleeve **254** of the device. In this manner, the proper rotation/orientation of the insert **288** is insured when guiding the insert into the hollow body of the guide sleeve **254**.

Referring now to Figures 32A-34B, further illustrations of a cutting guide (such as the one depicted in Figure 13 above), are provided. According to one embodiment, the cutting guide comprises a plurality of patient-specific contacting surfaces **302** about at least one surface of the cutting guide. The cutting guide further comprises, in a preferred embodiment, a patient-specific "track" **303** for facilitating insertion of a cutting instrument (as shown in Figures 33A-C) and controlling the depth of insertion for that instrument to prevent unnecessary cutting of the underlying surface during a particular surgical procedure by further providing one or more instrument contacting surfaces **304**. According to the embodiment shown in connection with Figures 32A-34B, the cutting guide may be provided for a laminectomy. According to other embodiments, the patient-specific guide may be fabricated for use in performing a corpectomy, a Pedicle Subtraction Osteotomy (PSO), a Smith-Peterson Osteotomy (SPO), a Vertebral Column

Resection (VCR), or an Asymmetric Osteotomy (in either the sagittal or coronal plane), among others.

5 These patient-specific cutting guides may be fabricated from patient anatomical data, and may assist in performing complex procedures with greater certainty in their outcomes. For example, certain osteotomies, specifically PSO and SPO, require a great deal of surgical skill and are often time consuming. This is due in part to the intimate relationship of the vascular and neural elements to the boney structures, which create navigational challenges for a surgeon to safely and efficiently resect the bone during one of these procedures. This is especially true from a posterior approach. By using a patient-specific guide, a surgeon may confirm positioning and alignment of the cutting trajectory and path prior to initiating the procedure, and in furtherance of the disclosure provided above in relation to Figures 32A-34B, may also provide a degree of depth control essential for avoiding contact with vascular and neural elements.

10 In one embodiment, the cutting tool associated with the cutting guide shown in Figures 32A-34B is typical of the type of tools currently used in surgical procedures today. According to another embodiment, a specialty cutting bur or tip may be included with the instrument to facilitate further control of the location and depth of the instrument, as described in further detail below. For example, as shown in Figures 33A-33C, the cutting portion of the instrument may have a track ball **308** that prevents greater insertion of the instrument into the cutting guide than required for the patient-specific procedure.

20 As shown in greater detail in Figures 34A-34B, the track ball **308** may be inserted into a first portion of the "track" **303** of the cutting guide, but not permitted to insert a second or deeper portion of the "track" of a cutting guide (through which the cutting surface is permitted to travel), thereby insuring proper depth of the cutting instrument. Further geometrical configurations other than those shown in Figures 34A-34B may be provided that allow the track ball **308** to move horizontally with respect to the top surface of the cutting guide, and in some instances laterally and downwardly into the track **303** of the cutting guide. In this embodiment, the cutting instrument would therefore be permitted to move at a certain depth about a patient's anatomy in a certain location of the "track" **303** of the cutting guide, but achieve a greater depth at yet other locations about the "track" **303** of the cutting guide. Thus, the depth permitted with respect to the instrument relative to the cutting guide may be variable about the "track" **303** of the cutting guide.

Other benefits achieved from the use of these patient-specific cutting guides include: providing means to achieve quick and controlled removal of bone; providing spatial orientation of cutting tools used during the procedure; ensuring correct orientation of cuts, both through controlled guiding of the instrument and visualization during the pre-surgical planning process; providing accurate calculation of deformity correction, prior to cutting; providing accurate bone resection, which in turn ensures deformity correction; depth controlled cutting restrictions to protect neural and vascular elements; controlled cutting vector and avoiding contact or injury to neural elements; and ability to provide approach for cuts in a posterior, anterior, posterior lateral, transforaminal or direct lateral approach.

Figure 35 is a top plan view according to yet another alternative embodiment of the present disclosure. In this embodiment, the device **310** may provide one or more patient contacting elements comprising break-away portions **314**, which allow for placement of a fixation device (such as a pedicle screw) without detaching the device from the patient's boney anatomy. The break-away lateral edged may be formed by creating slots **315** in the surfaces of the surgical guide portions of the device, which provide perforation axes for the portions **314** to be broken.

According to this embodiment, the guide sleeve may be asymmetric, which would permit two different inner diameters: one that facilitates guidance of the hand tools (i.e. drill, tap) and one that accommodates the boss or cap of the device (such as the tulip of the pedicle screw). Once the break-away portion **314** of the guide sleeve is removed, a clear view and path to the vertebra is possible and allows pedicle screw placement without removing the guidance device.

Fig. 36 is a detailed view of the device according to the embodiment shown in Figure 35. In Fig. 36, a detailed view of the slots **315** are shown, which in a preferred embodiment may be formed during the fabrication of the device **310**, but in alternate embodiments may be formed after the device has been fabricated by perforation or other techniques for creating a slot **315** about a certain surface of the guide sleeve of the device **310**.

Figs. 37-39 are additional views of the device according to the embodiment shown and described in relation to Figure 35. In Fig. 37, the asymmetrical guide sleeve is shown with the two break-away portions **314** separated from the device **310**. In Fig. 38, the

embodiment shown and described in relation to Figs. 26A-B is shown, but now having an asymmetrical guide sleeve with break-away portions **314** as described above.

Figs. 40A-D are additional perspective views of the devices described above in relation to Figs. 35-39, according to the embodiments having at least one or more break-away portions. Once removed, the break-away portions are preferably disposed by the surgeon.

Each of the embodiments described herein may be provided in a modular (i.e., single level) or a monolithic (i.e., multilevel) configuration. Thus, for ease of facilitating the description provided herein, certain embodiments have been shown in one (modular or monolithic) embodiment, but may be provided in a different (monolithic or modular) configuration without departing from the spirit of the disclosure. In various aspects, the monolithic embodiments may comprise anywhere from two to ten levels with respect to vertebral bodies, or enclose multiple locations of a patient's boney anatomy other than the spine. It is expressly understood that the embodiments described herein are for the purpose of illustrating certain embodiments of the disclosure, and are not intended to be limiting with respect to the scope of the disclosure.

According to the various embodiments described herein, a variety of fixation devices may be quickly and easily fabricated for use in a surgical or educational setting, including but not limited to pins, screws, hooks, clamps, rods, plates, spacers, wedges, implants, etc. Similarly, a variety of instruments and/or other devices may be fabricated based on patient-specific data, including but not limited to patient-matched inserters, scrapers, cutters, elevators, curettes, rongeurs, probes, screwdrivers, paddles, ratcheting mechanisms, removal and rescue tools, cannula, surgical mesh, etc.

Included among the apparatus that may be fabricated using patient-specific data and including a plurality of patient-matched surfaces are devices used as implants, including numerous implants used to restore disc space height in a patient's vertebrae. For example, a variety of patient-matched metallic, polymeric or elastomeric implants may be fabricated using the methods described herein, where certain patient contacting surfaces of the implant accurately and precisely match the anatomy of the patient. In one embodiment, the implant may be matched to an anatomic feature of a patient that has degenerated and needs to be restored. In another embodiment, the implant may be necessary to correct structural or physiological deformities present in the patient anatomy, and thereby serve to correct position or alignment of the patient anatomy. Other implants may be patient-

specific but do not serve a restorative or other structural function (i.e., a hearing aid implant casing).

The implants described herein may be manufactured via additive manufacturing. In the context of spinal implants, the implants may be used in all approaches (anterior, direct lateral, transforaminal, posterior, posterior lateral, direct lateral posterior, etc.). Specific features of the implant can address certain surgical objectives, for example restoring lordosis, restoring disc height, restoring sagittal or coronal balance, etc.

Other applications contemplated by the present disclosure include interbody fusion implants, disc space height restoration implants, implants having footprint matching, surface area maximization, shape and contour matching to endplates or other vertebral defects, and may further specify the contact surface such as the relative degree of roughness or other surface features. For example, an implant may be fabricated based on the patient anatomy which further comprises a direction-specific shape, such that the implant may fit through an access portal and into the disc space without difficulty. Alternatively, the implant may be fabricated in a manner to account for anatomic constraints both at the point of implant and through the path the implant must travel, and may further compensate for anatomical defects. In the context of a spinal implant, the implant may further specify a desired angle of lordosis or coronal defect correction, specify a patient-specific height of the implant or (desired height following disc height restoration), specify a degree of expansion permitted (for expandable implants), and may be unidirectional or multi-directional depending on the surgery and the surgeon preference.

According to one embodiment, the fabrication of a patient-matched device may be used to create patient-matched vertebral plates. By way of example but not limitation, patient data may be obtained to create matching surfaces of one or more anterior cervical or lumbar plates used for spinal reconstructive surgeries. Plates may comprise contours or surface features that match boney anatomy, including matching surfaces spanning more than one segment or vertebrae. In yet another embodiment, the patient data may be used to create specific patient-matched plates with identifiers for the location of the plate, and may further comprise custom drill holes or other alignment points specific to the patient. Other types of plates, besides those utilized in spinal surgery and described, may incorporate patient-matching features described herein without departing from the present disclosure.

Referring now to Figs. 41-44, an alternate embodiment of the present disclosure is shown. In certain procedures, there is a need for a plurality of trajectories in or near a particular surgical site. For example, a first fixation device may need to be secured in a first trajectory, and a second fixation device may also be needed to be secured in a second trajectory that is different than the first. According to this embodiment, multiple trajectories may be achieved without requiring multiple guides, and indeed may be facilitated by the customized guide or components thereof.

With reference being made to Figs. 41-44, the present embodiment may comprise a first guide sleeve **320** having a first trajectory through aperture **325**, and may further comprise a second guide sleeve **320'** having a second trajectory **D** and an insert having a third trajectory **C**. According to this embodiment, an insert may be used with a surgical guide or guide sleeve, such as the type described herein, or with the guide depicted in Figures 42-44. The insert may be generally cylindrical in shape and may be similarly sized so that it may be inserted into a guide sleeve, and preferably includes at least one tab **322**, **322'** for proper alignment with a slot (not shown in Fig. 41). The registration of the guide against the boney anatomy permits the surgeon to validate the proper positioning of the guide and thereby the customized orientation of the insert providing the orientation for placement of a fixation devices in the desired locations.

The concept for this additional embodiment includes using at least one part of the guide (when placed/attached to patient's anatomy) to create additional trajectories into the patient anatomy. By way of example but not limitation, the following aspects of the surgical guide described herein may be used to determine and create alternate trajectories without the need to create a new guide:

- The guide sleeve(s);
- The guide sleeve insert(s);
- The holder attachment area;
- The arms of the guide (i.e., via clips, holes, registration points, etc.).

Any point of reference associated with the above components may be used to determine the second or other multiple of trajectories. For example, an axis line, tangent line, intersection, radius, pre-determined marker (such as a radiographic marker), surface feature, end point or other registerable location may be used as a reference for determining the orientation of a second insert.

Similarly, any known point or geometry on the guides can be used to create another modular part that can "snap" into the guide providing a plurality of trajectories. For instance, the holder attachment area of the guide could be used to attach an "outrigger" arm that provides a different trajectory. This could also be applied to a hole through the arms of the guide, such as the fixation screw holes, into which the outrigger arm could be inserted.

Another embodiment could use the fixation screws or pedicle screws as additional spatial orienting features. The fixation screws and pedicle screws are placed in planned, specific orientations. Because the length and direction of these screws is predetermined, trajectories for adjacent levels can be based off of the orientation and features of these screws.

Alternatively, a surgeon may use the locations of the fixation screw holes in the guides to create additional trajectories, including with or without the need for a custom insert. In another alternate embodiment, the surgeon may use pedicle screws placed in a specific orientation to create additional trajectories.

Figs. 42A-B are top plan views of a guide **400** according to another alternative embodiment of the present disclosure. The guide **400** preferably comprises at least a first set of guide sleeves **410** and a second set of guide sleeves **412**. This embodiment is particularly useful for, by way of example but not limitation, sacroiliac fixation, due in part to patient-matching surface data not being ascertainable in certain areas requiring access during the procedure. More particularly, in order to reach the iliac crest bilaterally, a very wide soft tissue exposure is required, which is unduly disruptive to the normal anatomy. By using, for example, the location of the S1 pedicle screw guide, custom guide trajectories may be fabricated. The orientation of the trajectory may be determined by employing a more medial location of registration, and thereby permit access to a variety of iliac and sacral trajectories without creating a new guide or other custom fabricated instruments.

In a preferred embodiment, the guide of Figs. 42A-B is floating above and does not necessarily contact the iliac crest, which is desirable in certain patients who possess unstable or sensitive anatomy. Additional trajectories may be based on the original orientation of the guide sleeve or the guide sleeve insert. Furthermore, trajectories into

other sacral structures, such as the sacral ala, the S2 pedicle, or a trans-sacroiliac joint may also be achieved.

According to at least one embodiment, the patient-contacting end of the insert may not be patient-matching, and according to other embodiments may provide orientation as well as depth control for the fixation device to be placed through the second trajectory. While Figures 41-44 show only one different trajectory, it is expressly understood that additional trajectories may be provided with a single guide insert.

Fig. 43A is a top plan view of the guide for a three level procedure (sacroiliac plus 1 additional level), which depicts a pair of inserts having two different trajectories than a first pair of guide sleeves. Fig. 43B is a detailed plan view of the device shown in Figure 43A. More specifically, the guide sleeves **422**, **423** provided with this embodiment permits the variation of the inserts **424** used with the guide to provide a customized and unique trajectory, which is different from the general trajectory of the sleeve(s) **422**, **423** of the guide. The inserts **424** may comprise different and/or additional trajectories as those shown in Figures 43-44, or alternatively may extend outwards from the body of the guide in desired directions, which may not be coaxial to the guide sleeve(s).

This embodiment may also be used in tumor surgery or where the bone surface is not present or is altered (revisions). The guides from adjacent levels may be used to provide these additional trajectories.

Referring now to Fig. 45, two surgical drilling sleeves **432**, **434** are depicted in a side elevation view, which may be used with a surgical guide according to an alternate embodiment of the present disclosure. Drilling sleeves are generally known in the art, however, the present embodiment relates to custom drill sleeves **432**, **434** which may be placed through one or more patient-matched inserts or guide sleeves to provide contact with the boney surface at the distal end of the drilling sleeve (*see* Figure 46). While custom drill sleeves **432**, **434** may be made of any material, a preferred embodiment would have the sleeves **432**, **434** manufactured out of a metal or metal alloy that is of sufficient strength and brittleness that breaking and/or flaking of the drill sleeve material is avoided. Accordingly, the drill sleeves **432**, **434** may withstand the effects of high-speed drilling without damaging the sleeves **432**, **434** or permitting material from the sleeves to become deposited in the drilling site, as well as re-use of the drilling sleeves **432**, **434**. The sleeves **432**, **434** must also withstand the high temperatures encountered during

sterilization. Another benefit of metallic sleeves **432**, **434** is the ability to "trephine" or machine with a cutting surface to permit the distal end **435** of the guide to "bite" into the bone and provide means for fixation.

Fig. 46 is a front elevation view of a surgical guide **450**, guide sleeve **452** and drilling sleeve **432** assembly according to an alternate embodiment of the present disclosure. In this embodiment, a drilling sleeve **432** is provided which permits a gap between the intersecting boney anatomy and the sleeve **432**. Alternatively, a trephined or patient-specific edge of the sleeve may provide better contact with the underlying boney surface.

The drill sleeves placed through the patient-matched guide sleeves and into the bone at opposing, dissimilar angles provides additional fixation of the guide to the vertebra. The convergence of the drill sleeves through the insert also eliminates the need for additional fixation. It is expressly understood that more or fewer inserts and/or guide sleeves may be provided with a patient-specific guide for facilitating a drilling operation in a surgical procedure without deviating from the spirit of the present disclosure. In one embodiment the sleeves are disposable, and in other embodiments the sleeves are reusable.

Figs. 47A-D are views of an assembly tray and method of arranging patient-matched surgical devices according to one embodiment of the present disclosure. According to this embodiment, an assembly tray **460** is provided with a plurality of patient-specific devices **D**, which enhances the organization, structure and efficiency of the arrangement of devices **D** according to the preferences of the surgeon or to the particular surgery.

The assembly tray provides an arrangement that is essential to the users success in the operating room, including but not limited to the following factors:

- Number of and specific levels **Z1-Z4** of surgery (i.e., where multiple guides are to be used);
- Pedicle screw implant diameter and length selection (including optional variations);
- Navigational guide(s) corresponding to the selected implants;
- Combination of guides and/or sleeves, including in series and/or with monolithic guides provided for the particular application.

According to one embodiment, the assembly tray **460** consists of "zones" **Z1-Z5** that contain all of the necessary parts needed to operate on a specific area of in a specific level. The tray **460** is preferably organized and the devices **D** arranged in the desired location prior to the surgery, and may also arrive at the facility for sterilization immediately prior to the operation. Each "zone" on the tray may contain the guide **D**, inserts **I**, and pedicle screws **S** for, by way of example but not limitation, a particular vertebral level. Additionally, any drill sleeves, fixation screws or other accessory specific to a particular vertebral level may be included in that "zone". The tray preferably comprises unique indicia **462** for the particular surgery, which correspond to the different devices, areas, levels, etc.

The trays may come in various sizes dependent on the size of the surgery being performed (i.e. 2 level versus 3 level), and may be labeled to match zone to level of the spine (Zone 1 would be for L1) or comprise other unique indicia. For example, the zones may be color-coded and the different corresponding inserts complementary to a particular guide may be coded similarly to facilitate matching of inserts with guides for a certain area or level. In another embodiment, the components are bar coded, RFID coded or have other unique features which may be read by appropriate scanning equipment.

Furthermore, the tray provides safer packaging and orientation of the guides. This is especially important for plastic guides that, due to the delicate nature of the material and the different projections fabricated for a particular guide, may require protection during transportation or steam sterilization. The packaging is needed to ensure dimensional integrity during these critical steps.

As described above, certain embodiments of the present disclosure may be incorporated into surgical methods and apparatus for use in performing operations on the cervical spine (i.e., C1 through C7). Due to the similarities in the geometry of the vertebrae between the thoracolumbar and cervical spine, many of the concepts described above may be incorporated into a patient-matched surgical guide for use in a cervical spine procedure. However, unique characteristics of the cervical vertebrae and surrounding anatomy require consideration when orienting and placing a patient-matched cervical guide, several of which are discussed below in relation to Figures 48-63.

Referring now to Figures 48A-C, one embodiment of the present disclosure for use in a procedure performed at level C7 is shown. According to this embodiment, the cervical guide **470** comprises a plurality of patient-matched contacting surfaces in a manner that

permits a surgeon to accurately and reliably place the cervical guide in the proper position relative to the patient's boney anatomy. As shown in Figure 48A, the cervical guide of this embodiment comprises an arch or bridge section **471** in the medial body of the guide **470**, which is oriented to avoid the spinous process and be placed in contact with the vertebral
5 body (in this embodiment, at level C7). The cervical guide **470** preferably comprises a first patient-specific surface preoperatively configured to mate with a corresponding surface of a first transverse process, and a second patient-specific surface preoperatively configured to mate with a corresponding surface of a second transverse process opposite the first transverse process. The cervical guide **470** further comprises first and second legs **472**
10 having corresponding first and second ends, wherein the first and second ends provide the location of the first and second patient-specific surfaces configured to mate with corresponding portions of first and second transverse processes of the vertebra.

In one embodiment, the first and second legs **472** are substantially cylindrical as shown in Figure 48A-C, and may further be hollow to permit a sleeve to be inserted
15 therein. In one embodiment, as described in greater detail above, the sleeve may comprise a distal end having a patient-specific surface which mates with corresponding anatomical features of the patient after the sleeve is inserted through the hollow portion of the first or second legs **472**. In certain embodiments, the sleeve and the legs **472** comprise patient-specific surfaces. In another embodiment, only one of the sleeve and the legs **472**
20 comprise patient-specific surfaces.

The sleeves may comprise an aperture for inserting a device or instrument or tool, such as a screw, K-wire, or drill. In certain embodiments, the guide **470** is oriented to permit insertion of a sleeve configured to receive one of a pedicle screw, a lateral mass screw, a cortical screw or a facet screw. The screws and other devices contemplated for
25 use with the guide of the present disclosure may be standard or may be customized for use only with a particular guide or at a particular level.

As shown in Figure 48B, the guide may further comprise a first and second extension **474** on the first and second legs **472**, which may comprise an auxiliary aperture and path for inserting, for example, a fixation screw. According to this embodiment, the
30 extension **474** may receive a fixation screw for insertion through the aperture of the extension and into the transverse process for securing the cervical guide **470** to the patient's boney anatomy. It is expressly understood that other types of devices may be

utilized to temporarily ensure seating of the cervical guide to the patient without departing from the novelty of the disclosure as discussed herein.

Referring now to Figure 48C, a top plan view of the cervical guide described in relation to Figures 48A-B is shown. The arch or bridge **471** is shown avoiding the spinous process, although in alternate embodiments the lower surface of the bridge **471** may further comprise a patient-specific surface for mating with a corresponding surface of the spinous process. Examples of this embodiment are described below in relation to Figure 54A. The cervical guide **470** may further comprise indicia relating to the patient, the particular guide, the location or level of the spine where the guide is to be used, the size of the device or instrument or tool to be received by the particular guide, the orientation of the guide, etc. Several examples of indicia are depicted in Figures 48A-C. The cervical guide **470** may also comprise a slot, channel, groove or keyhole for receiving the distal end of an instrument, such as an inserter.

Referring now to Figures 49A-C, another embodiment of the present disclosure is shown, which relates to a cervical guide for use at level C2. This particular level of the cervical spine requires orientation of the bridge **491**, legs **492** and sleeves described above in relation to Figures 48A-C. In particular, the first and second legs **492** are oriented with a slightly upward trajectory for placement of a device, instrument or tool therethrough, which is ideally oriented for contacting the pedicle of the vertebrae. Although this embodiment is depicted without an extension for receiving a fixation screw or other device for temporarily seating the guide **490**, it is contemplated that such an extension may be provided with the cervical guide for level C2. Other levels besides C7 and C2, as described in relation to Figures 48-49, are also contemplated for applications of the present disclosure.

Referring now to Figures 50A-D, another embodiment of the present disclosure is shown. This particular cervical guide **500** includes sleeves **510** oriented to receive inserts (not shown) for receiving, for example, lateral mass screws. The particular guide shown is designed for application with level C5 of the cervical spine. As shown best in Figure 50C, the bridge **502** includes a slot **503** for receiving the distal end of an instrument, such as an inserter. In another embodiment, the slotted portion of the bridge **502** may include a connection for joining two separated portions of the cervical guide in a medial area. Further details regarding this particular embodiment are described in relation to Figures 53A-E. In addition to the patient-specific legs shown in Figures 50C-D, this embodiment

further comprises a first and second tab **520** for placement under the laminar surface of the vertebrae. The tabs **520** assist in securing the cervical guide to the patient-specific anatomy, and are described in the following paragraph in further detail.

Referring to Figures 51A-C, additional views of the embodiment depicted in
5 Figures 50A-D are shown. According to this embodiment, the tabs **520** are oriented to separate the facet joint capsule and enter the facet joint when the cervical guide **500** is placed into position. One or both sides of the tabs **520** may be patient-matching. The patient-matching tabs **520** may enter the facet joint above or below, or in certain embodiments provide both. In this embodiment shown, the tabs **520** create an interference
10 fit with the facet joint and secure the cervical guide in place. The tabs **520** may be made of material suitable for flexing to permit the interference fit described above, which may be the same or a different material than the remainder of the surgical guide. The tabs **520** may also be made of a non-flexible material, utilizing the guide material's flexibility to permit the interference fit described above.

Referring now to Figures 52A-C, an embodiment of the present disclosure is
15 shown that depicts a slotted bridge **502**, which further comprises an aperture **504** for receiving a device, such as a fixation screw, which in this embodiment is placed into the spinous process. In one embodiment, the aperture **504** is threaded, and in another embodiment (as depicted in Figure 55B) it is not. The aperture **504** may further comprise a
20 specific trajectory, for example by orienting the fixation screw shown in Figures 52A-C in a more upward direction as desired for securing the cervical guide to a particular level of the cervical spine. The embodiment shown in Figures 52A-C may also be incorporated into an embodiment comprising a patient-specific surface located on the lower surface of the bridge **502** for mating with a corresponding surface of the spinous process, such as the
25 embodiment described in relation to Figure 54A.

According to one alternate embodiment, the cervical guide described above may further comprise means for locking. Referring to Figures 53A-E, such an embodiment may comprise means for locking a first section **525** of a guide to a second section **527** of a guide, and further comprise a first collar section **526** and a second collar section **528**
30 oriented to mate with each other about a particular anatomical feature, such as the spinous process. The first and second section **525**, **527** and first collar section **526** and second collar section **528** may be joined by suitable techniques known in the art, including but not limited to by inserting one or more tabs into complementary slots on the adjoining

surfaces as shown in Figures 53A-C. In this manner, the joining of the first and second sections **525**, **527** may permit an interference fit by first placing the first and second legs of the cervical guide in position, and then joining the first and second sections **525**, **527** of the guide. The interference fit is caused by the tension in the first and second section **525**, **527** of the guide being joined while the first and second legs (and the corresponding first and second patient-specific surfaces) remain positioned against the patient's boney anatomy. In addition to, or instead of, an interference fit, one or more pins and/or screws may be passed between the first and second sections **525**, **527** of the guide in order to join them into a rigid assembly. These pins and/or screws may additionally pierce the spinous process, or any other part of the vertebral anatomy, in order to stabilize and fix the guide assembly to the bone. While the first and second collar sections **526**, **528** shown in the Figures do not have patient-specific surfaces, it is expressly understood that including this feature is within the scope of the present disclosure.

As referenced above, the cervical guides may further comprise a patient-specific surface on a lower portion of the bridge for mating with the spinous process, as depicted in Figures 54A-C. The patient-specific surface may be substantially concave for receiving a complementary convex surface of the spinous process located below the location of the bridge. The cervical guide in certain embodiments may also comprise a slot, channel, groove or keyhole for receiving the distal end of an instrument, such as an inserter. An exemplary inserter is depicted mating with a slotted portion of the cervical guide in Figures 54B-C. As best seen from Figure 54C, the distal end of the inserter may comprise two tines, whereby one of the tines may be received within the slot located on the bridge of the guide and the other tine placed on the lateral side of the bridge. The insertion instrument may also be rotated 180 degrees to permit the second tine to be placed against the opposite lateral side of the bridge. In certain embodiments, the tines may comprise an interior surface that includes texturing or a plurality of small barbs for gripping into one or more the surfaces of the bridge, or to contact and become joined with complementary dimples in the surfaces of the bridge (which are not shown in Figure 54C).

According to yet another embodiment, the cervical guide may further comprise one or more apertures for placement of a clamp, such as the type shown in Figures 55A-C. The clamp **540** may be secured and tightened by providing a threaded aperture and a corresponding threaded post of the clamp **540**, or may have a threaded post and a corresponding nut to lock the clamp **540** into the proper position. As shown in Figure 55B,

the clamp **540** may be positioned against an anatomical surface of the vertebrae and then tightened into a secured position by way of the threaded post and threaded aperture or nut, as is the case in the embodiment shown in Figure 55C. More than one clamp **540** may be provided to improve the act of securing the cervical guide. In this same manner, one or
5 more tabs or hooks may be provided with the cervical guide to secure the guide to the patient's boney anatomy, as shown in Figures 59A-B. In practice, the clamp **540** or hook may first be placed in the desired location and position, and then the guide lowered so that the post of the clamp **540** or hook enters the corresponding aperture on the guide. Once the post is positioned through the aperture (as shown in Figures 55C and 56C-D), a nut may
10 be threadably connected to the threaded post and tightened to secure the cervical guide against the patient's anatomy.

As described above with thoracolumbar guides, the cervical guides described herein may provide axial or alternatively off-axis trajectories into the patient-specific anatomy. Such an off-axis trajectory may be provided with a sleeve **550** as described
15 above and now shown in Figure 57. The trajectory may be determined from the use of scanning equipment described above, and selected based on optimal patient anatomy, bone density, etc. The off-axis trajectory may be particularly important in areas of the cervical spine, where the generally smaller vertebrae do not permit the legs or corresponding sleeves to be positioned such that the desired axis of a device, instrument or tool to be
20 used with the guide may be achieved in a co-axial relationship. By providing off-axis trajectories, the guide may serve to secure a device or permit the insertion of a tool or instrument in a direction that could not otherwise be achieved.

The embodiment of the present disclosure depicted in Figures 58A-C comprises a patient-specific guide calibration model. The model provides a user with both a visual and
25 tactile representation of the patient anatomy for creating a patient-specific guide, including one or more predetermined screw trajectories. The modeling of predetermined screw trajectories assists in the orientation and placement of patient-matched surfaces and direction of the components of the guide (i.e., legs, sleeves, inserts, etc.). By using the model, a user may also create a non-patient-specific guide that is adjustable and reusable.
30 One example of this could be a surgical guide with hinges, ratchets, swivels, pivots, set screws, etc., that when adjusted or tuned "click" into place and can be locked once the user has finished their adjustments. Then, guide sleeves could be placed over the protruding pegs **560** (as shown in Figs. 58A-C) to provide the desired drill/tap/screw trajectory, while

the rest of the guide could be configured at the user's discretion or to achieve optimal fit with the patient-specific anatomy.

Figs. 59A-D show another embodiment of a surgical device, which preferably may be use with a procedure involving a patient's cervical spine. According to this
5 embodiment, the device comprises a plurality of sleeves **572** and one or more of the plurality of sleeves **572** may receive a selectively removable clip, for example the clip **574** shown in Figs. 59C-D. In one embodiment, the selectively removable clips **574** are received by placing a post **573** associated with a clip **574** into a slot **571** in the body of sleeve, as shown in Fig. 59A. This receiving may be a frictional fit, but more preferably is
10 a snapping or latching attachment that prevents undesired removal of the clip **574** once the device has been placed against the patient's anatomy. Other connections within the ordinary skill of those familiar with the art are also contemplated for use with this embodiment.

Figs. 60A-C include additional views of a device described in the preceding
15 paragraph. Fig. 60A is a side elevation view of the device with at least one clip **574** engaged to the body of the sleeve of the device and further engaged to the underside of an adjacent boney structure. Here, the boney structure is a lamina of a cervical vertebrae, although the clips are contemplated for use with other anatomical features as well. Fig. 60B shows the device with two clips **574'**, similar to the clips **574'** shown in Fig. 59D.
20 Fig. 60C shows details regarding the connection between the clips and the sleeves of the device according to one particular embodiment.

Figs. 61A-C show yet another embodiment of a guide and associated clips. Here, the clips **575** are preferably spring clips, and are normally biased away from the body of sleeve at the distal end of clips as best seen in Fig. 61A. The connection between clips **575**
25 and sleeves of guide are such that the clips **575** may be depressed against or closer to the body of sleeves, with the normally biasing associated with clips causing resistance to the same. Once depressed, the clips **575** may be inserted beneath adjacent anatomical features as shown in Figs. 61B-C. In this embodiment, the clips **575** may be oriented so as not to cause unwanted damage to the associated patient anatomy, here, the superior facet joint of
30 a patient's vertebrae. By placing the distal end of the clip **575** in the superior facet complex, the clip **575** may be wedged between the boney anatomy without penetrating the anatomy and otherwise causing damage to the patient. Although the attachment between clips **575** and sleeves is depicted as being a permanent attachment, it is contemplated that

the clips **575** of Figs. 61A-C may be selectively removable as described in the embodiment of Figs. 59 and 60.

Figs. 62A-E show views of yet another embodiment of the device of Figs. 59-61. According to this embodiment, the clips **575** may be selectively coupled to a rigid connector **576** for adjustment relative to the body of the device. According to a preferred embodiment, the adjustment is made by a threaded post **577** inserted into a corresponding threaded bore on a surface of the device, as best shown in Figs. 62A-B. The positioning of threaded post **577** relative to the device preferably causes rotation of cam elements, which in turn provide secure points of contact about surfaces of the patient's anatomy.

The adjustment of threaded post **577** may also permit a user to selectively engage and disengage distal ends of clips **575** from a patient's anatomical feature. In one embodiment, this adjustment is caused by post **577** and rigid connector **576** to distract clips **575** away from the body of device, as best shown in Figs. 62B and 62D. Rigid connector **576** may be coupled to each of the plurality of clips **575** as shown in Figs. 62A-E, which preferably comprises cam elements **580** located at the distal end of each clip. Other connections and orientations of rigid connector **576** are contemplated for use with this embodiment.

Clips described above may be tapered or pointed such that the distal ends of clips contact and penetrate a boney surface of the patient's anatomy. In other embodiments, the clips may further comprise a textured or machined surface, which engages the patient's anatomy and creates a frictional engagement therewith. Other surface variations and geometries may be incorporated into the design of clips for improving the connection to the patient's anatomical features.

The clips are preferably not patient-specific, although they may include patient-specific surfaces is desired. The clips may also be substantially deformable to conform to the variations of patient anatomy. The clips may also be attached, either permanently or selectively, to inserts of the device as opposed to the sleeves of the device as described above.

The device in one embodiment may further permit engagement with a spacer, such as the one depicted in Figs. 63A-H. The spacer **590** may comprise one or more patient-specific surfaces as shown in Figs. 63A-B, or may be fabricated for use in a variety of different applications. In spine surgery procedures, the spacer **590** permits a device to have patient-specific surfaces about multiple levels of the patient's spine. The spacer **590** is

preferably coupled to the device as well, as best shown in Fig. 63C-E. The spacer in this embodiment provides another surface(s) for aligning the device to the desired anatomy and/or orientation of the guide elements described above.

5 The concepts described above in relation to Figures 48-63 have been described for convenience in the context of a cervical spine procedure, but are not limited to application in the cervical spine, and may be applied to thoracolumbosacral spine and ilium as well.

Referring now to Figures 64-67, various embodiments according to one aspect of the present disclosure are shown, which relate to the use of guiding wires/pins and cannulated devices, such as screws, and corresponding instruments and/or implants.
10 According to these embodiments, the surgical guides described above may further comprise a "cannulated" system wherein a K-wire or guide pin/wire is placed through one of the sleeves or inserts associated with a patient-specific guide, and any subsequent instruments and/or implants use the wire for guidance into their proper location along the longitudinal axis of the wire.

15 Referring to Figures 64-65, a guide has received instrument sleeves which each have a longitudinal channel for receiving a wire **600**, preferably through the center of each insert, which then may be used for centering other instruments and/or implants. As seen in Figure 66, the instrument sleeves may extend above the top surface of the guide, which in turn may accommodate a longer guide wire **600** and stabilize the wire **600** in the proper
20 location while it is being inserted into the patient's boney anatomy.

Next, the instrument sleeves may be removed as depicted in Figure 67. If the guide assists the surgeon in performing the surgical procedure, the surgical guide may remain. However, it is contemplated that the guide may be completely removed once the wires **600** are properly seated as shown in Figure 68.

25 Once the wires **600** are in place, one or more instruments or implants, such as cannulated screws, may be slidably received by the wires **600** and thereby placed in the proper position and trajectory. By way of further example but not limitation, a cannulated screw comprising at least one bore therethrough may be positioned on a wire **600** established by the guide depicted in Fig. 64. It is expressly understood that other implants
30 besides cannulated screws may be utilized with these embodiments, as well as a variety of instruments, including those listed above and made part of this disclosure.

Referring now in detail to Figures 69-73, a device is shown for performing MIS procedures on a vertebral body. The device is comprised of a generally cylindrical, hollow

retractor **692**, which has a first end and a second end. The retractor **692** body is hollow throughout its longitudinal axis, which makes the retractor **692** capable of receiving dilators and progressively expanding retractors as described above and further capable of receiving tools, instruments or devices therethrough, including a custom or standard
5 fabricated insert as shown in Figure 69. The first end of the retractor **692** is preferably designed to matingly receive one or more patient-specific end-pieces **694**, which are also shown in Figure 69. Retractor **692** may also comprise an attachment joint located preferably along the outer wall of the generally cylindrical body of retractor **692** for receiving a coupling device **710**.

10 Coupling device **710** preferably has a slot or groove on each end for receiving one or more attachment joints. In one embodiment, the attachment joint and slot or groove of a particular coupling device **710** are complementary and create a secure connection when joined. In certain embodiments, the connection between attachment joint and slot or
15 groove of coupling device **710** is such that a desired angle or direction of coupling device is achieved once the joint and slot or groove are mated (as seen best in Figure 72). In one embodiment, the connection is a locking connection. In another embodiment, the connection is a snap fit connection. In another embodiment, the connection is a frictional engagement between the joint and the slot or groove. For further illustration, *see* Figures 95-97.

20 Coupling device **710** may be used to secure one or more retractors **692** to one another, and in a preferred embodiment are coupled above the patient's skin surface (i.e., percutaneously). Coupling device **710** may be sized and shaped to secure a first retractor **692** and a second retractor **692** to each other in a desired position. According to yet another embodiment, the coupling device **710** may be secured to one or more retractors
25 **692** to provide a desired orientation or trajectory for related inserts. Coupling device **710** may also be used in a multi-level MIS procedure, and according to at least one embodiment, may be joined to other coupling devices in order to secure both lateral and longitudinal spacing among an array of retractors **692**.

30 Inserts **695** may be of varying shapes and sizes, and may comprise features such as those associated with inserts described above in relation to Figures 1-68. Varying views of the apparatus described above are shown in Figures 70-73, and include embodiments involving multi-level MIS applications.

Referring now to Figure 74, an embodiment is shown similar to that of Figures 69-73, except coupling device includes multiple channels, which are preferably custom fabricated through the body of coupling device **710**, and which may receive one or more alignment elements **695**. The alignment elements **695** may be fixation pins, as referred to
5 in Figure 74, and used to secure the assembly shown in Figure 74 to a particular boney anatomy. Variations on this embodiment are depicted in Figures 86A-C, which include custom fabricated channels oriented to guide alignment elements to penetrate a patient's lamina, facet, pars, spinous process, or other anatomical features. In addition, the channels may be provided in different or multiple locations, such as those shown in Figures 87A-B,
10 which provides the benefits described above without requiring a coupling element. In certain embodiments, the use of channels in the coupling element and in the body of the retractor may be combined, as shown in Figures 88A-B.

The alignment devices **695** may also comprise a first dimension and a second dimension which provide the surgeon with the ability to gauge the depth of the alignment
15 element. For example, the alignment element **695** may comprise a collar, which is thicker than a first dimension of the alignment element, to stop the penetration of the alignment element **695** into the boney anatomy.

Referring to Figure 75, another embodiment is shown wherein the assembly further comprises a bridge element **715** for joining two or more coupling elements **711**, **712**. In
20 this embodiment, the bridge element **715** and coupling elements **711**, **712** create a more stable assembly. Also shown in Figure 75, the inserts for each retractor tube shown comprise different shaped and sized openings for accommodating differing tools, instruments or devices. In this manner, the customized insert may be specific to a particular application associated with a specific retractor tube, and only receive a specific
25 tool, instrument or device.

Referring now to Figs. 76A-C, an alternative embodiment of a surgical device is shown. In this embodiment, a preferably reusable handle is comprised of a first and a second portion **732**, **734**, which may be selectively coupled to each other and to the device. This handle is preferably attached to the device in a minimally invasive surgical
30 procedure and provides both alignment and stability to the associated device(s). The handle first and section portions **732**, **734** preferably comprise an ergonomic shape for ease of grasping with a single hand of a user, and are preferably offset from the vertical axis of the device(s) to avoid interference with the user's vision during the surgical

procedure. Alternatively, the handle portions **732**, **734** may be contoured and/or angled to avoid interference with the user's vision. Although a slotted connection is shown in Figs. 76A-C, other means of connecting the handle portions **732**, **734** and the handle to the device(s) are contemplated. In particular, various connection devices described below in
5 Figs. 95-97 may be incorporated in the embodiment shown in Figs. 76A-C.

Figs. 77A-G depict another alternative embodiment of the surgical device comprising one or more optional alignment/depth/position control elements. Here, a handle includes at least a first and a second portion **732**, **734**, which may be positioned in a plurality of positions relative to one another to adjust the width of the handle. At least one
10 of the first and second portions **732**, **734** comprises indicia **744** denoting the width in known dimensions. The device of Figs. 77A-G preferably comprises at least one rotational adjustment **742**, which permits the angle of the handle to vary according to the desired orientation of one or more devices. The handle is preferably coupled to insert(s) which are placed into device(s) (not shown in Figs. 77A-G). A preferred embodiment also comprises
15 one or more depth control adjustment elements **740**, as shown in Fig. 77C. This permits translation of the "legs" of the device. The device preferably includes indicia about the legs reflecting known dimensions for ease of use when adjusting the device for a particular procedure and patient anatomy.

Figs. 78A-B depict adjustment guides **790**, **792**, which assist in achieving a desired
20 angular and/or width and/or height adjustment. The adjustment guides **790**, **792** preferably couple to the handle or legs of the device and are fixed into place when a desired position or orientation is achieved. For example, the width may be set by placing adjustment guide **790** against handle, as best shown in Fig. 78B, which prevent movement of the handle once the adjustment guide is secured in place. Similarly, an angular
25 adjustment guide **792** serves as a wedge, and prevent greater or lesser rotation of the legs relative to the handle once securely placed against the device (as shown in Fig. 78B).

Figs. 79A-B include views of a device for assisting in determining the incision and entry portal location for a particular surgical procedure. The device preferably comprises at least one reference element **802**, which may be aligned with a known anatomical
30 feature. Here, the feature is the centerline of the patient's spine and/or longitudinal axis of the spinous process. The device further comprises a height, width and angular adjustment **803**, **800**, **806**. The angular adjustment **806** is associated with at least one guide member **804**, which may be rotated or pivoted to a desired location according to the user's

preference. The guide member **804** is preferably also height adjustable, and may further comprise a distal end including a marking surface, which permits the user to mark a desired location on the patient for future reference. The marking surface may be direct contact, or may be indirect, such as with a laser or other similar optical marking device.

5 Fig. 79B depicts the device according to this embodiment in a final position, whereby the guide member is in the desired location and directed towards the underlying patient anatomy for the associated procedure. Fig. 80 is a detailed view of the device of Figs. 79A-B.

Referring now to Figures 81A-C, another example of an embodiment is provided
10 wherein the connection between attachment joint and slot or groove of coupling device **710** is such that a desired angle or direction of coupling device **710** is achieved once the joint and slot or groove are mated. Reference is again made to previously described Figures 69-75. Figures 81A-C also depict an embodiment wherein the retractors may be coupled spanning the spinous process and between different levels of a patient's spine.
15 Other variations of this embodiment for use in non-spine procedures is expressly contemplated. Furthermore, as discussed in some detail above, the retractors and coupling elements **710** and bridge elements may also comprise one or more unique indicia which provide a surgeon or other medical professional with identifying information to assure that each component of a particular assembly is assembled in the proper location and joined to
20 the proper apparatus.

In certain applications, it is desirable to provide a surgeon with an expandable retractor tube, such as the embodiment shown in Figures 82A-84E. In this embodiment, a collapsed retractor tube **820** in a first orientation is shown in Figure 82A, and is of a smaller cross-section than a retractor in a second orientation, as shown in Figure 82B. The
25 retractor of Figure 82A may be inserted through a smaller incision and mated with a patient-specific anatomical feature. After the retractor **820** is properly positioned, the retractor **820** may be expanded, such as, by way of example but not limitation, through the use of an instrument or tool provided with the retractor **820** (not shown in Figures 82A-B). Once the retractor **820** is positioned in its second position, additional instruments, tools,
30 devices or even retractors may be positioned therethrough as shown in Figure 82C. Referring to the embodiment shown in Figures 82A-D, the expandable retractor **820** may further comprise a means for attaching a patient-specific end-piece **825**, such as described above in relation to Figures 69-73.

Variations on the embodiment described in the preceding paragraph are depicted in Figures 83-84. According to these embodiments, the retractor tube is expandable by a plurality of longitudinal hinges placed along the interior circumference of the retractor tube, as best shown in Figure 84D. The hinges may be mechanical hinges or may be living hinges (i.e., formed from the material of the retractor tube). In other embodiments, variations on the hinge may be incorporated without departing from the novelty of the embodiment described herein. In certain embodiments, the retractor tube is disposable. In other embodiments, the retractor tube is reusable.

Referring now to Figure 85, inserts provided with retractor tubes described herein may further comprise a longitudinal bore of varying dimension, which in practice permits the safe and effective application of one or more surgical tools or instruments. For example, as shown in Figure 85, an insert **830** may provide a safety stop or depth control stop **832** by virtue of its geometrical configuration (*i.e.*, preventing the instrument or tool from passing beyond a certain depth within the longitudinal bore of the insert). According to another embodiment, a patient-specific end-piece **834** may provide the ability to prevent an instrument or tool from extending beyond a controlled depth.

Referring now to Figures 89A-90C, it is often desirable to provide a coupling **900** between retractors located about multiple levels of a patient's spine when performing a MIS procedure. As shown in Figures 89A-B, one embodiment of the present disclosure is to provide such a coupling **900** that further comprises a secondary location for an additional retractor tube **910**, which is located between two adjacent retractor tubes. The combination of the two adjacent retractor tubes, including their secure fixation to the patient boney anatomy, and the rigid structure provided by the coupler **900** shown in Figures 89A-B provide a well-defined reference point for insertion of an additional retractor **910** through a secondary location between the two positioned retractors. This additional retractor **910** can then be used to perform additional surgical procedures at locations between, for example, two adjacent vertebrae without requiring additional fixation of the retractor to the patient anatomy.

Referring now to Figures 91A-92D, various other embodiments are shown relating to the retractor and related elements described above. One embodiment, as shown in Figures 91A-D, provides a coupling element **920** which is adjustable. The adjustable features may include, but are not limited to, length, width, height, angle of orientation and depth. In this embodiment, no patient-specific coupling element or bridge needs to be

preconfigured, and the adjustable coupling element may be reused. In one embodiment, patient-specific data may be used to provide a surgeon with specific settings for adjusting the adjustable coupling element **920** in a desired setting for use in a particular MIS procedure. This data may be provided before the MIS procedure and included with a
5 specific surgical plan, either with or without any patient customized apparatus.

A variety of mechanical characteristics may be incorporated into the coupling device described above without departing from the spirit of the disclosure made herein. Applicant incorporates by reference U.S. Patent Publication No. 2009/0105760 in its entirety, which is co-pending and names Dr. George Frey as the sole inventor, for the
10 purpose of further supplementing the disclosure and providing additional support for various mechanical characteristics capable of being employed in the coupling device.

Another embodiment is shown in Figures 93A-D, wherein a template of a surgical tool, instrument or device is provided which may be customized or contoured to conform to a specific patient's anatomy. In certain embodiments, the template may provide a
15 surgeon with a particular dimension, shape, orientation, etc. for a device such as a rod, as shown in Figures 93A-B. In yet other embodiments, the template may be the device, such as the one shown in Figures 93C-D. .

Figs. 94A-C are various views of one embodiment of the present disclosure, which includes a plurality of patient-specific guides. The plurality of guides may receive and be
20 manipulated by an instrument, such as the inserter depicted in Fig. 54B. Alternatively, the plurality of guides may receive a plurality of elongated shafts or "indicators" to assist the user in visualizing the location, orientation, curvature and/or deformity associated with the patient's underlying anatomy. Here, the underlying anatomy is a patient's spine from T10 to L4. The indicators create a visual image of the deformity associated with these levels of
25 the patient's spine. Additionally, the indicators permit a surgeon to determine the length and orientation (including curvature) of a fixation rod or other implant for correcting the deformity or otherwise treating the patient, and may also be captured by an optical system to digitally reproduce the curvature for the purpose of determining correction, rod shape/length, or correct positioning of guides. The indicators may assist the user in other
30 aspects of the surgical procedure. For instance, Fig. 94C shows the plurality of indicators in a side elevation view, which allows the surgeon to visualize the difference in height of each level of the patient's spine and differences from one level to the next. The indicators

also allow the user to visualize whether a particular patient-specific guide is misaligned or has become dislodged.

Figs. 95A-C are side elevation views of a connector for attaching to a sleeve or an insert according to embodiments of the present disclosure. This connector comprises a threaded bore which is received by a threaded post, and is rotationally secured to the post by threaded engagement. This connection type may be used in varying manners, including but not limited to the connection between alignment devices and the surgical guide devices described herein. Figs. 96A-C show a clamping connector according to another embodiment of the present disclosure. Figs. 97A-C show a screw or pin connector according to yet another embodiment of the present disclosure. Here, the screw is inserted through a slot in a sleeve element and further inserted through a slot in the distal end of an apparatus associated with the device. For example, the apparatus may include a leg of an alignment device, such as the ones described above.

Figs. 98A-C are side perspective views of an insert and guide sleeve according to one embodiment of the present disclosure. Here, the insert comprises one reference marking, which may comprise a cut, groove, notch, scoring or other marking for aligning the insert with the desired orientation. The marking is preferably visible with both the naked eye and through fluoroscopy, and may be visible through other known scanning technologies. This embodiment is particular useful for aligning the insert for receiving a cutting or drilling instrument, or for inserting an implant therethrough.

Figs. 99A-G show various views of a system for aligning a guide according to one of the various embodiments described herein. This system further comprises an adjustable arm assembly, which may be affixed to an operating surface or alternatively to the patient. Fig. 99A shows the arm assembly in a first position away from the device(s), and Fig. 99B shows the arm assembly attached to the device(s), providing stability by resting on the patient's skin. This attachment between the device(s) and the arm assembly may permit a user to set and fix the sagittal angle of the device(s) when performing a surgical procedure on the patient's spine. Fig. 99C shows the embodiment of Figs. 99A-B in a perspective view.

Figs. 99D-E show an alternative embodiment, wherein the arm assembly comprises a telescoping member that rests on the patient's skin, which may be adjusted to a desired length and angle relative to the associated device(s). This serves to hold the handle of the device(s) in place when the user is not grasping the handle. Figs. 99F-G

depict yet another embodiment of the arm assembly, wherein the assembly is attached to an operating or side table or other horizontal surface. Each of these embodiments preferably includes a locking mechanism for securing the arm assembly components in place once the desired orientation and position has been established.

5 Figs. 100A-D are side perspective views of a percutaneous delivery device, according to one embodiment of the present disclosure. The device preferably comprises a distal end having an expandable/retractable tip. When in a first position, as shown in Fig. 100C, the device may be inserted through any of the guides and/or inserts described herein. After insertion, the device may be expanded as shown in Fig. 100D and locked in
10 an expanded position. The shaft of device may further comprise a collar for preventing insertion into the guide and/or insert beyond a desired distance.

Figs 101A-D are various views of a patient-specific guide according to yet another alternative embodiment of the present disclosure. In this embodiment, the patient contacting surfaces of the guide further comprise surface contacting elements. These
15 elements may engage soft tissue about the underlying boney surface, for example, and are beneficial for penetrating soft tissue. These elements also provide greater stability and improve haptic feedback, which in turn allow the user to determine whether the guide is in the right location. In a preferred embodiment, the contacting elements are shaped to resemble barbs or blades, although in other embodiments may have varying sharpness,
20 radius, length, and orientation.

Although the devices described above have been illustrated for use with certain guide screws and/or instruments, it is expressly understood that the devices may be used with a variety of other implantable and non-implantable apparatus, including by way of
25 example, medial-to-laterally placed transpedicular screws (commonly referred to as cortical bone trajectory screws). Other screws and instruments may be used with the surgical devices described above without departing from the spirit of the disclosure, and are considered to be within the scope of the appended claims.

While various embodiment of the present disclosure have been described in detail, it is apparent that modifications and alterations of those embodiments will occur to those
30 skilled in the art. However, it is to be expressly understood that such modifications and alterations are within the scope and spirit of the present disclosure, as set forth in the following claims. For further illustration, the information and materials supplied with the provisional and non-provisional patent applications from which this application claims

priority are expressly made a part of this disclosure and incorporated by reference herein in their entirety.

5 Additionally, although the fusion cages of the present invention are particularly well-suited for implantation into the spinal column between two target vertebrae, and although much of the discussion of the present invention is directed toward their use in spinal applications, advantages offered by embodiments of the present invention may also be realized by implantation at other locations within a patient where the fusion of two or more bony structures may be desired. As one of skill in the art will appreciate, the present invention has applications in the general field of skeletal repair and treatment, with particular application to the treatment of spinal injuries and diseases. It should be appreciated, however that the principles of the present invention can also find application in other areas.

10 It is expressly understood that where the term "patient" has been used to describe the various embodiments of the disclosure, the term should not be construed as limiting in any way. For instance, a patient could be either a human patient or an animal patient, and the apparatus and methods described herein apply equally to veterinary science as they would to surgical procedures performed on human anatomy. The apparatus and methods described herein therefore have application beyond surgical procedures used by spinal surgeons, and the concepts may be applied to other types of "patients" and procedures without departing from the spirit of the present disclosure.

20 The foregoing discussion of the disclosure has been presented for purposes of illustration and description. The foregoing is not intended to limit the disclosure to the form or forms disclosed herein. In the foregoing Detailed Description for example, various features of the disclosure are grouped together in one or more embodiments for the purpose of streamlining the disclosure. This method of disclosure is not to be interpreted as reflecting an intention that the claimed disclosure requires more features than are expressly recited in each claim. Rather, as the following claims reflect, inventive aspects lie in less than all features of a single foregoing disclosed embodiment. Thus, the following claims are hereby incorporated into this Detailed Description, with each claim standing on its own as a separate preferred embodiment of the disclosure.

30 The present inventions, in various embodiments, include components, methods, processes, systems and/or apparatuses substantially as depicted and described herein, including various embodiments, subcombinations, and subsets thereof. Those of skill in

the art will understand how to make and use the present inventions after understanding the present disclosure. The present inventions, in various embodiments, include providing devices and processes in the absence of items not depicted and/or described herein or in various embodiments hereof, including in the absence of such items as may have been
5 used in previous devices or processes, e.g., for improving performance, achieving ease and/or reducing cost of implementation.

Moreover, though the present disclosure has included description of one or more embodiments and certain variations and modifications, other variations and modifications are within the scope of the disclosure, e.g., as may be within the skill and knowledge of
10 those in the art, after understanding the present disclosure. It is intended to obtain rights which include alternative embodiments to the extent permitted, including alternate, interchangeable and/or equivalent structures, functions, ranges or steps to those claimed, whether or not such alternate, interchangeable and/or equivalent structures, functions, ranges or steps are disclosed herein, and without intending to publicly dedicate any
15 patentable subject matter.

The claims defining the invention are as follows:

1. A surgical device for use in a minimally invasive surgical procedure, comprising:

two or more guides each having a proximal and a distal end, the distal ends each comprising patient-contacting surfaces configured to anatomically mate with and are determined from corresponding subcutaneous anatomical features of a patient;

a coupling member selectively attachable to the proximal ends of a plurality of the two or more guides, thereby forming a medial portion of the surgical device;

wherein the proximal ends of the two or more guides extend outside of the patient and wherein the coupling member is configured to be selectively attached to at least a first guide and a second guide outside of the patient;

wherein the distal ends of the at least a first and second guides of the surgical device are configured to contact the corresponding subcutaneous anatomical features to ensure proper alignment and placement of the surgical device; and

wherein the two or more guides, when coupled with the coupling member, are oriented in a pre-determined direction.

2. The surgical device of claim 1, wherein the two or more guides are configured to receive a bone anchor, an implant, a drill, a rasp, a blade, a screwdriver, a curette, a retractor, a distractor, an elevator or a debridement instrument.

3. The surgical device of claim 1, wherein the two or more guides are substantially cylindrical for use as or in connection with a tubular retractor.

4. The surgical device of claim 1, wherein the device is made of a material selected from the group consisting of a stainless steel, a titanium alloy, an aluminum alloy, a chromium alloy, a PEEK material, a carbon fiber, an ABS plastic, a polyurethane, a resin, a fiber-encased resinous material, a rubber, a latex, a synthetic rubber, a polymer, and a natural material.

5. An orthopedic device for use in a minimally invasive surgical procedure, comprising:

a first patient- specific element configured to at least one patient-specific surface determined from a patient's anatomy and which anatomically conforms to at least a first subcutaneous anatomic feature of a specific patient;

a second patient-specific element configured to at least one second patient-specific surface determined from a patient's anatomy and which anatomically conforms to at least a second subcutaneous anatomic feature of a specific patient; and

an arcuate bridge coupling the first and second patient-specific elements, the arcuate bridge configured to be selectively engaged with the first and second patient-specific elements at a location beyond the patient's anatomy.

6. The orthopedic device of claim 5, further comprising first and second patient-specific bores passing through the corresponding first and second patient-specific elements and having patient-specific-orientations for guiding one or more fixation devices into the corresponding first and second anatomic portions of the patient.

7 The orthopedic device of claim 5, wherein in the first and second patient-specific surfaces correspond to first and second transverse processes of a vertebra of the patient.

8. The orthopedic device of claim 5, wherein the arcuate bridge further permits a user to verify proper placement and alignment of the first and second patient-specific elements.

9. The orthopedic device of claim 5, wherein the first and second patient-specific surfaces each anatomically mate with at least one contour of the lamina or inferior articular process of one or more vertebrae.

10. The orthopedic device of claim 5, wherein the device is configured to be used on one or more vertebrae of a patient.

11. The orthopedic device of claim 5, wherein the device may be selectively coupled to one or more additional orthopedic devices for mating with multiple anatomic features of a patient.

12. The orthopedic device of claim 6, wherein the first and second patient-specific bores are oriented along pre-determined trajectories determined from the anatomical features of the patient.

2014274748 05 Feb 2018

13. The orthopedic device of claim 11, wherein the device may be arranged in a monolithic or multi-level configuration for spanning multiple vertebrae of the patient.

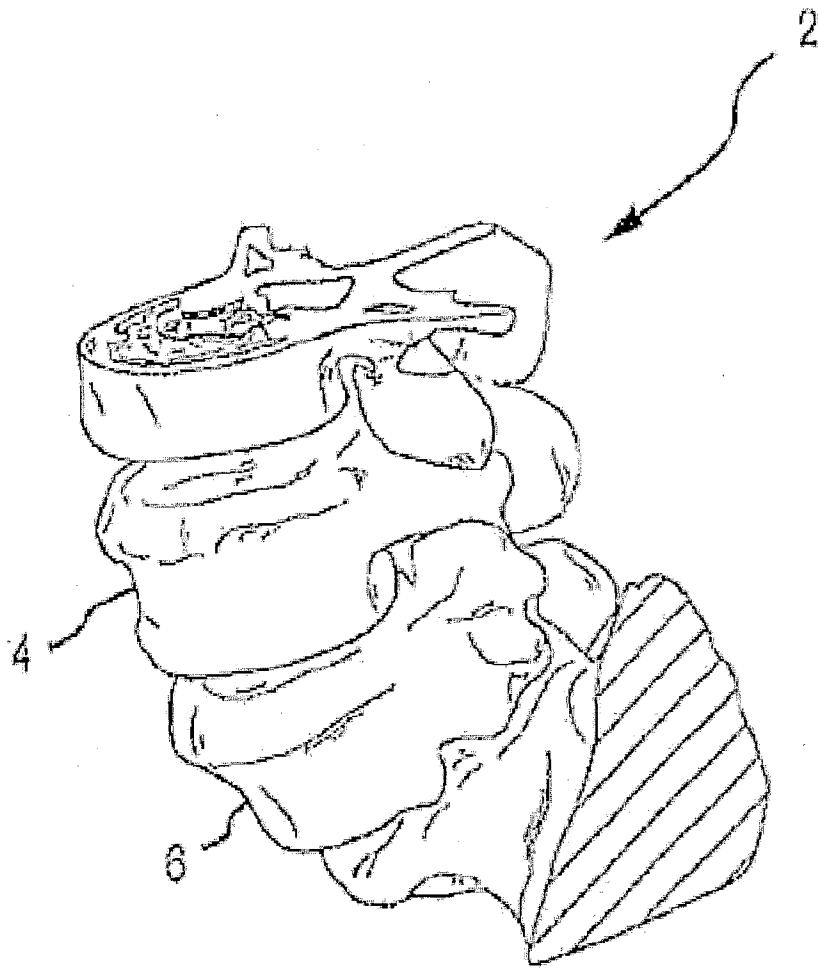


FIG.1

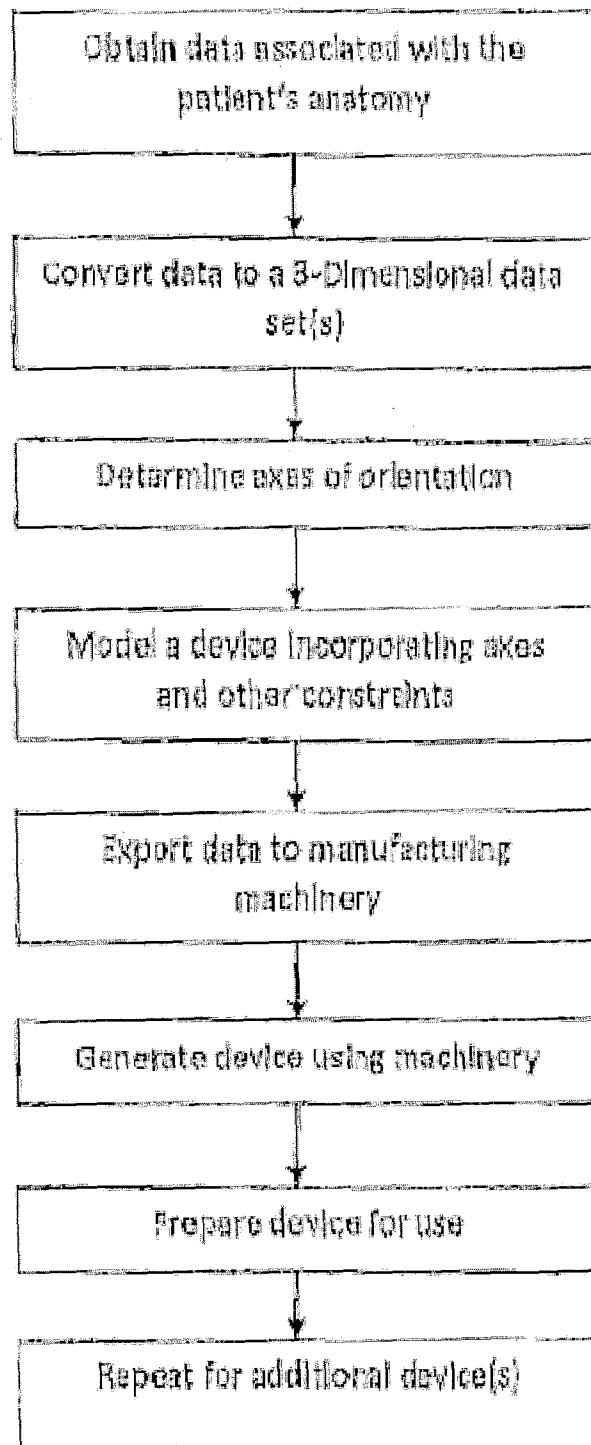
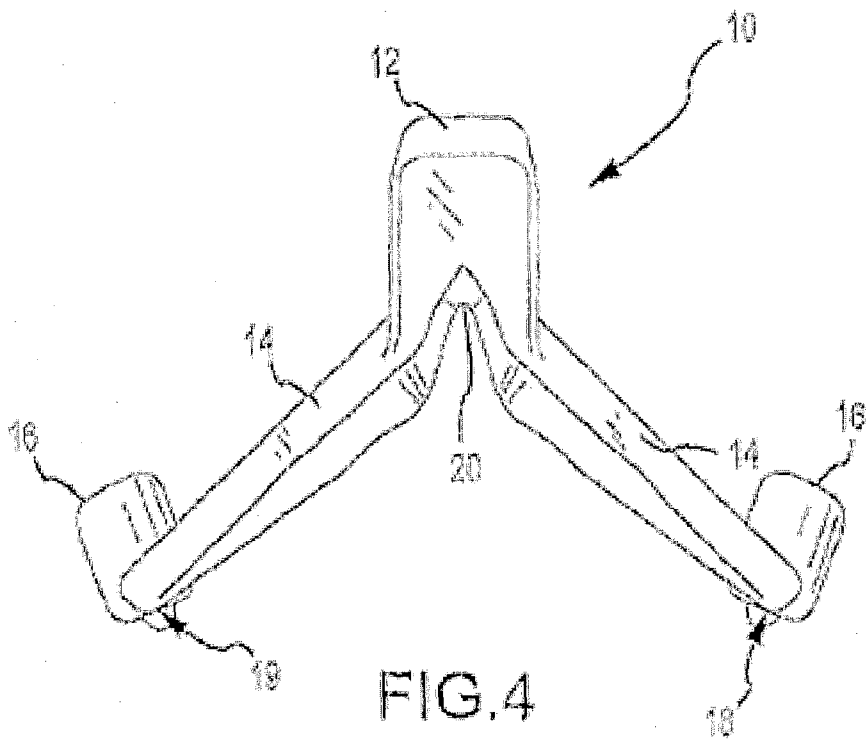
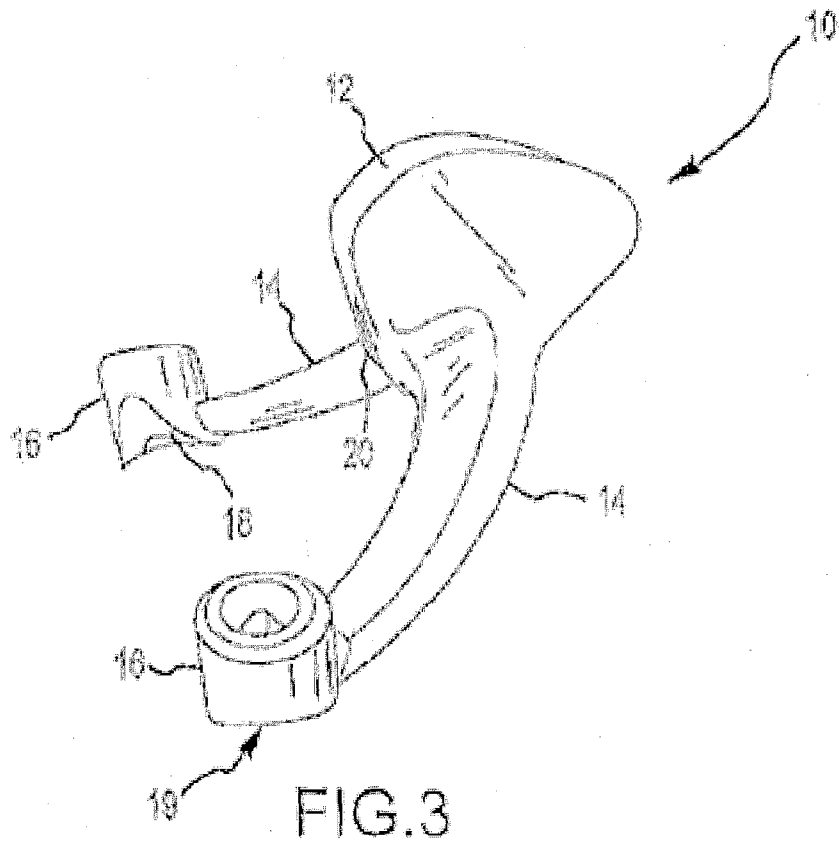


FIG. 2



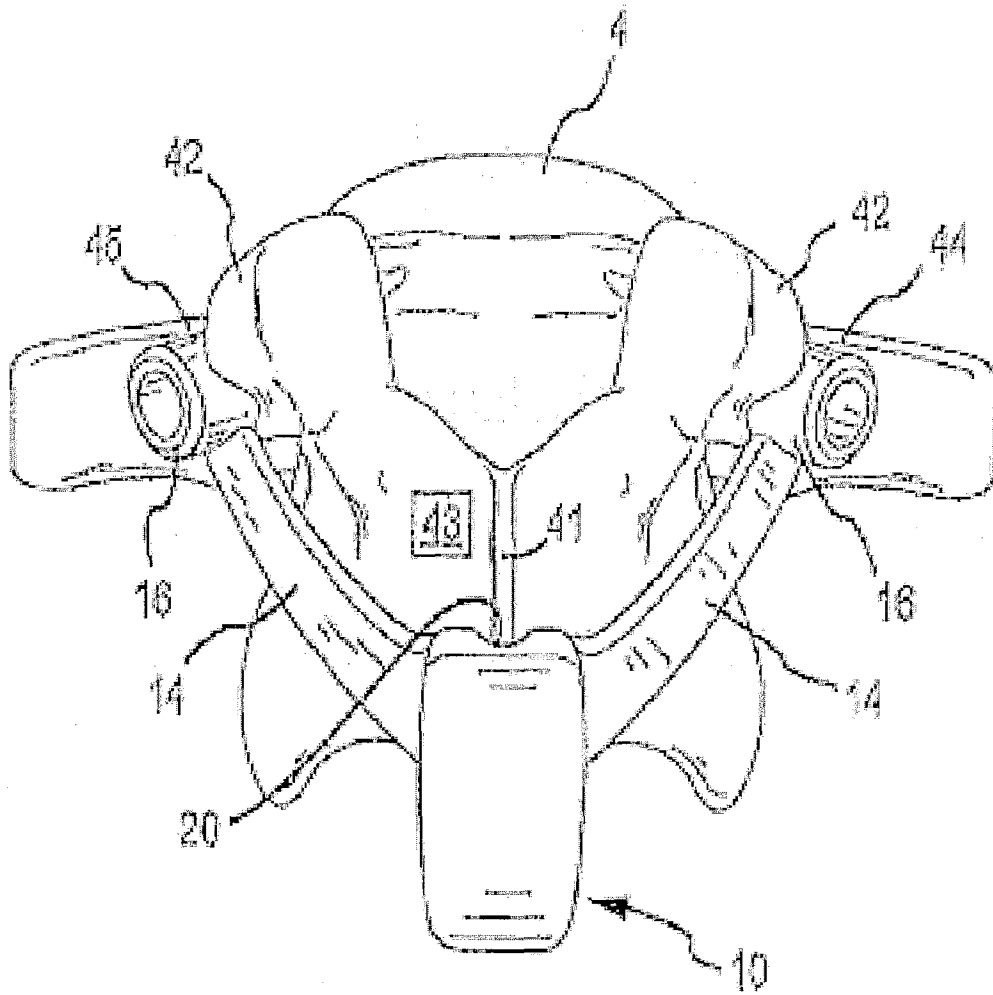


FIG.5

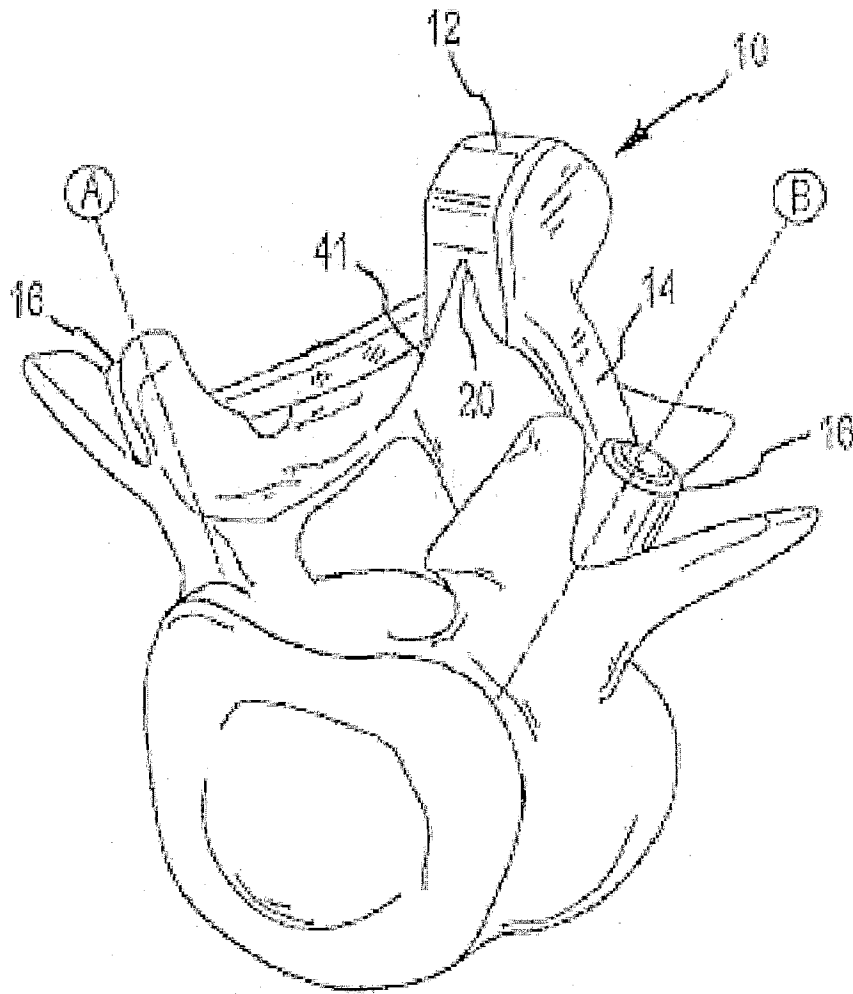


FIG. 6

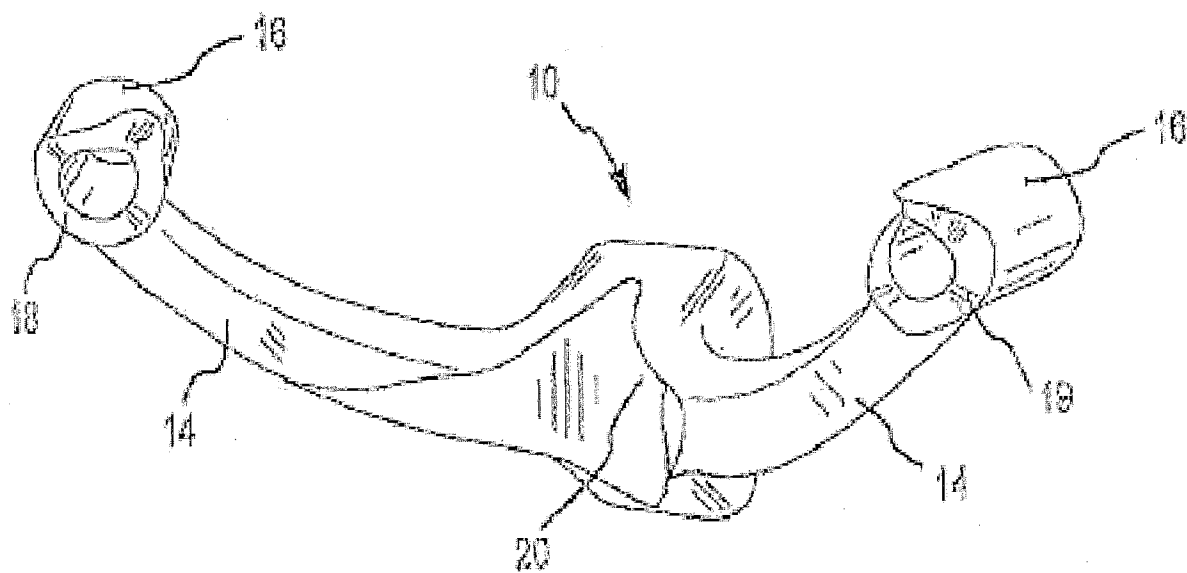


FIG.7

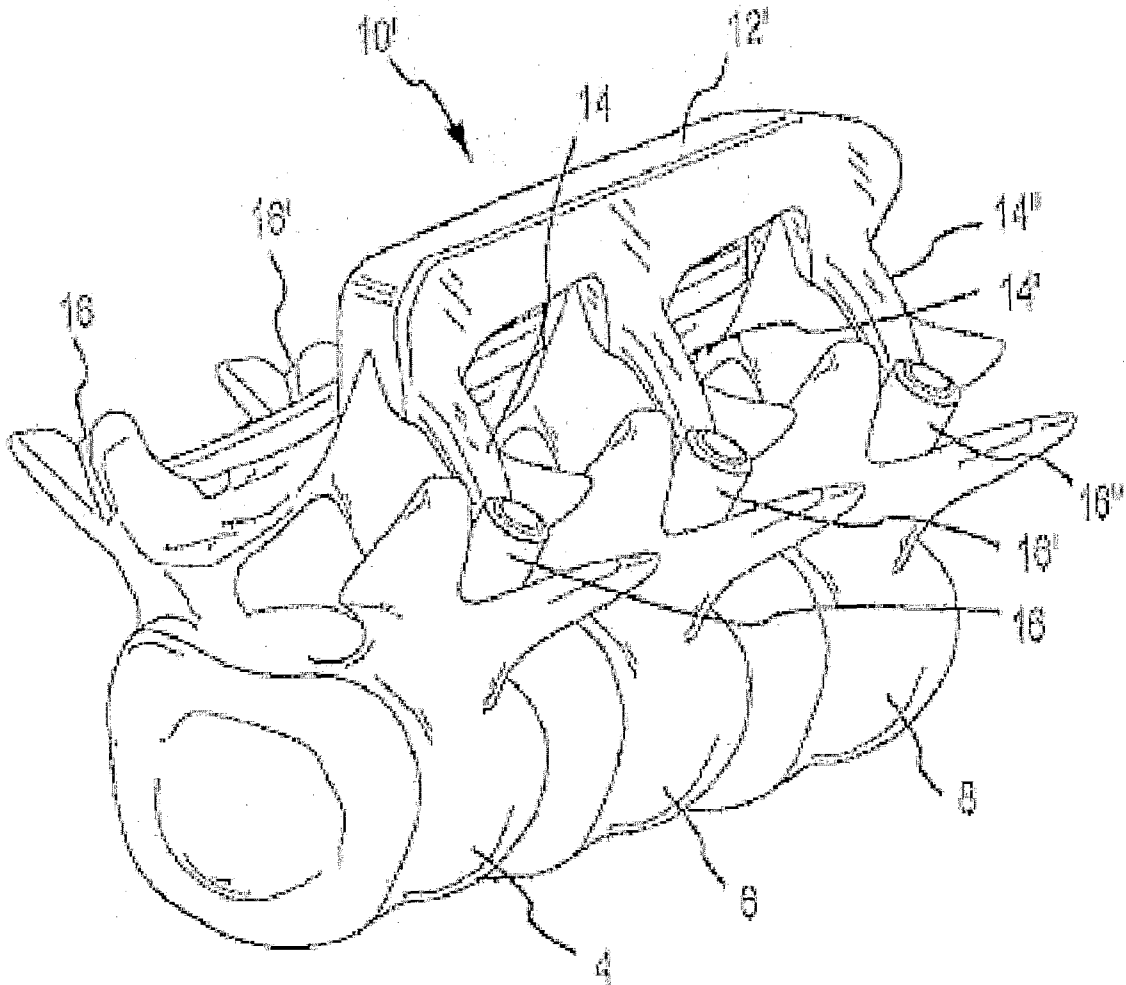


FIG. 8

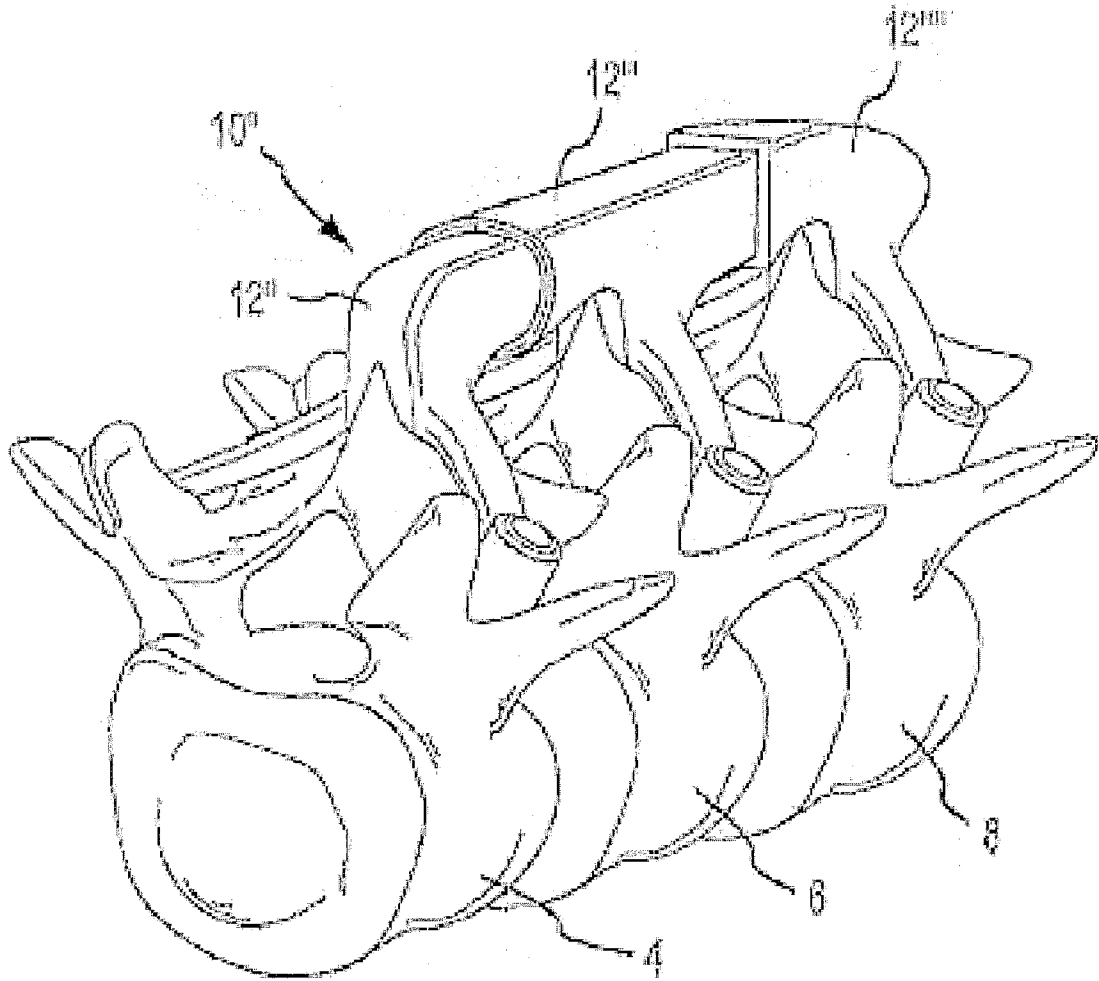


FIG. 9

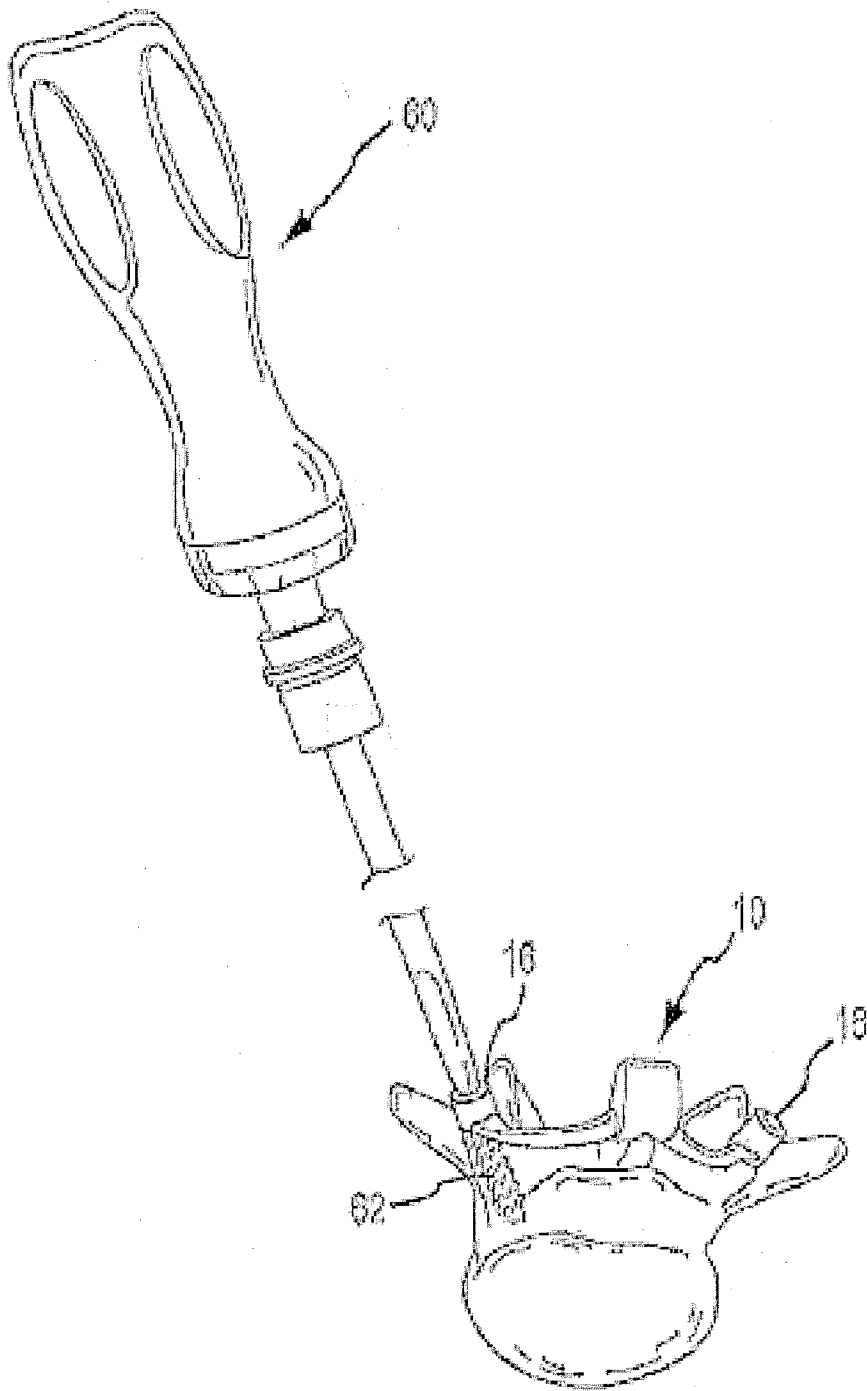
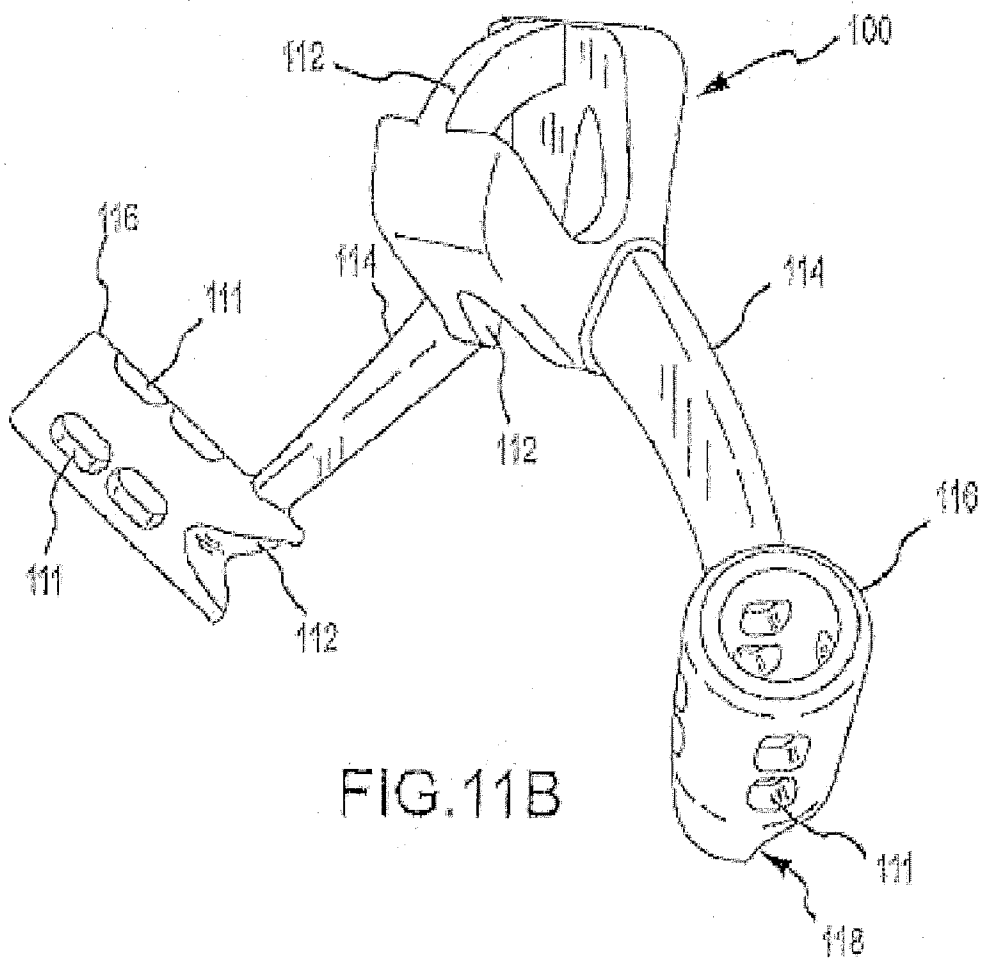
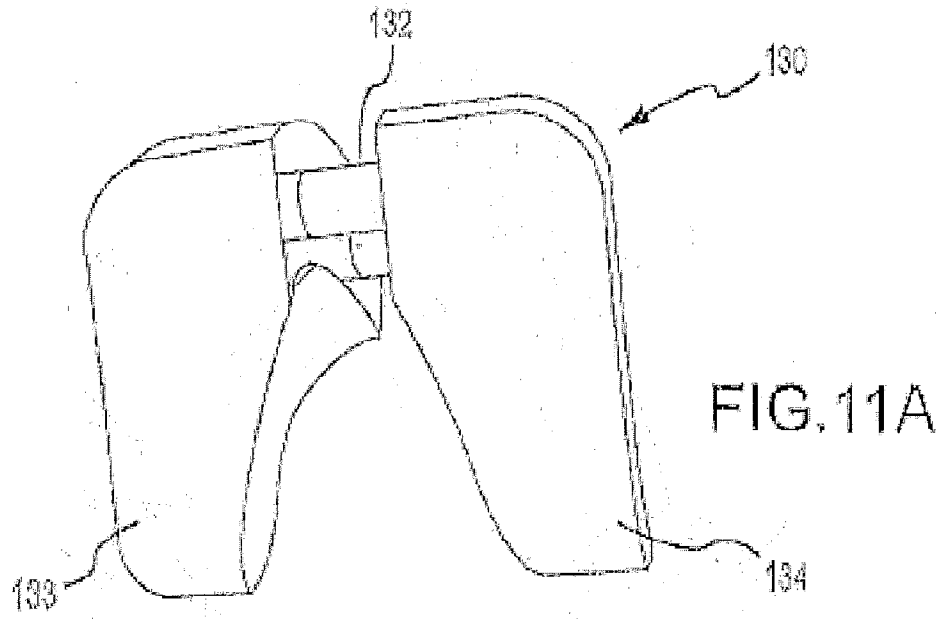
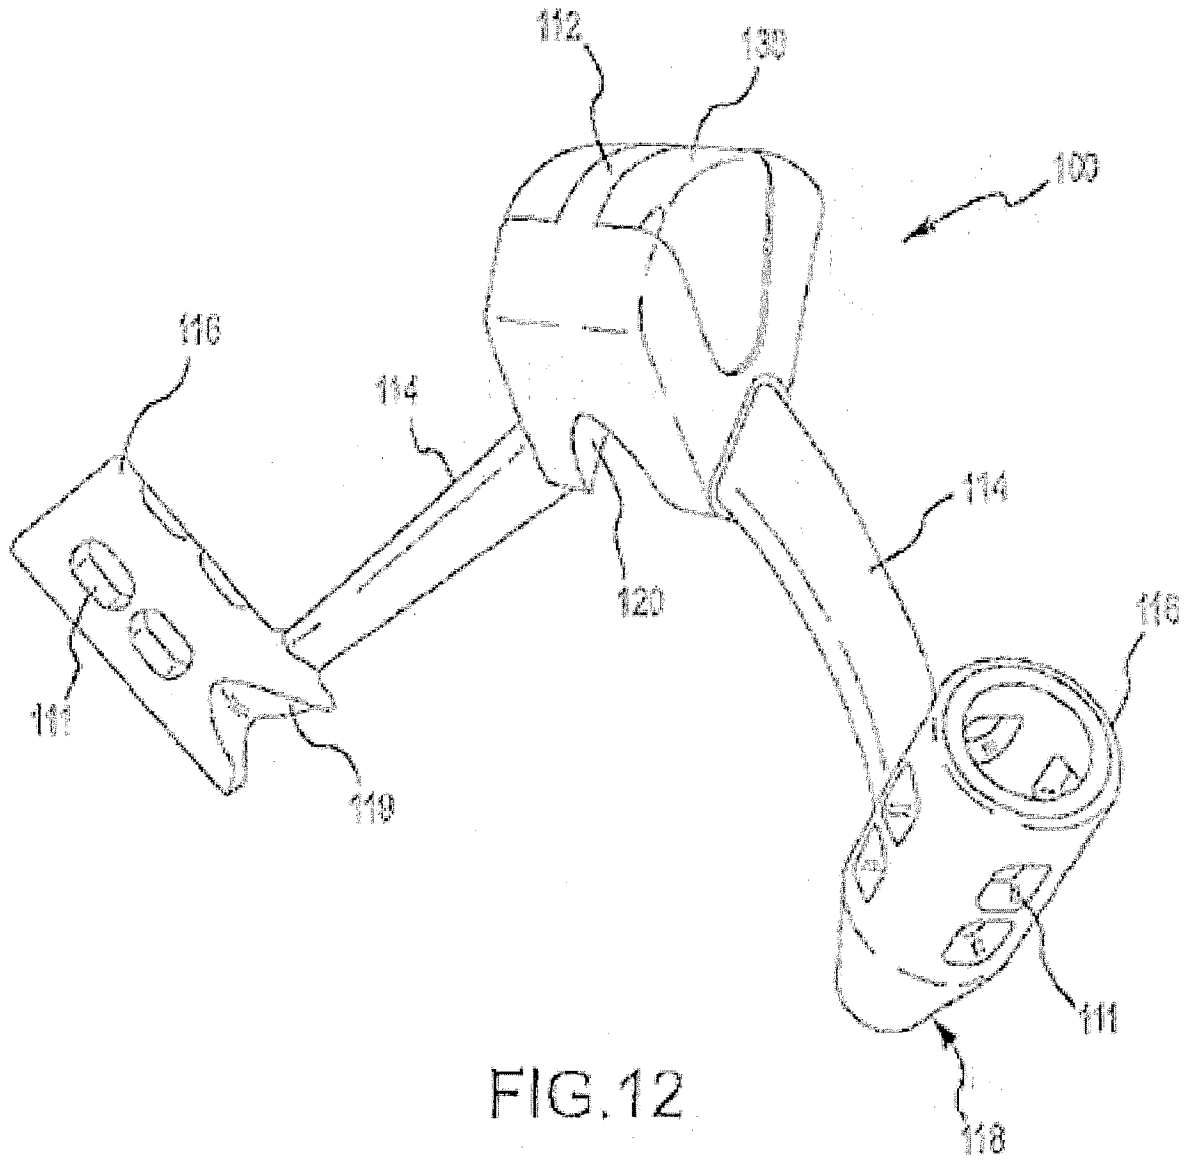


FIG. 10





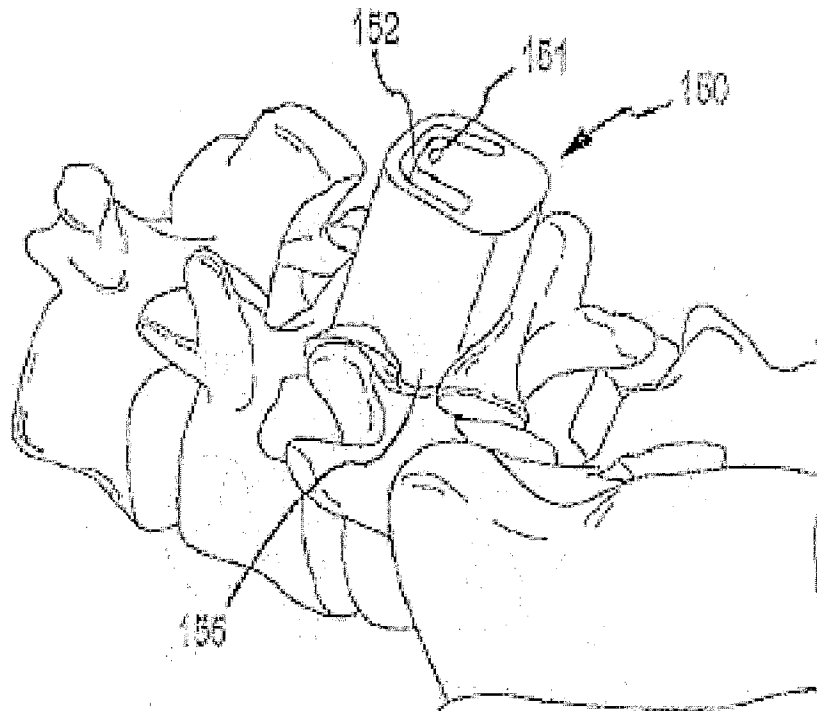


FIG. 13

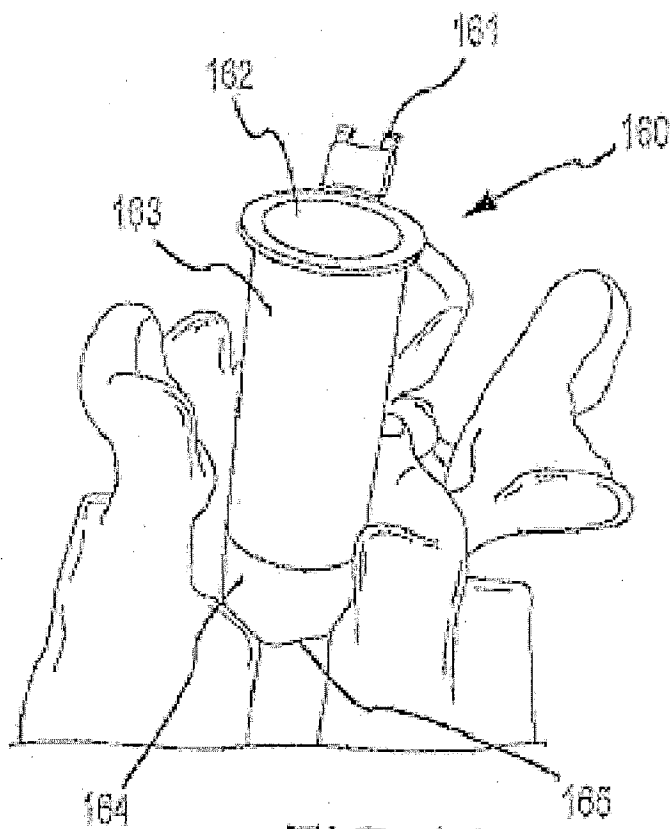


FIG. 14

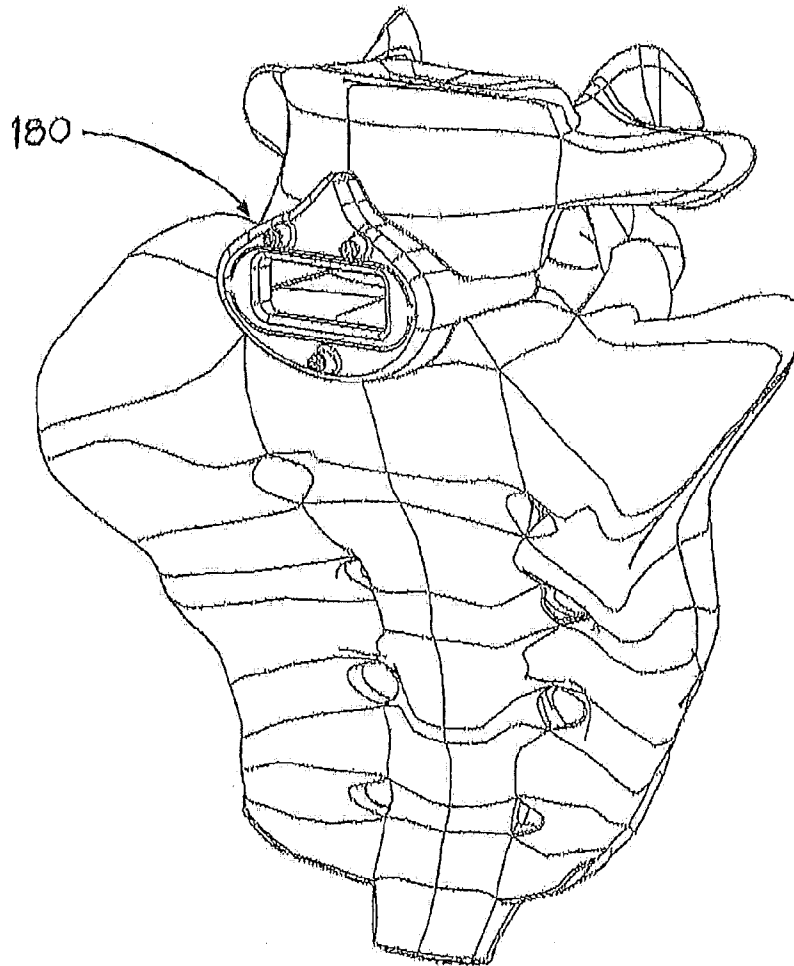


FIG. 15

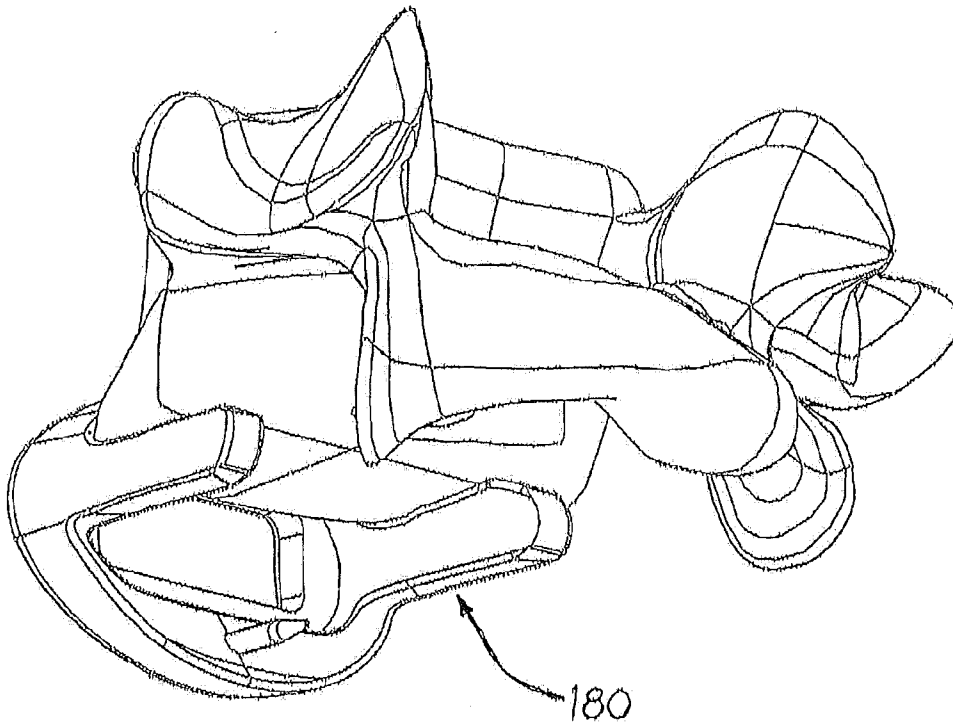


FIG. 16

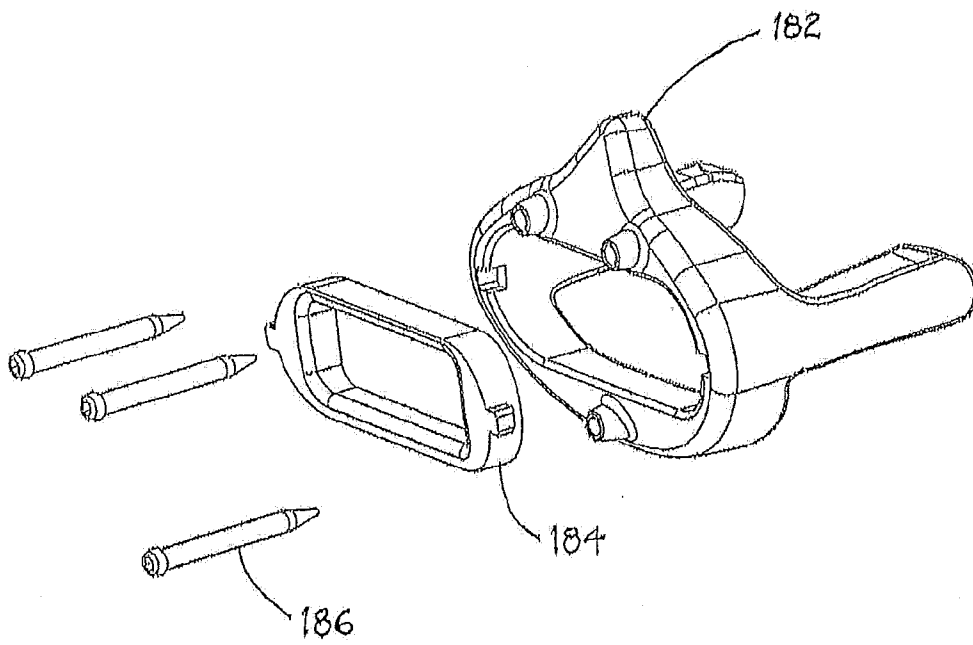


FIG. 17

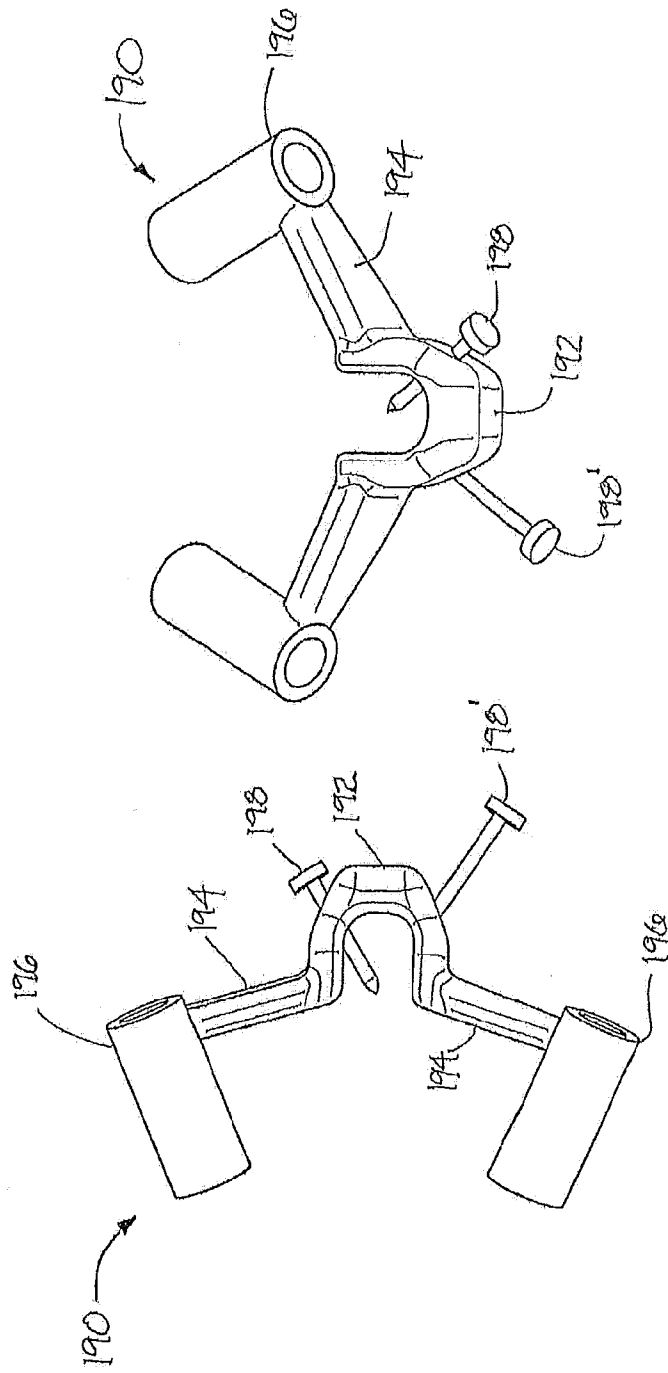


FIG. 19

FIG. 18

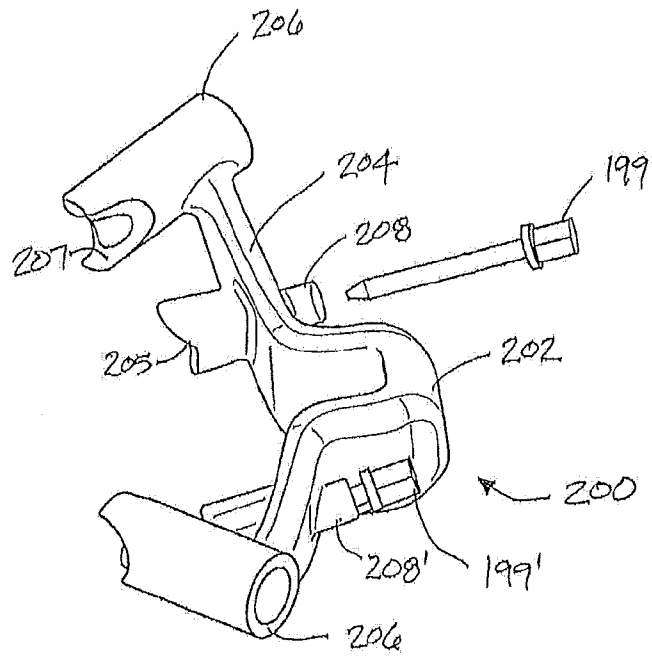


FIG. 20

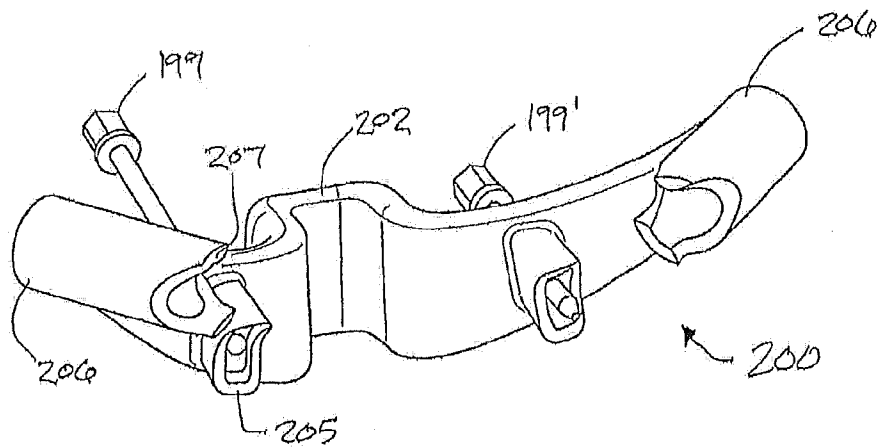


FIG. 21

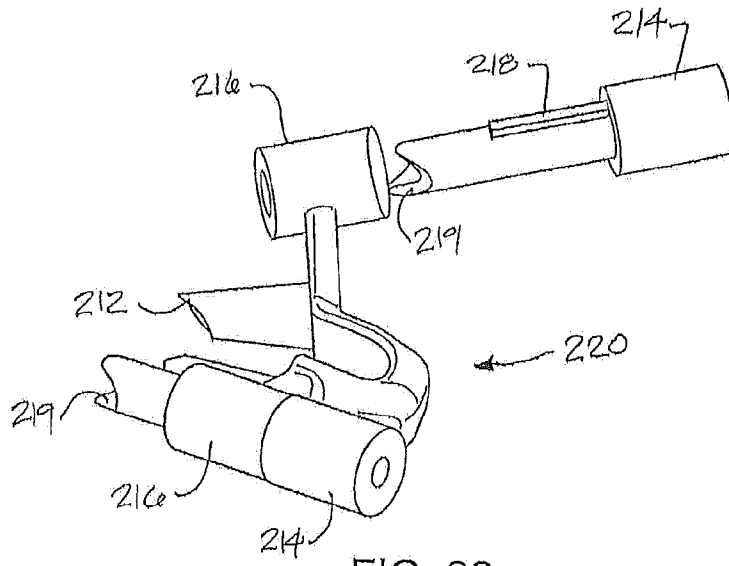


FIG. 22

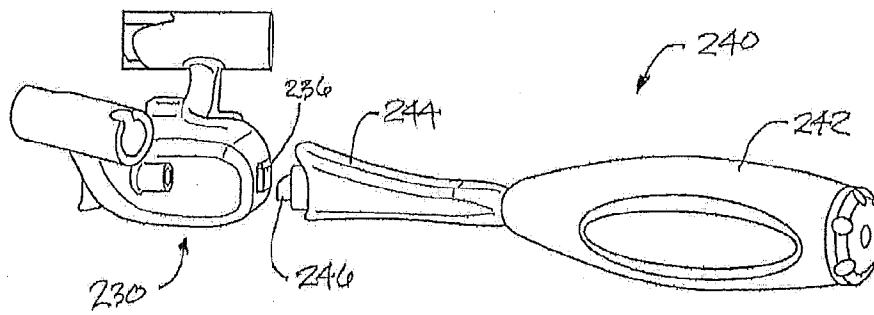


FIG. 23

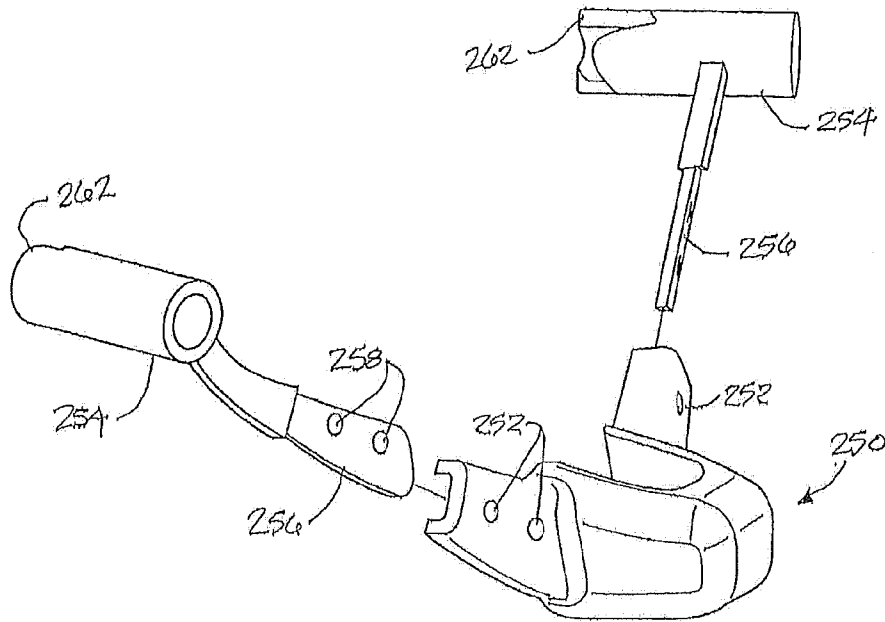


FIG. 24

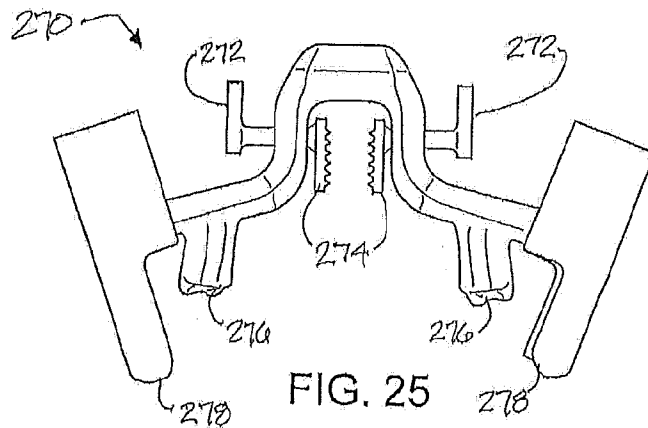


FIG. 25

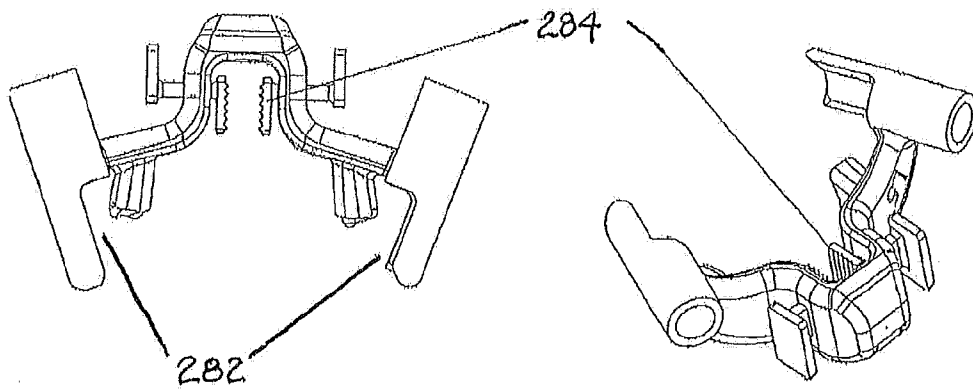


FIG. 26A

FIG. 26B

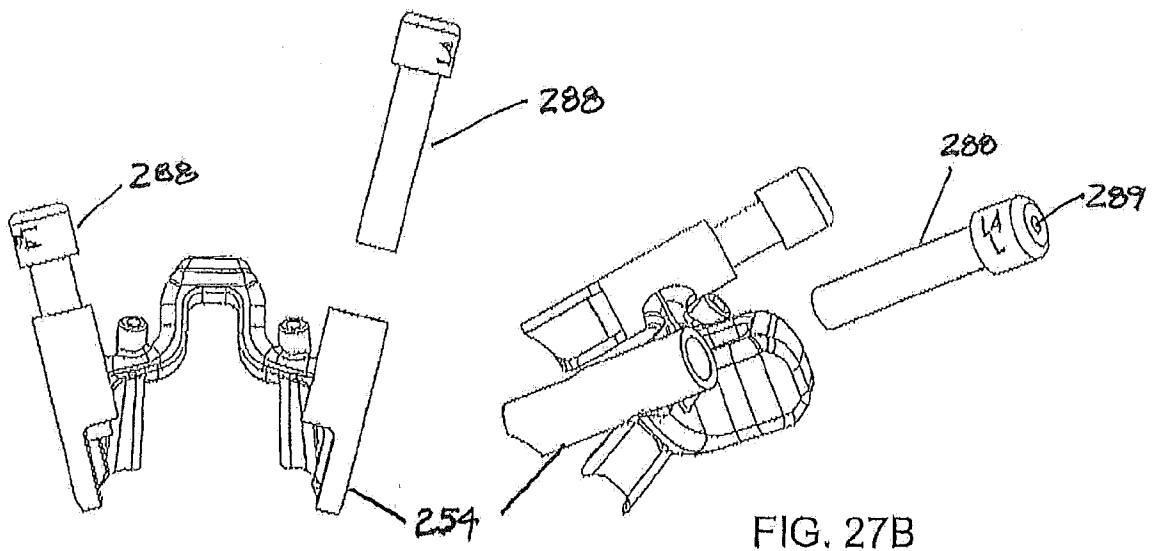


FIG. 27A

FIG. 27B



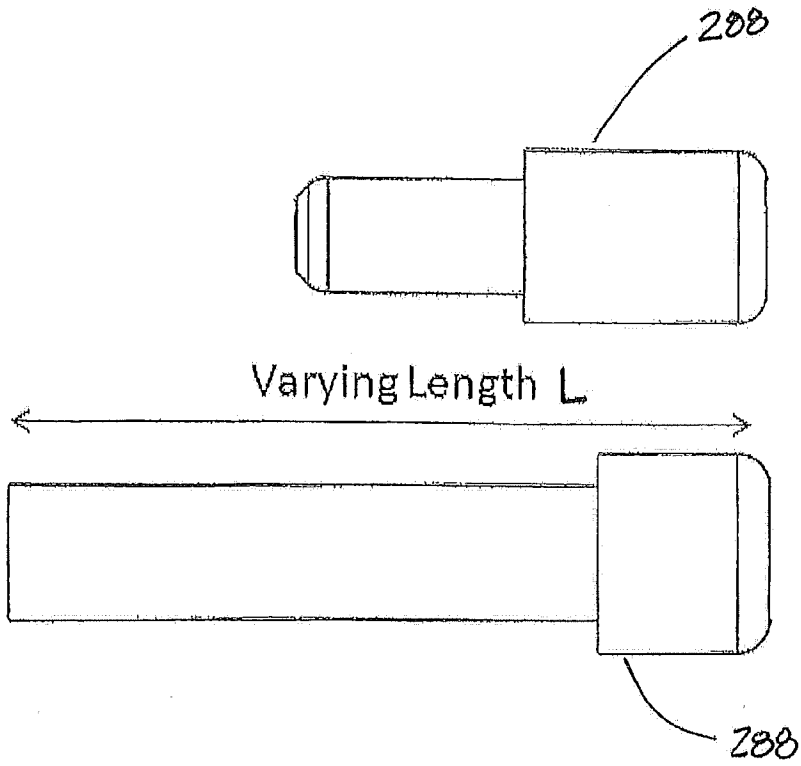


FIG. 28

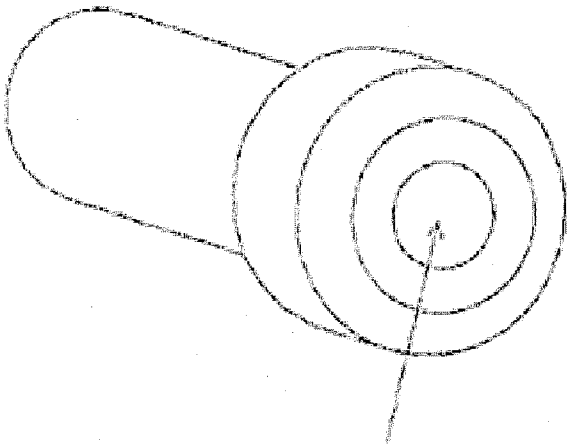

Insert Diameter for 4.5 mm Tap

FIG. 29A

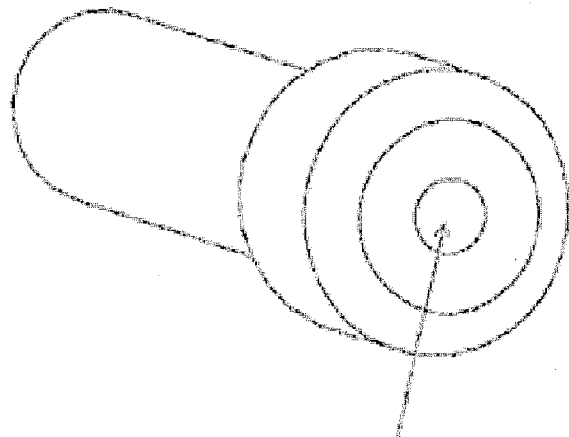

Insert Diameter for 1/8" Drill Bit

FIG. 29B

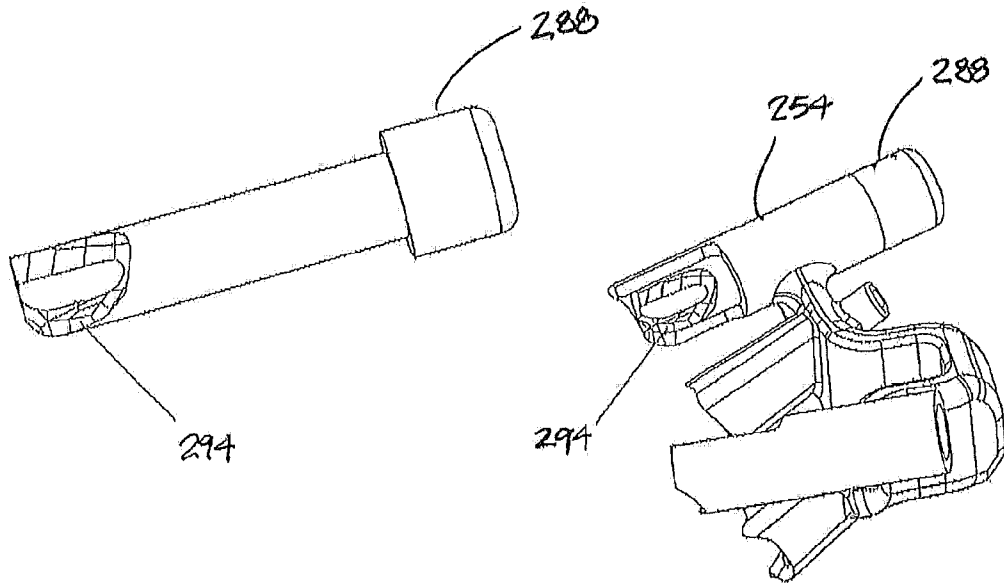


FIG. 30

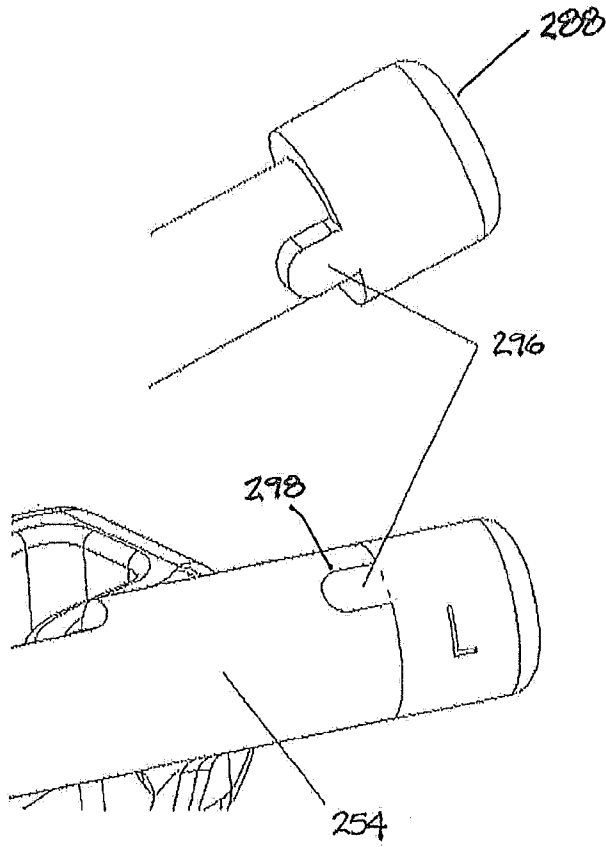


FIG. 31

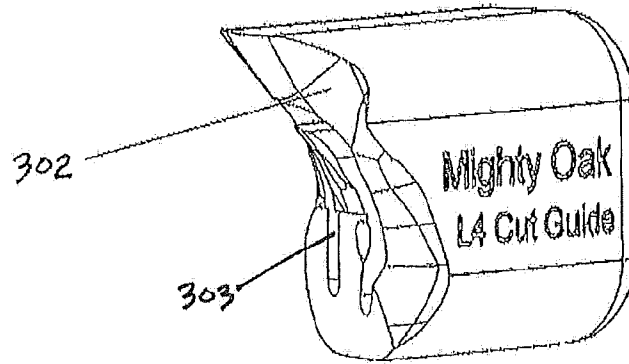


FIG. 32A

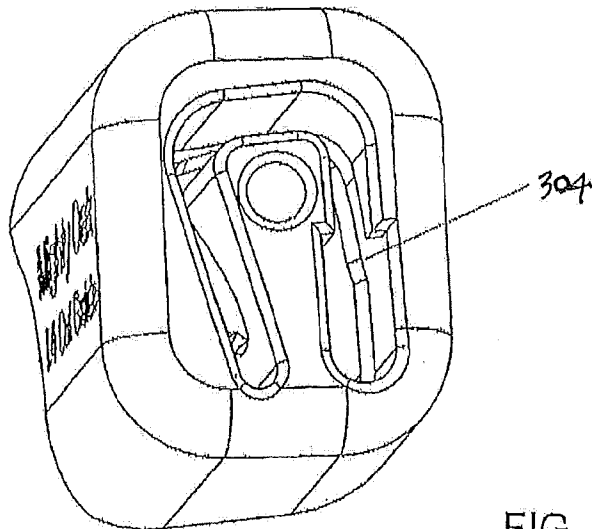


FIG. 32B

FIG. 33A

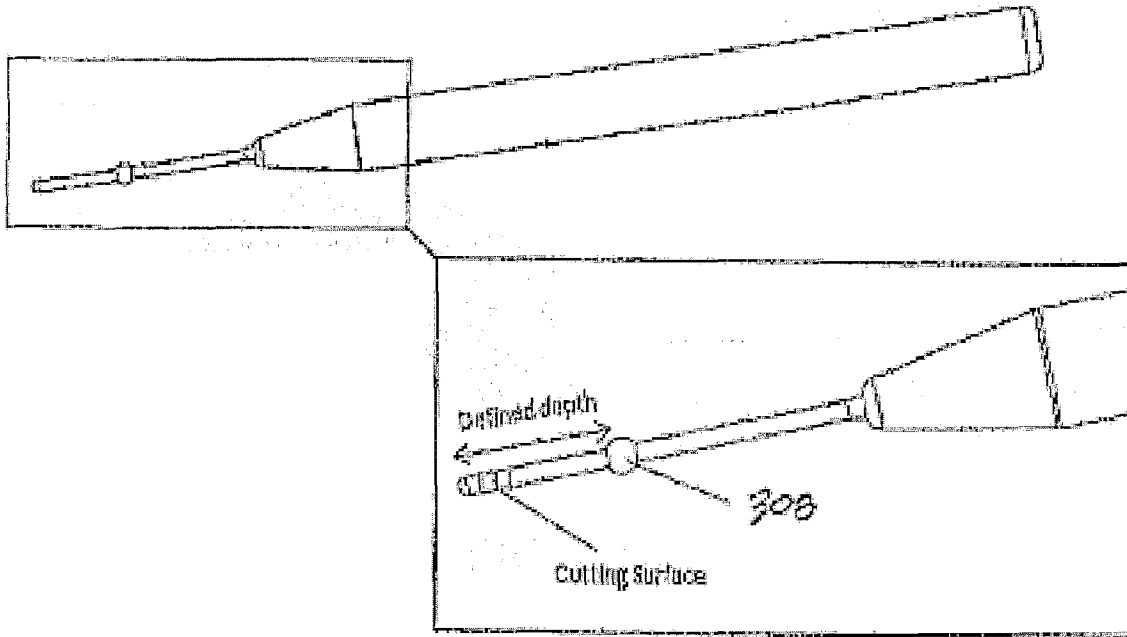


FIG. 33B

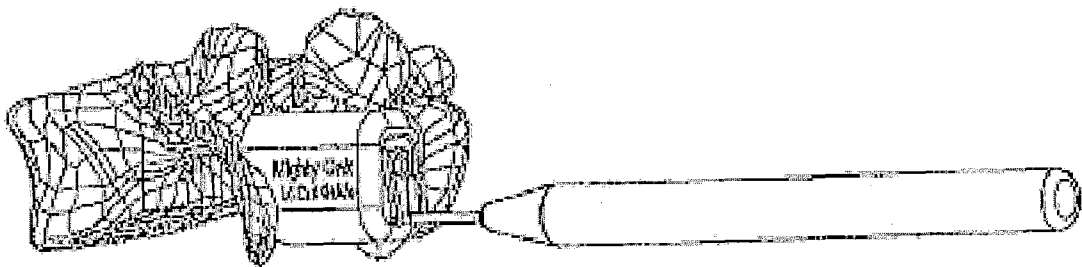


FIG. 33C

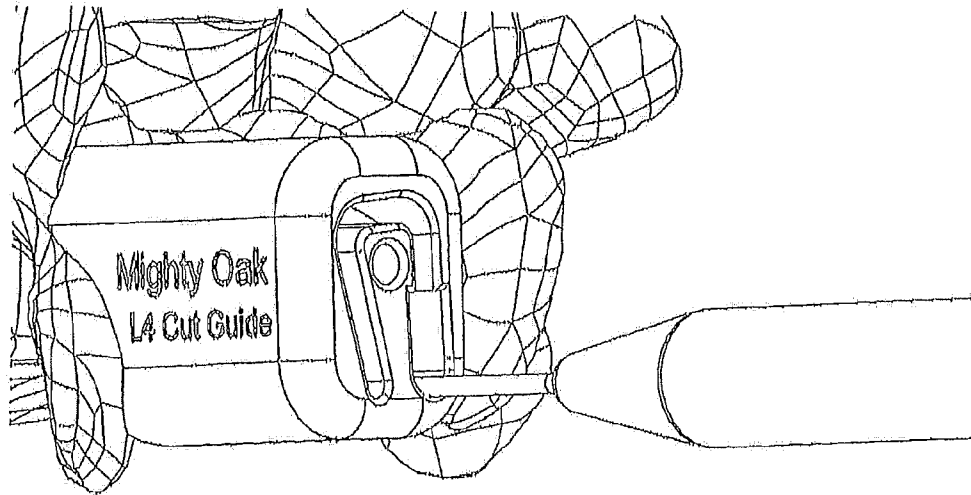


FIG. 34A

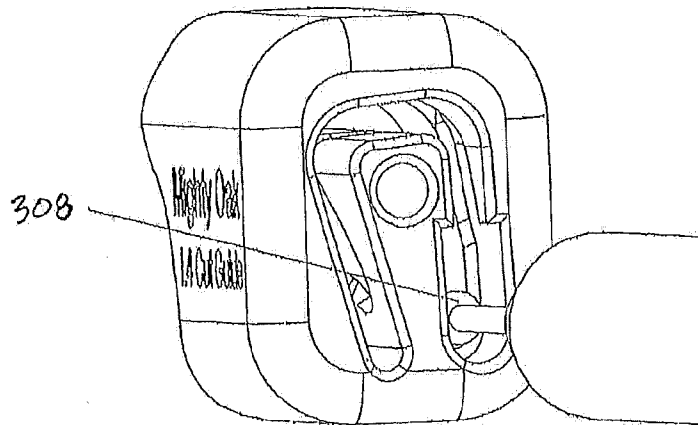


FIG. 34B

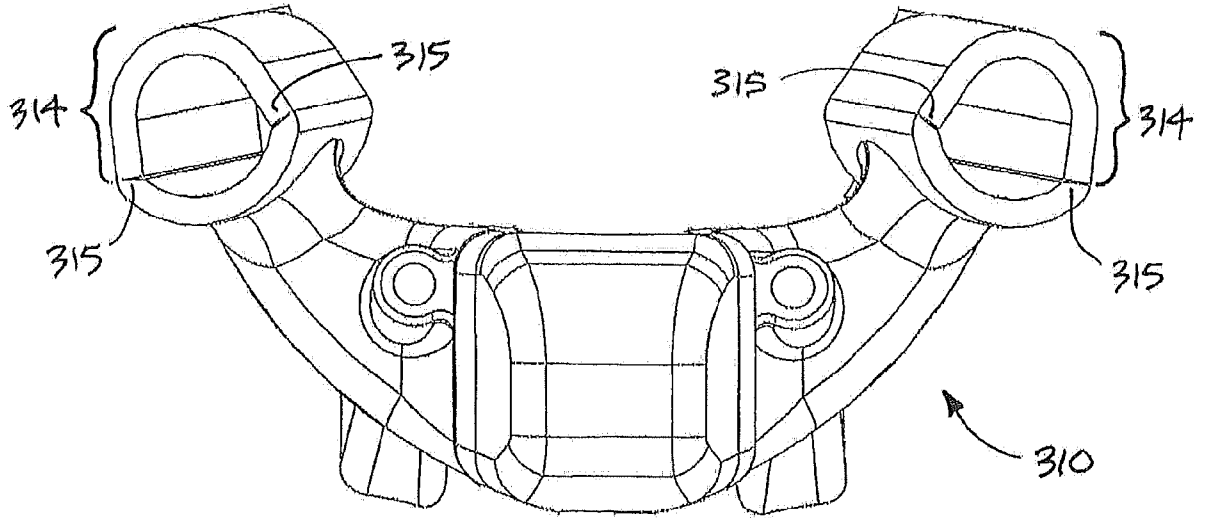


FIGURE 35

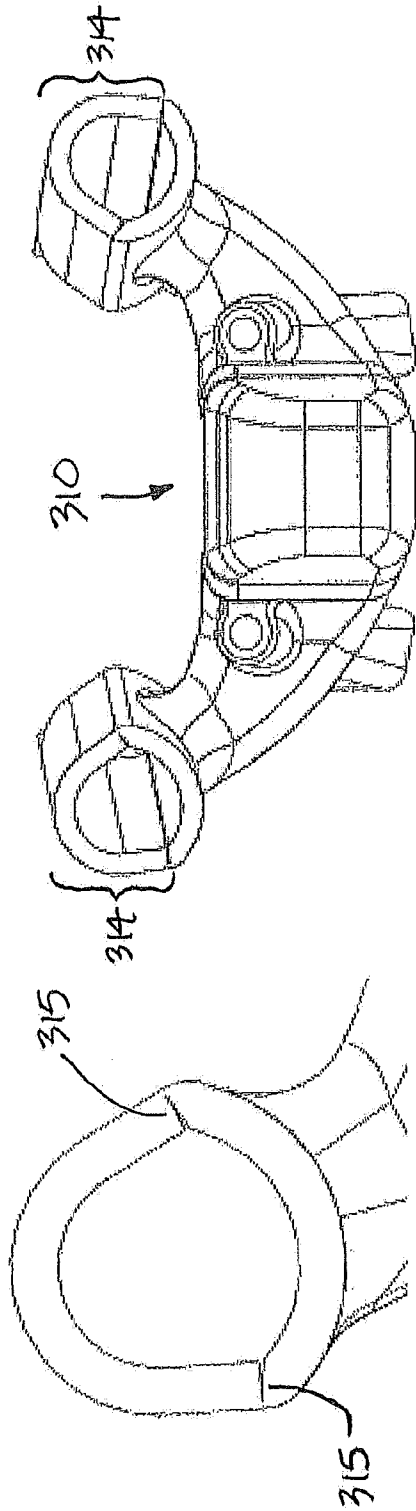


FIGURE 36

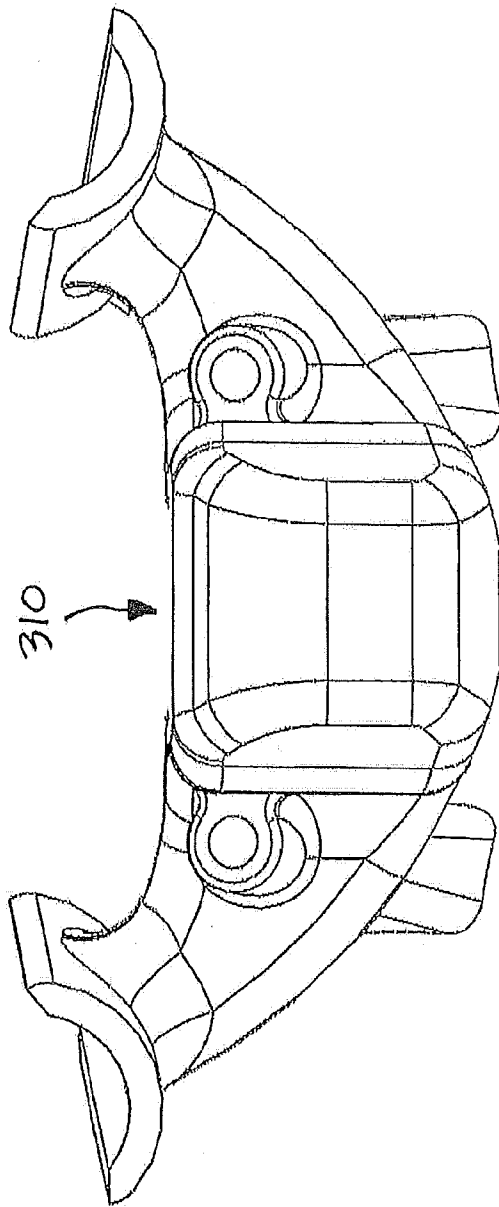


FIGURE 37

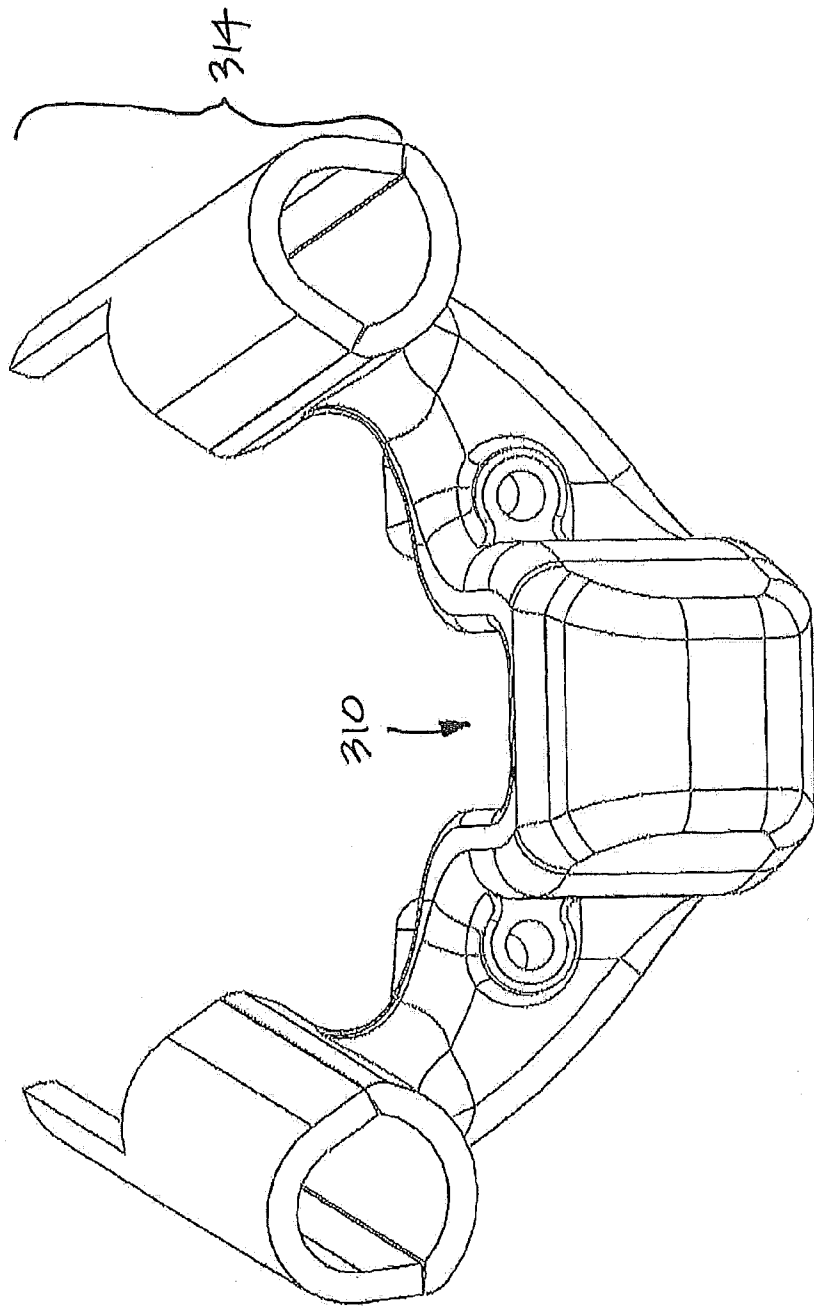


FIGURE 38

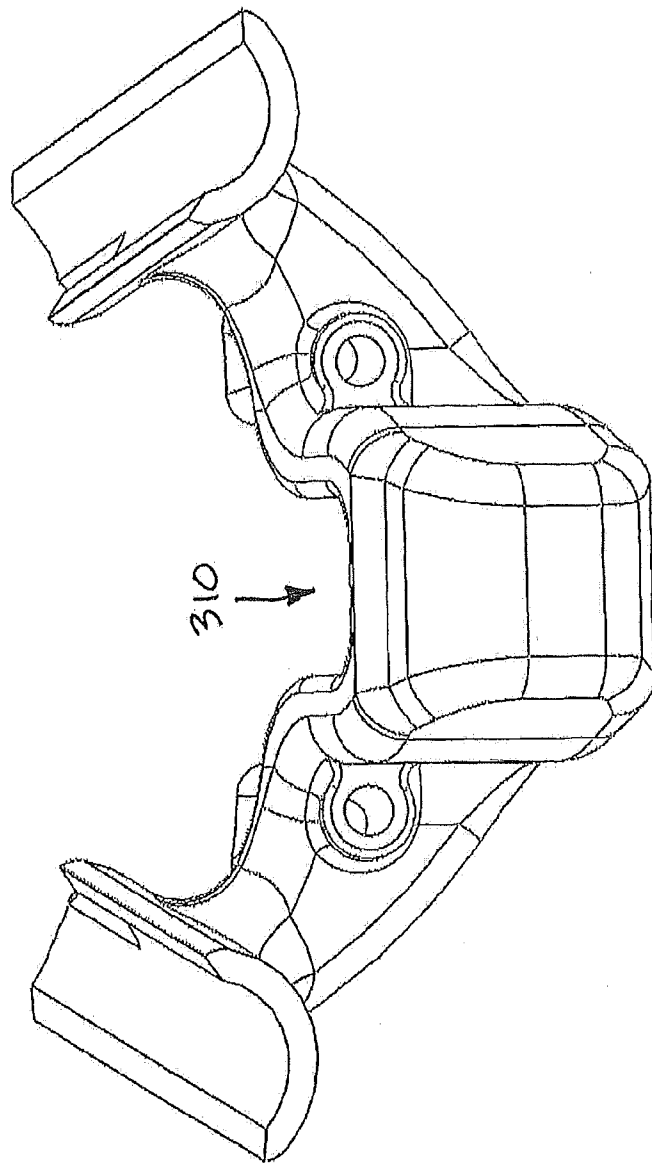


FIGURE 39

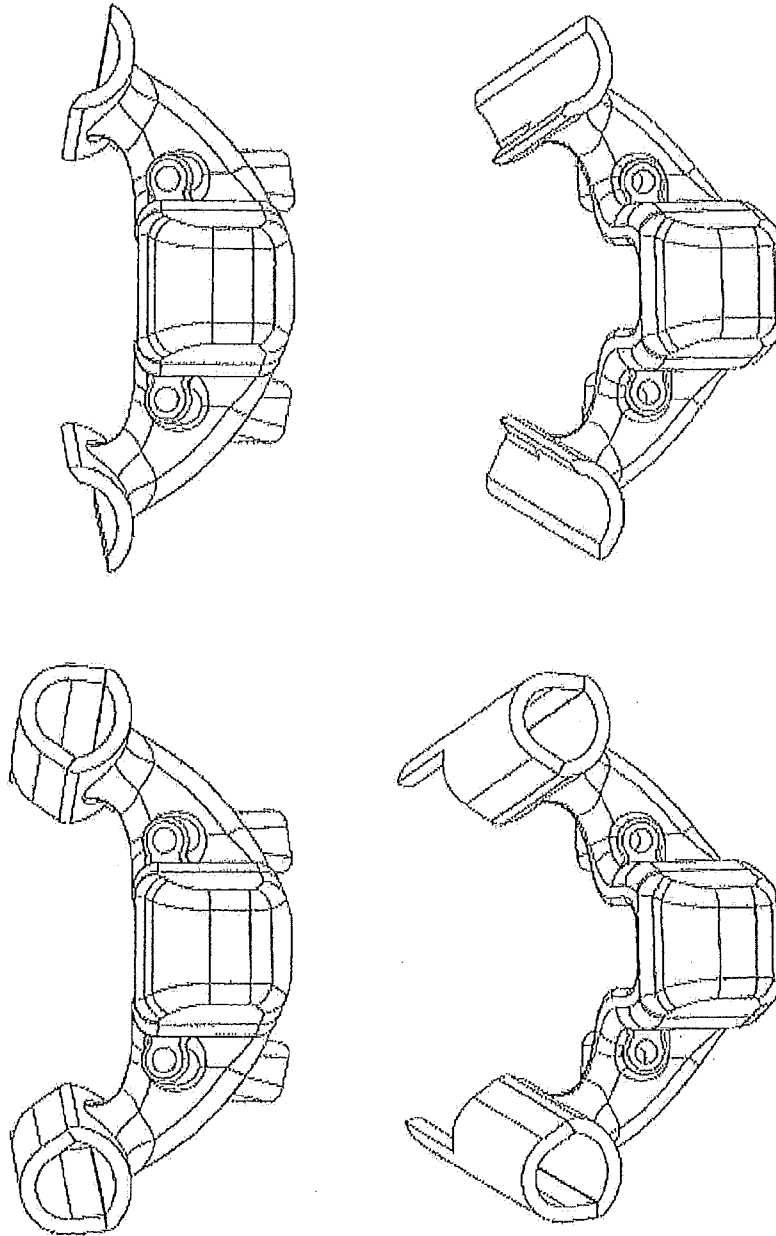


FIGURE 40 A-D

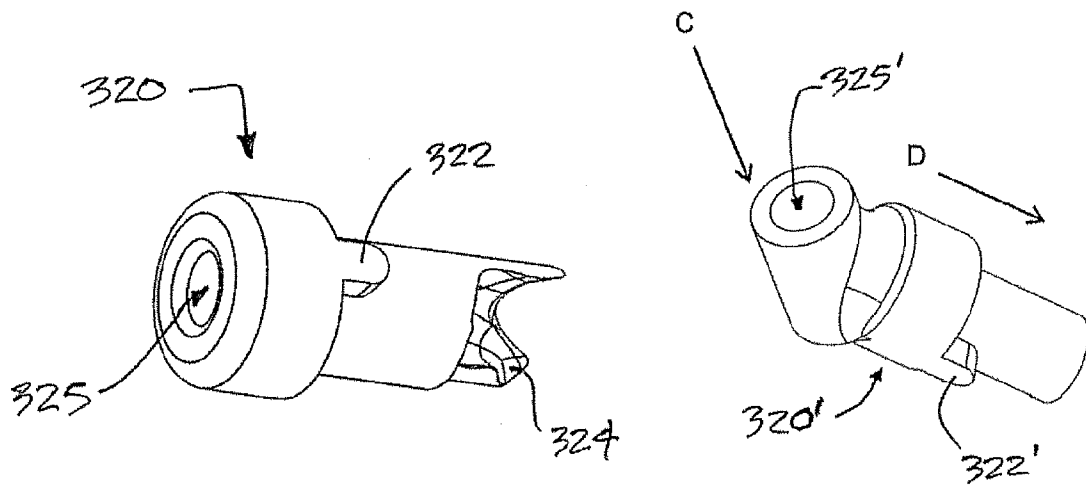


FIG. 41

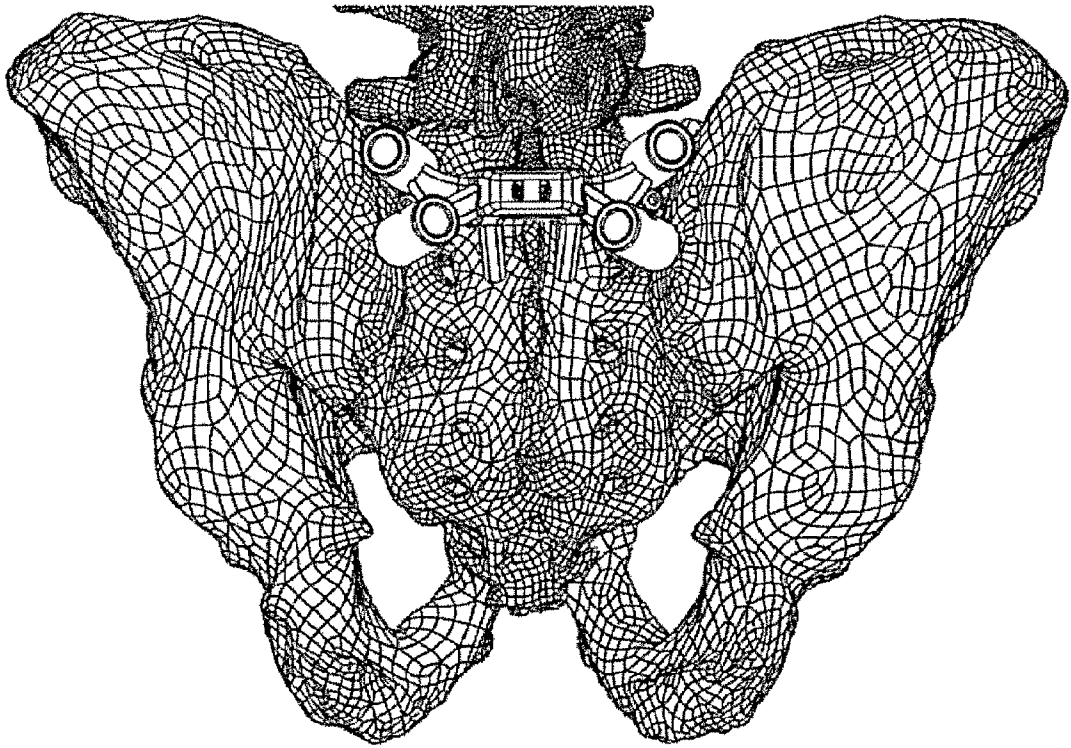


FIG. 42A

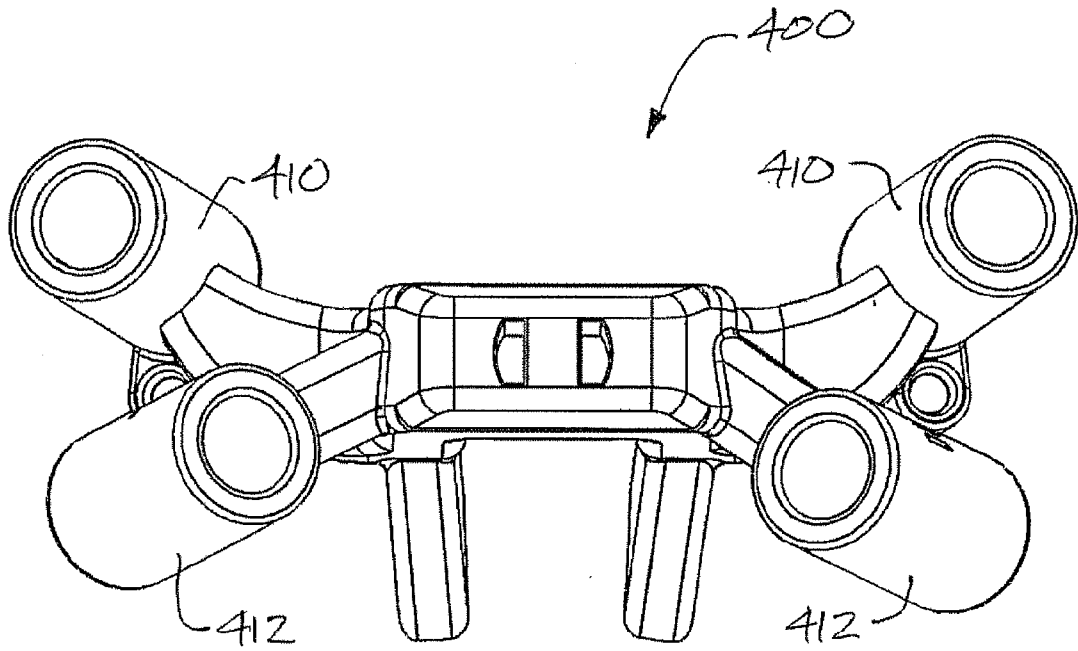


FIG. 42B

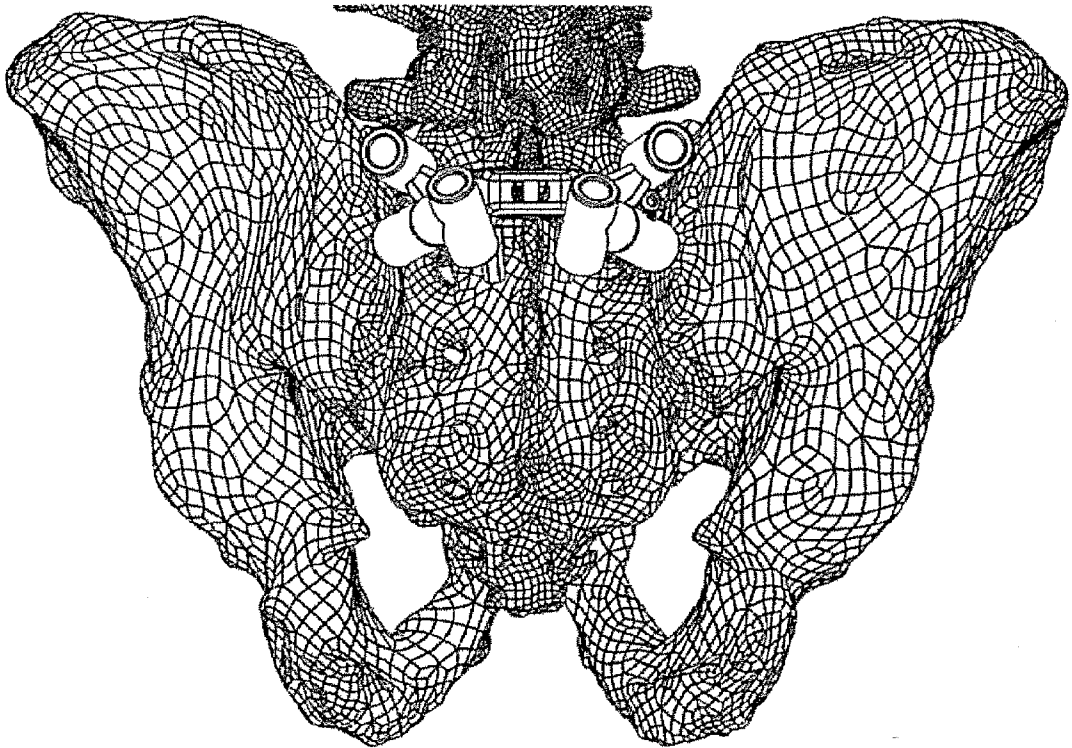


FIG. 43A

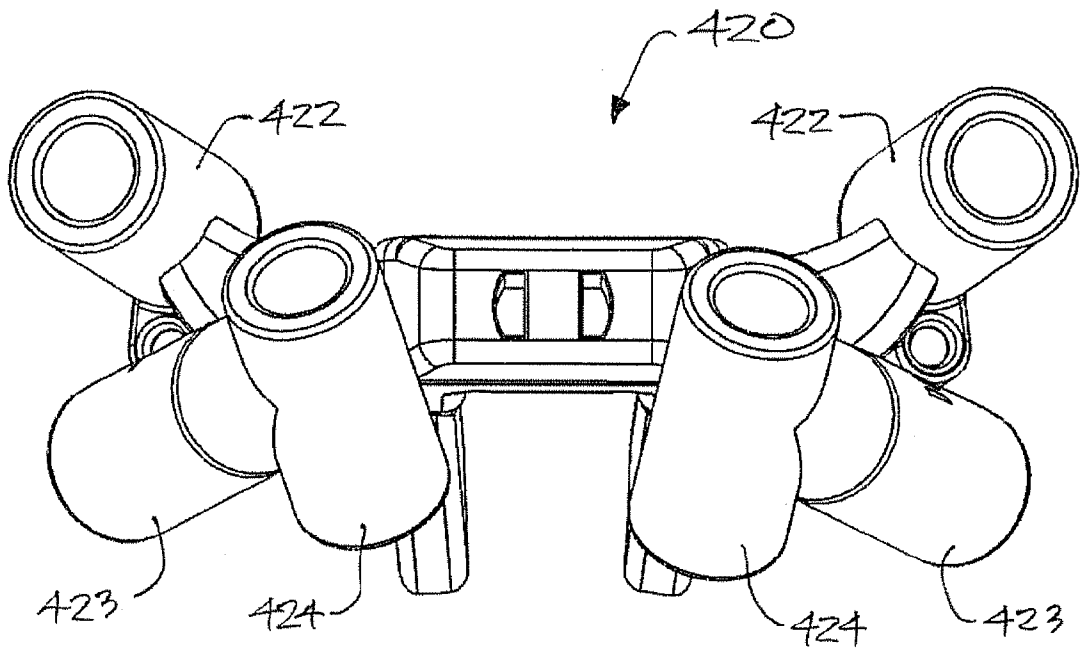


FIG. 43B

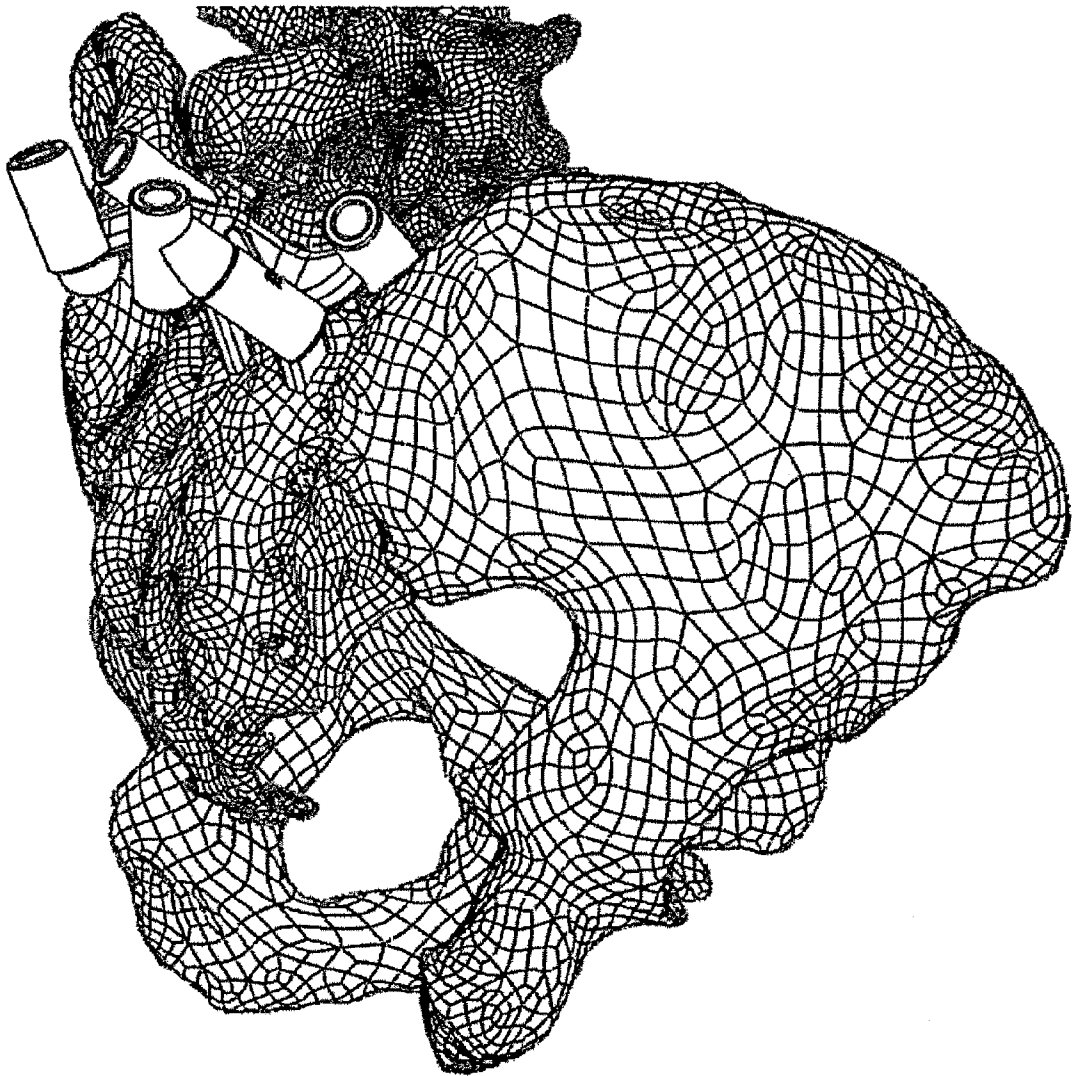


FIG. 44A

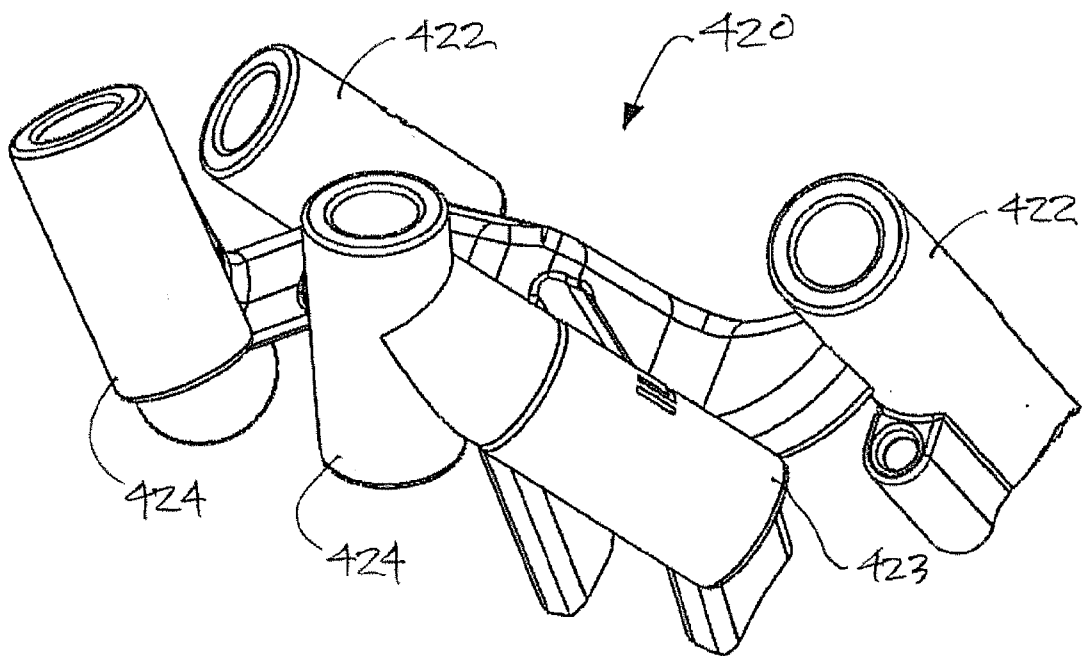


FIG. 44B

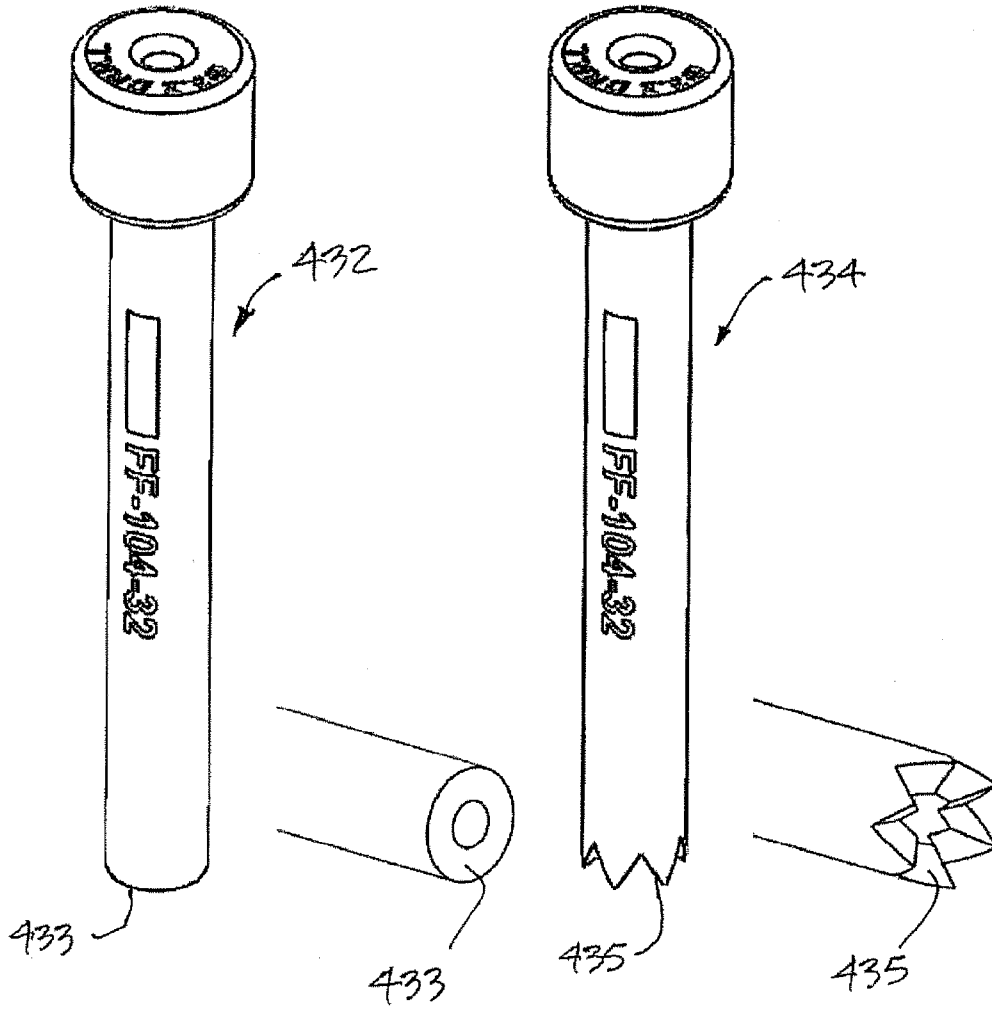


FIG. 45

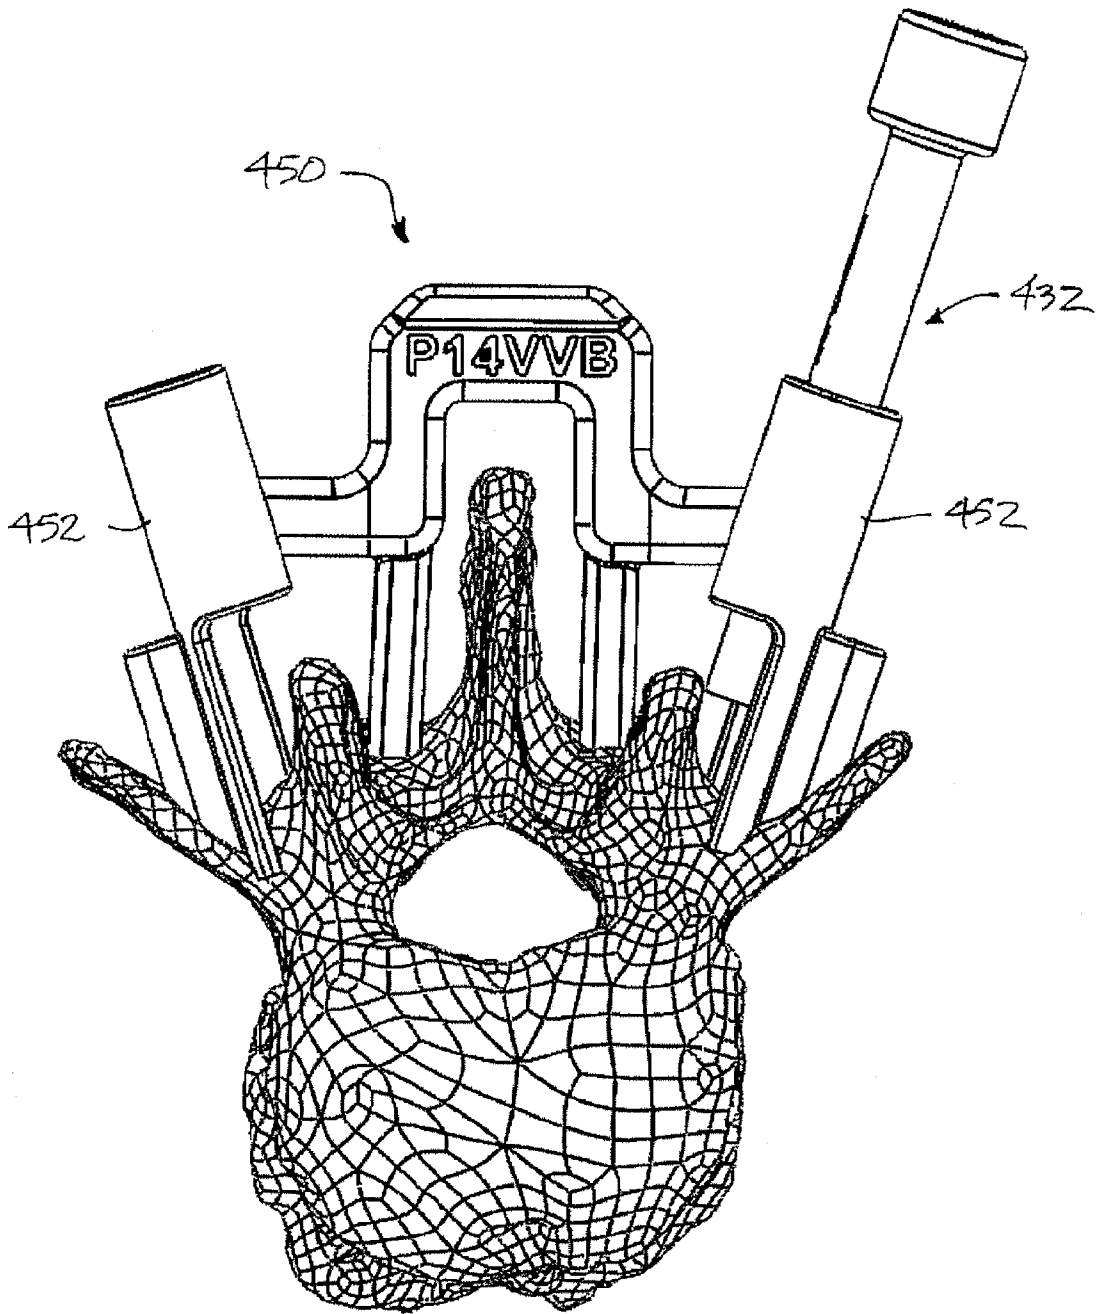


FIG. 46

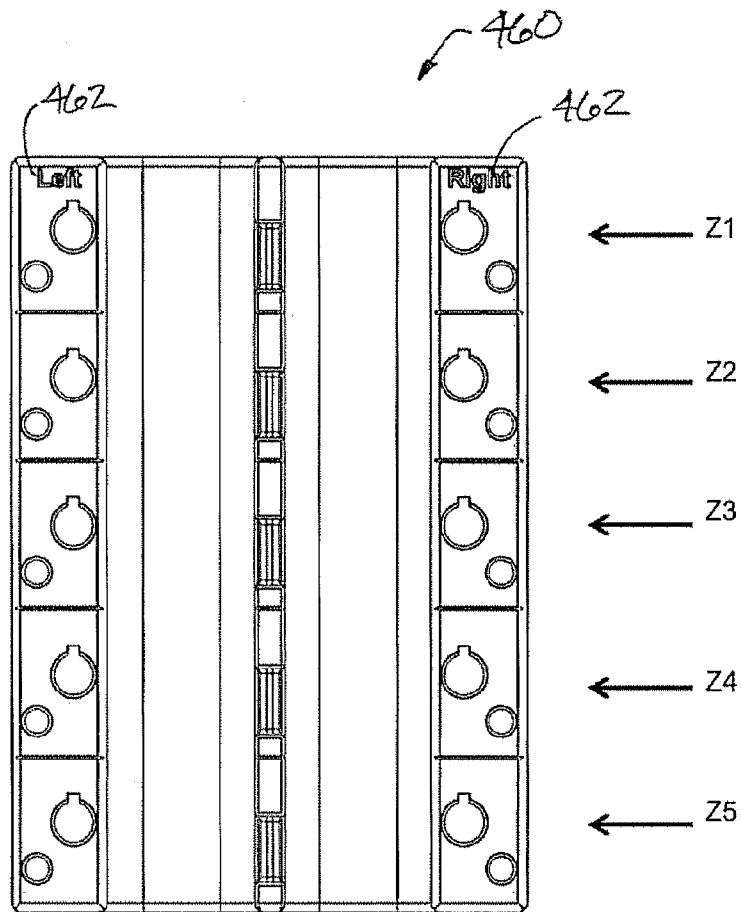


FIG. 47A

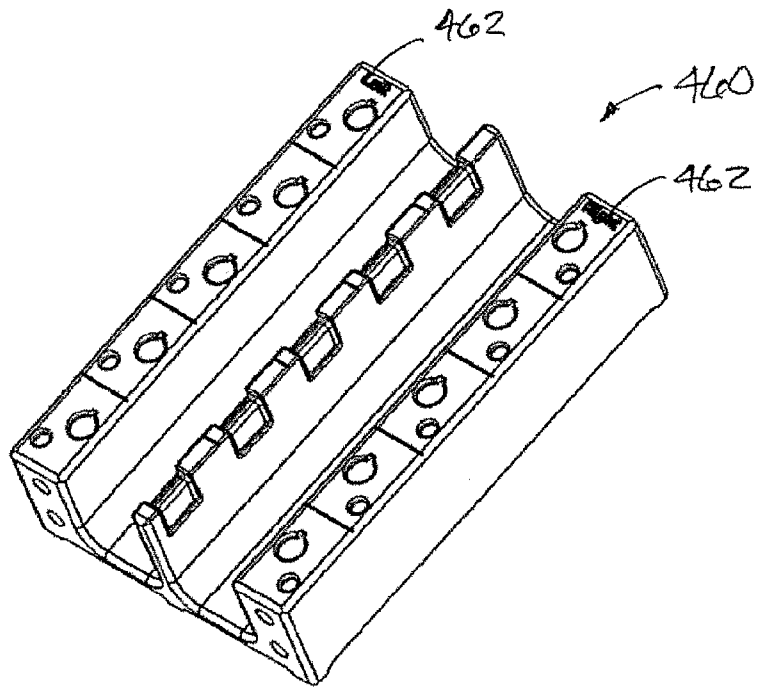


FIG. 47B

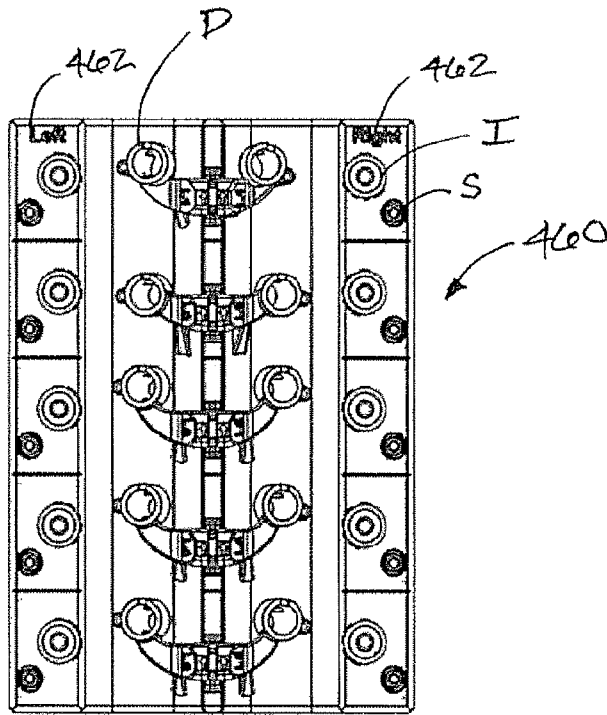


FIG. 47C

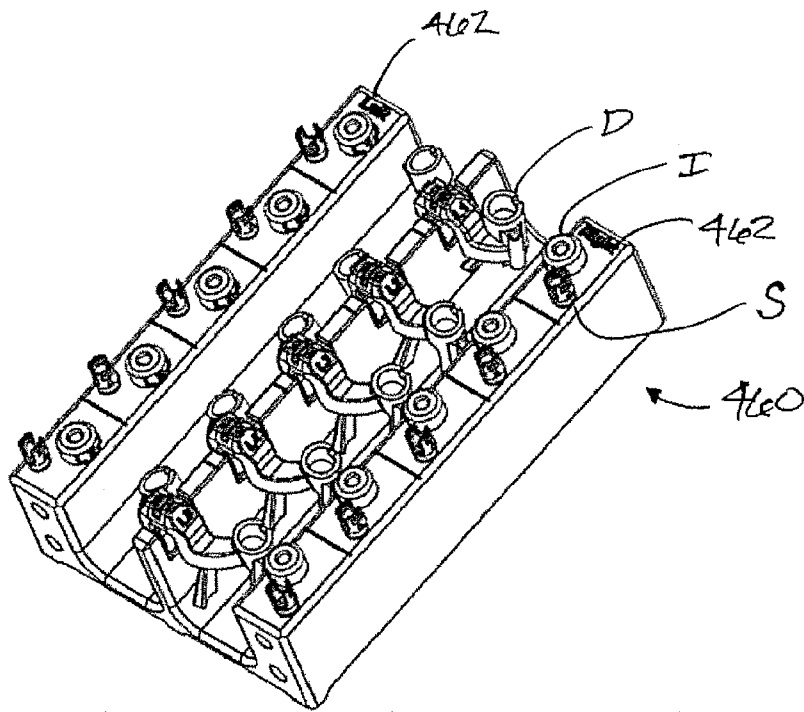


FIG. 47D

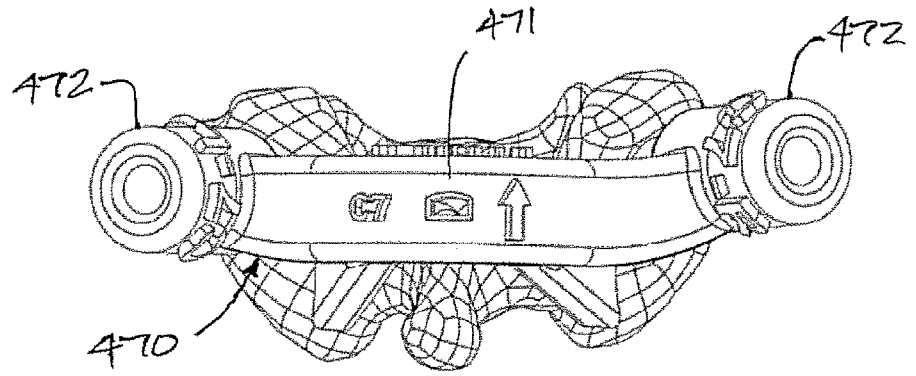


FIG. 48A

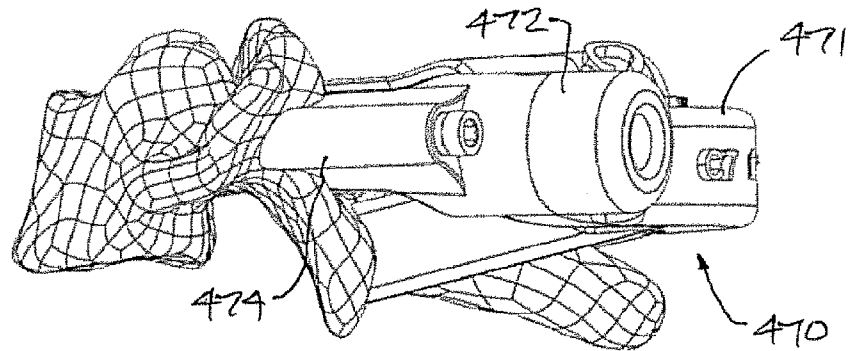


FIG. 48B

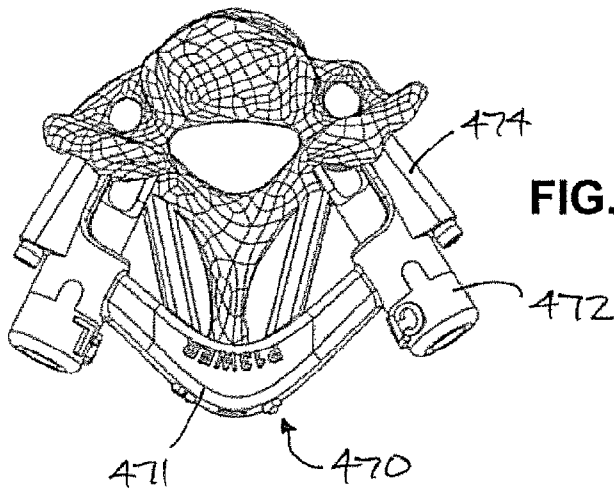
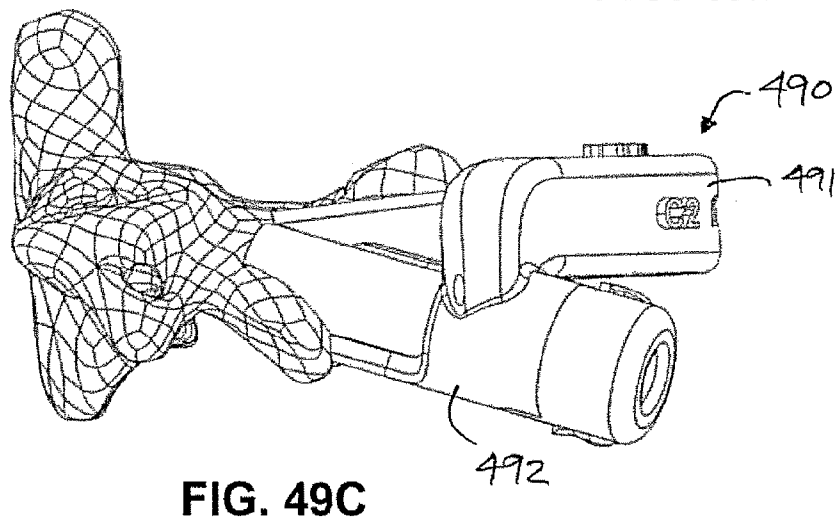
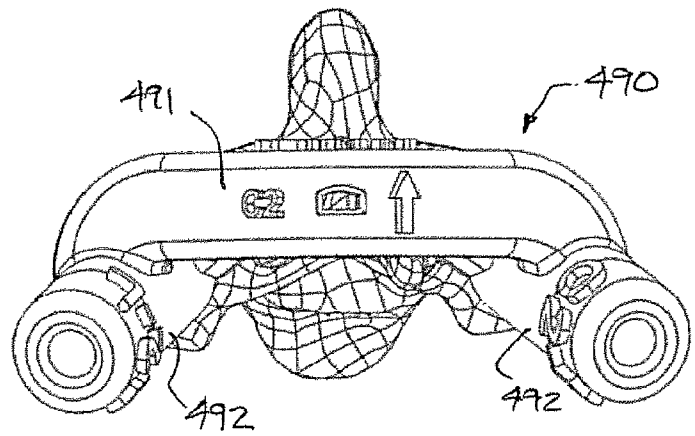
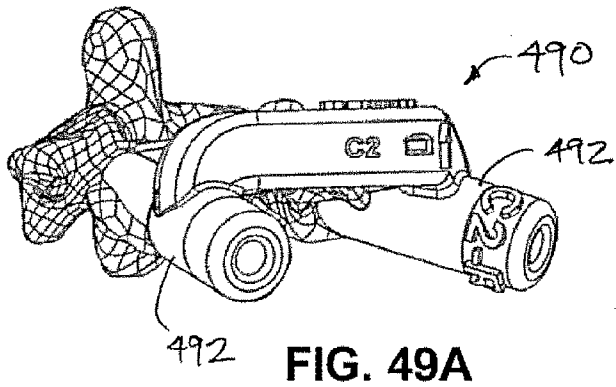


FIG. 48C



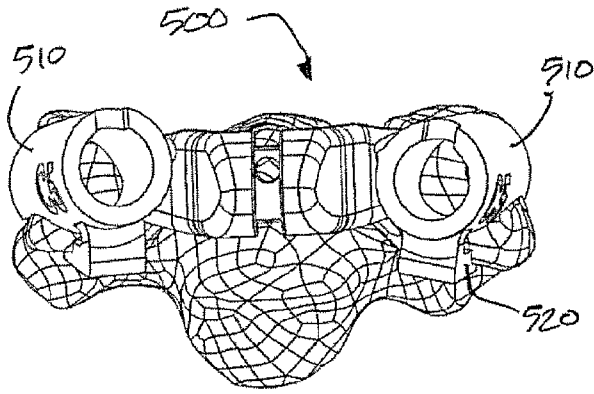


FIG. 50A

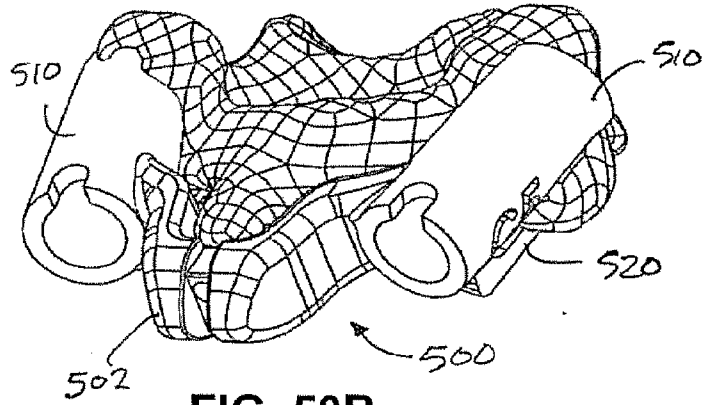


FIG. 50B

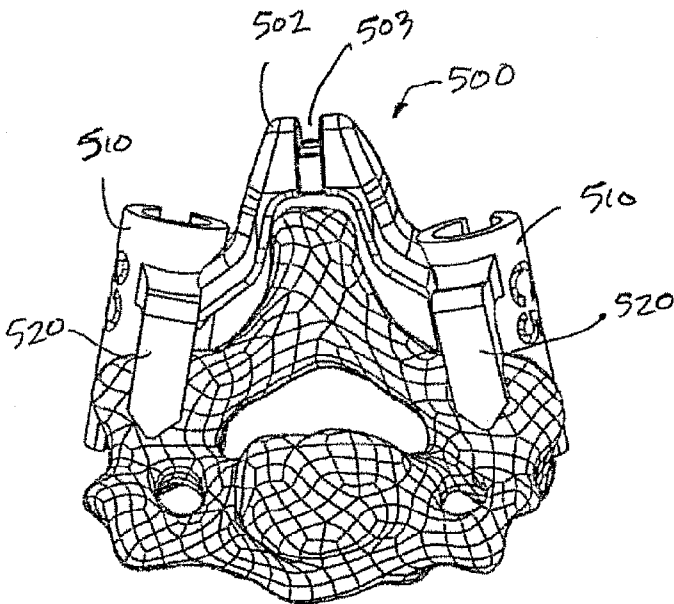


FIG. 50C

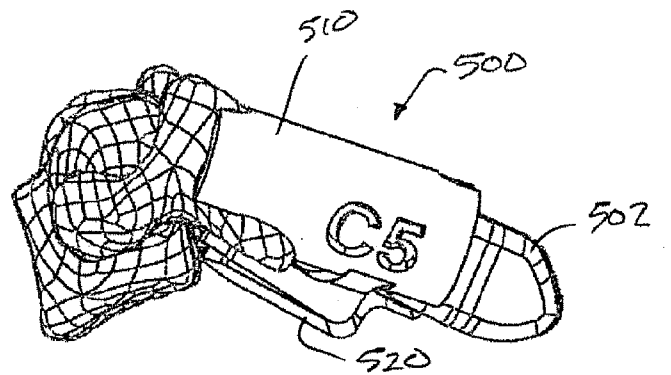


FIG. 50D

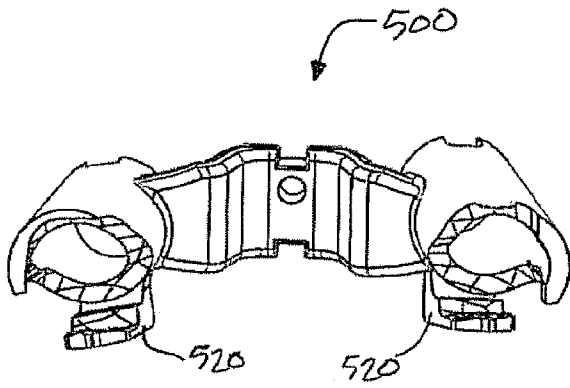


FIG. 51A

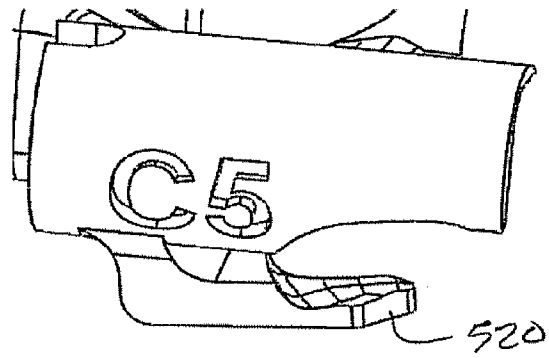


FIG. 51B

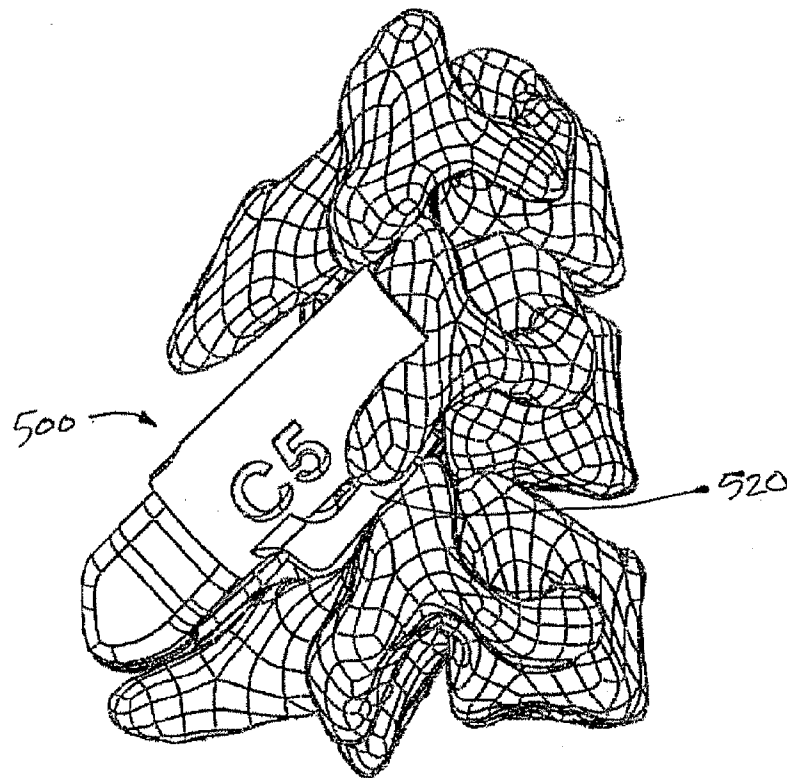


FIG. 51C

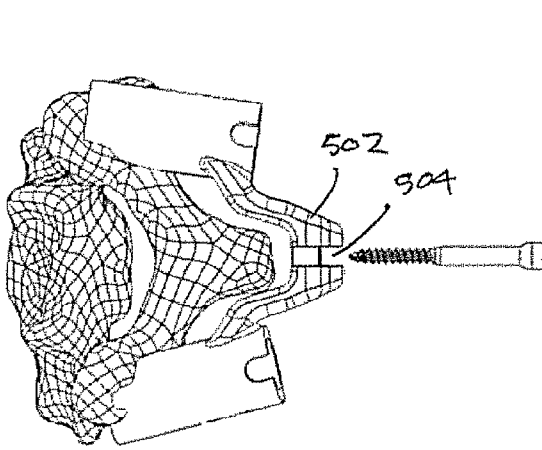


FIG. 52A

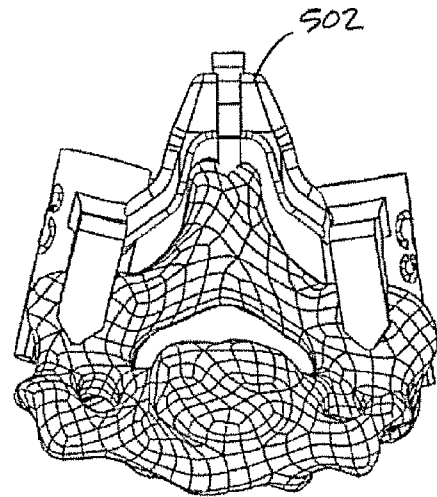


FIG. 52B

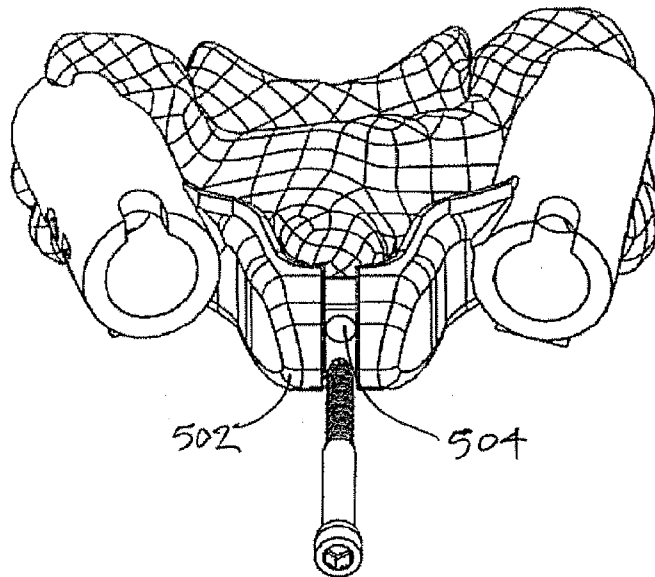


FIG. 52C

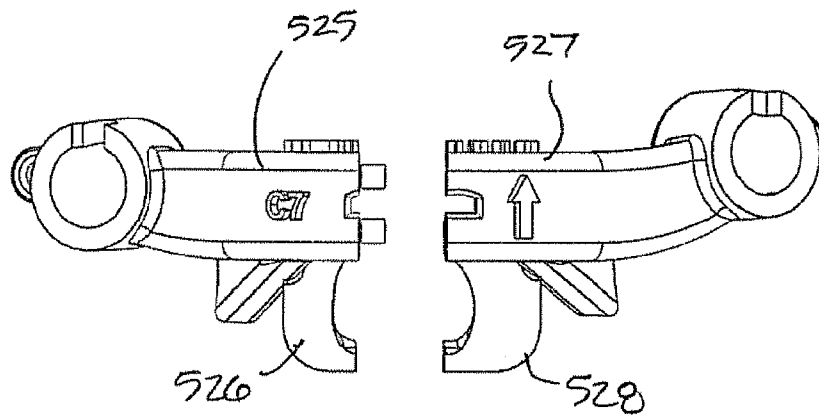


FIG. 53A

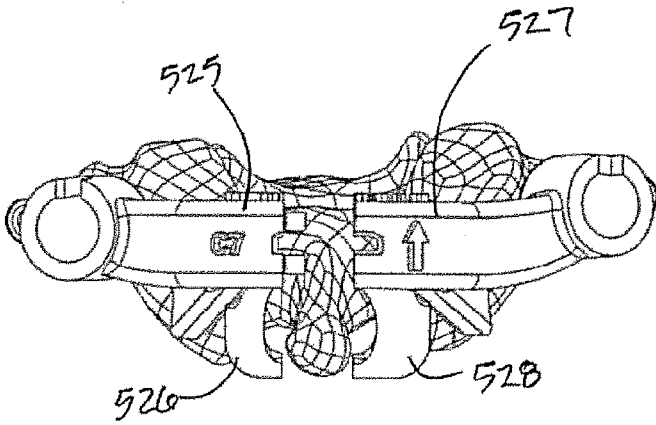


FIG. 53B

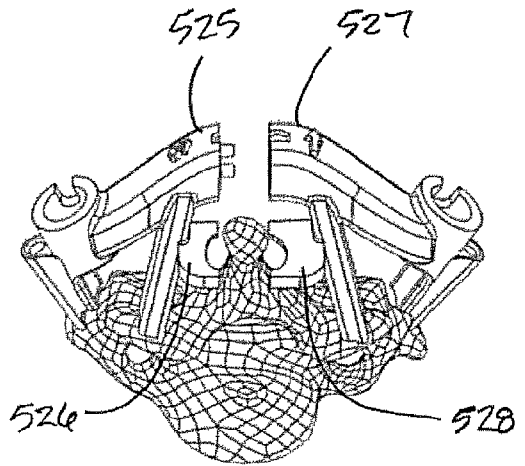


FIG. 53C

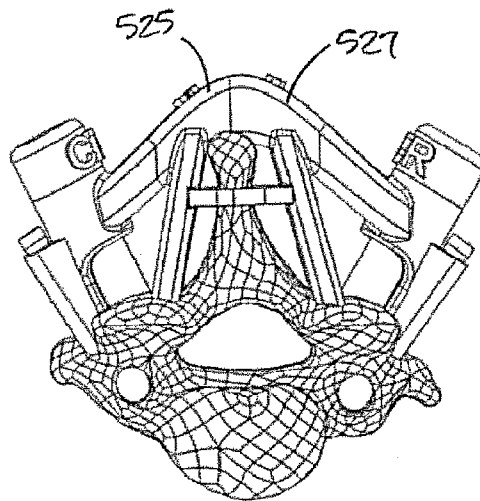


FIG. 53D

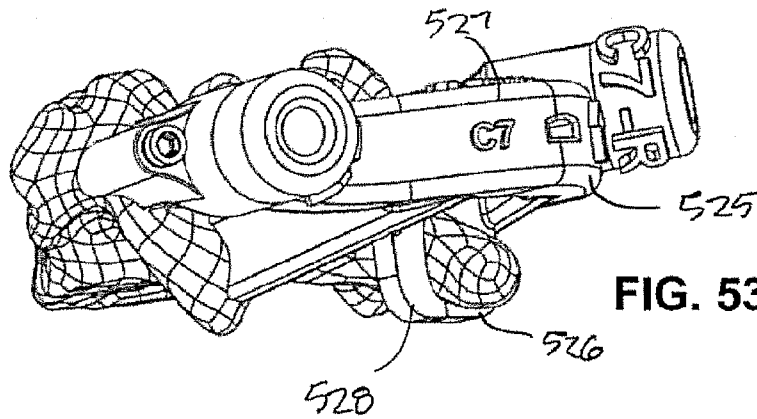


FIG. 53E

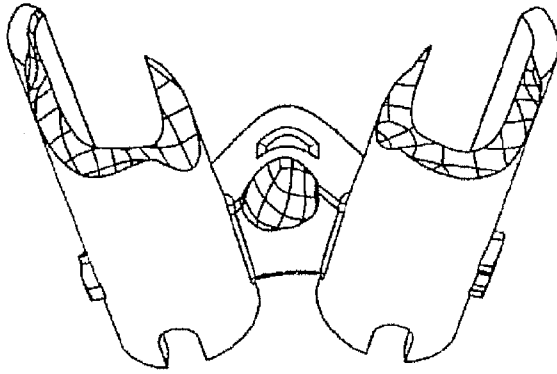


FIG. 54A

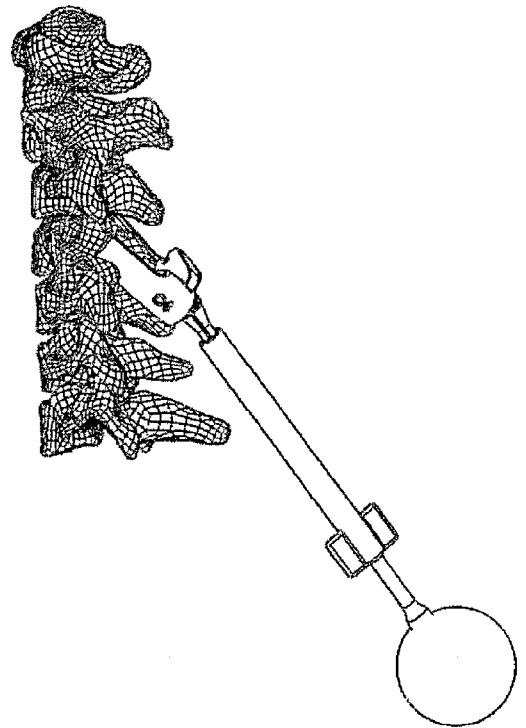


FIG. 54B

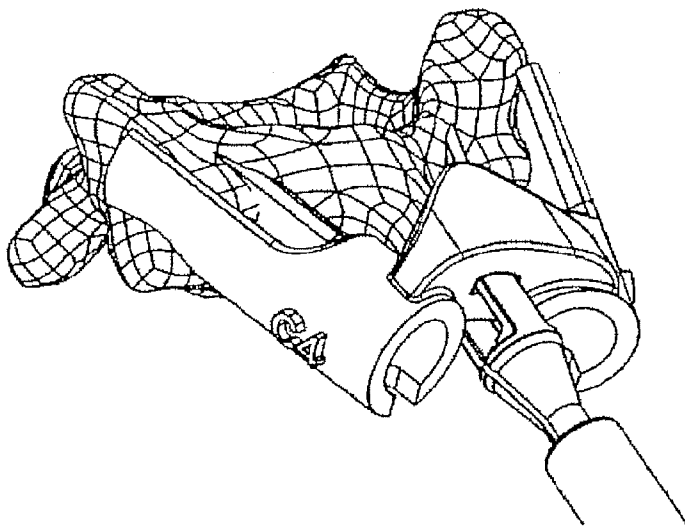


FIG. 54C

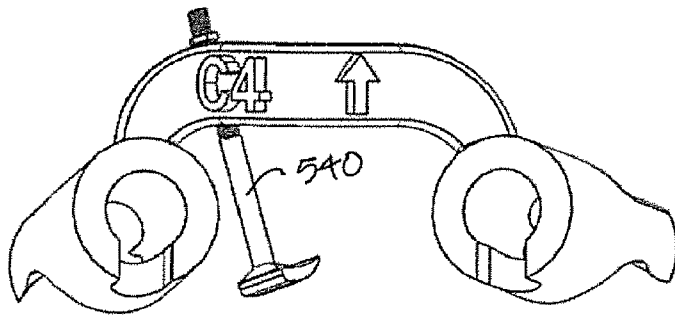


FIG. 55A

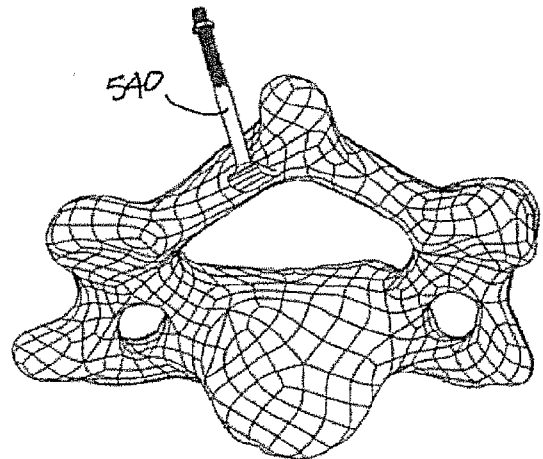


FIG. 55B

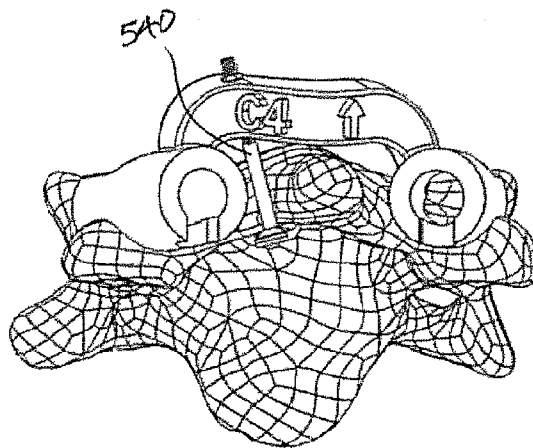


FIG. 55C

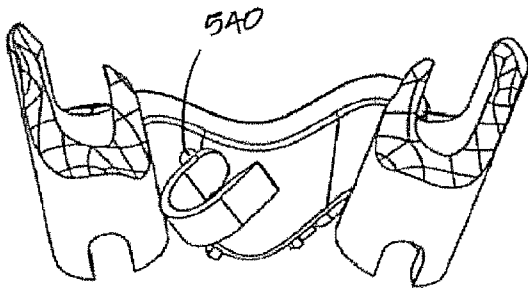


FIG. 56A

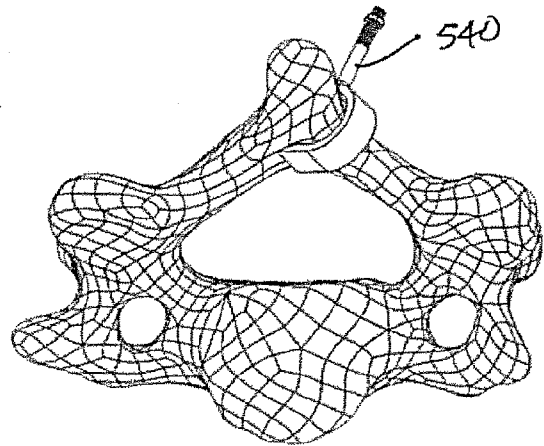


FIG. 56B

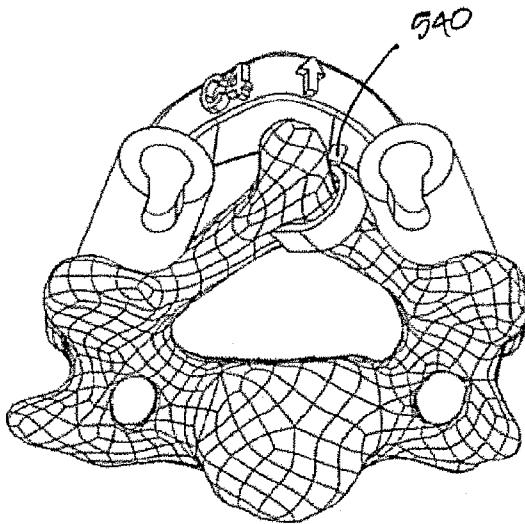


FIG. 56C

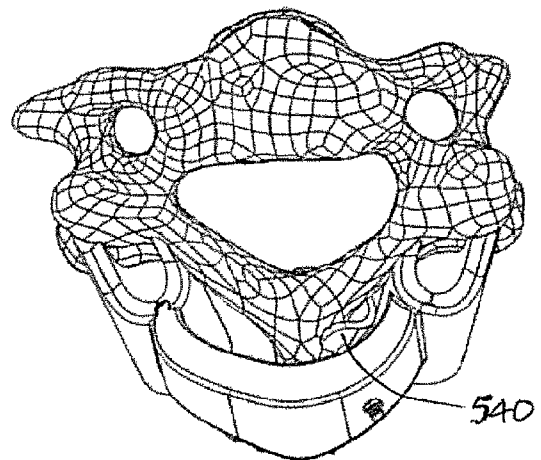


FIG. 56D

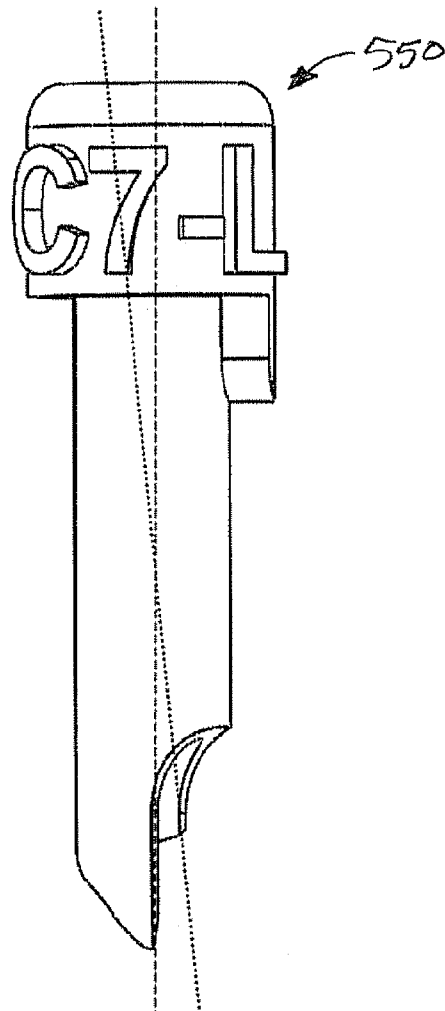


FIG. 57

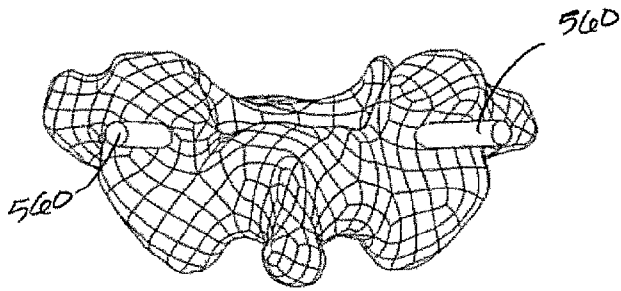


FIG. 58A

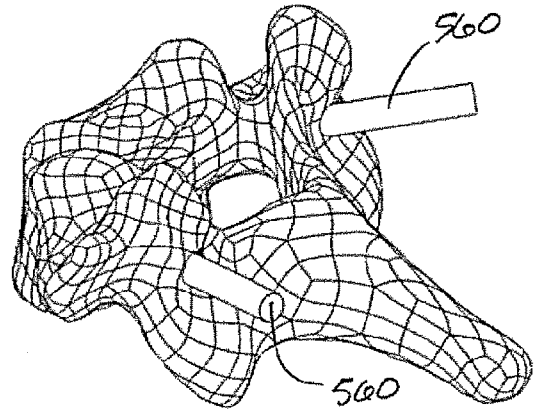


FIG. 58B

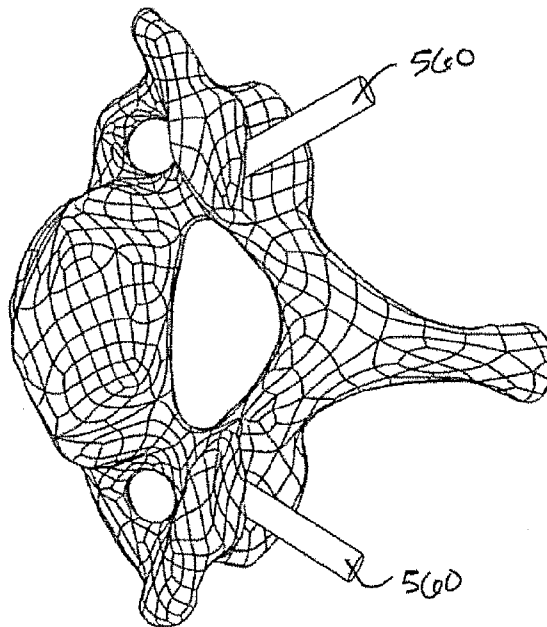


FIG. 58C

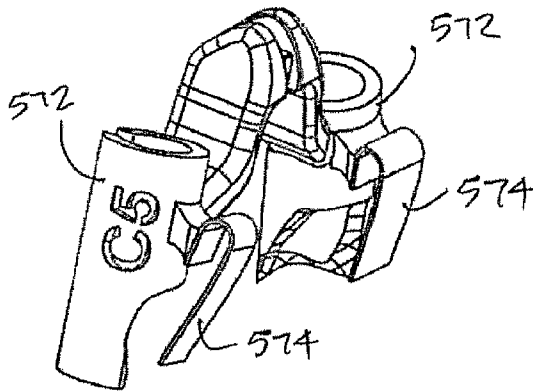


FIG. 59A

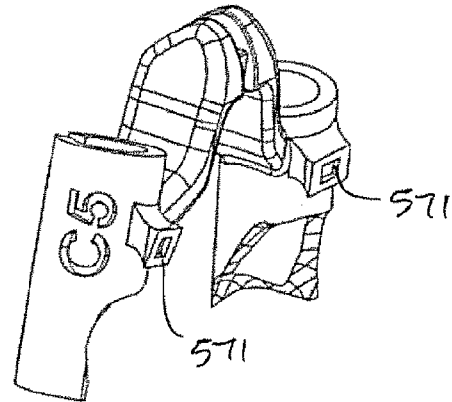


FIG. 59B

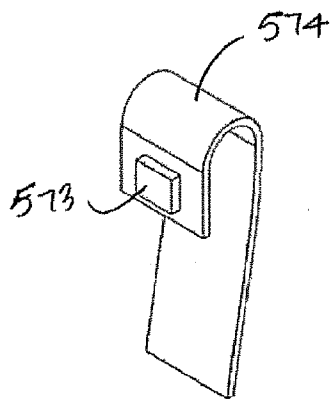


FIG. 59C

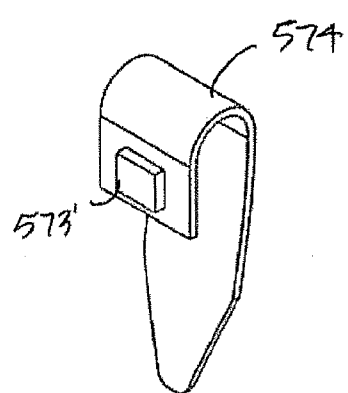


FIG. 59D

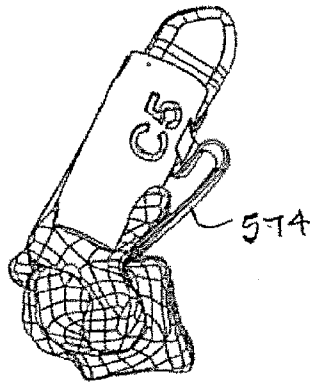


FIG. 60A

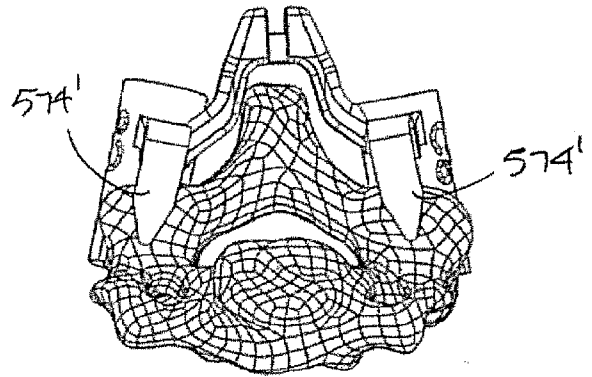


FIG. 60B

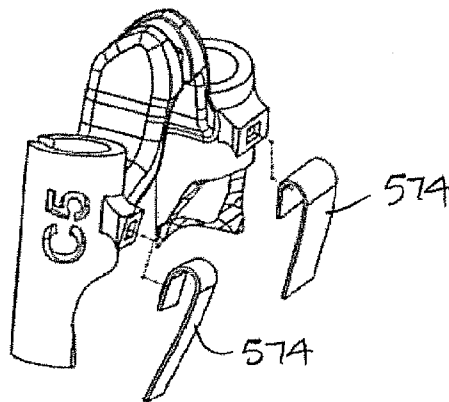


FIG. 60C

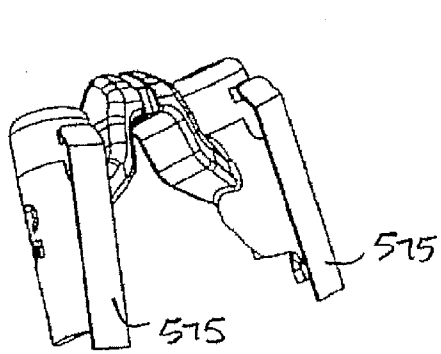


FIG. 61A

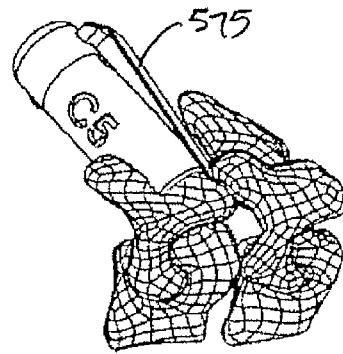


FIG. 61B

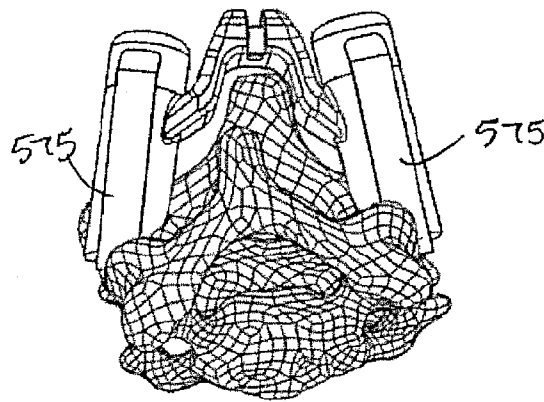


FIG. 61C

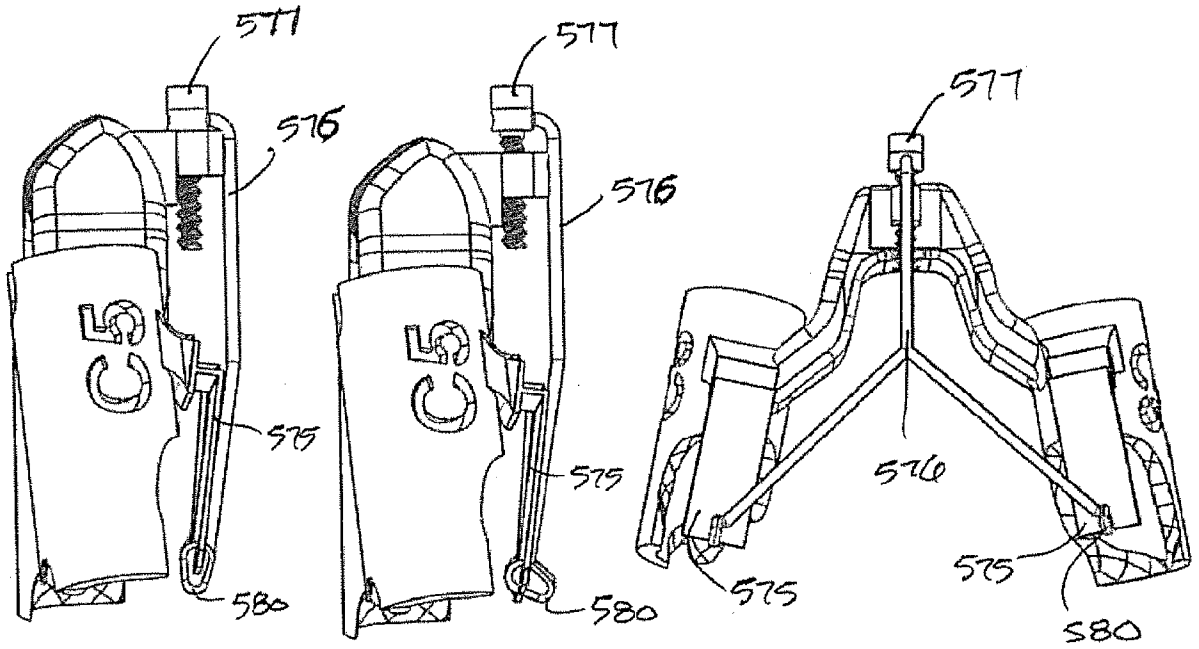


FIG. 62A

FIG. 62B

FIG. 62C

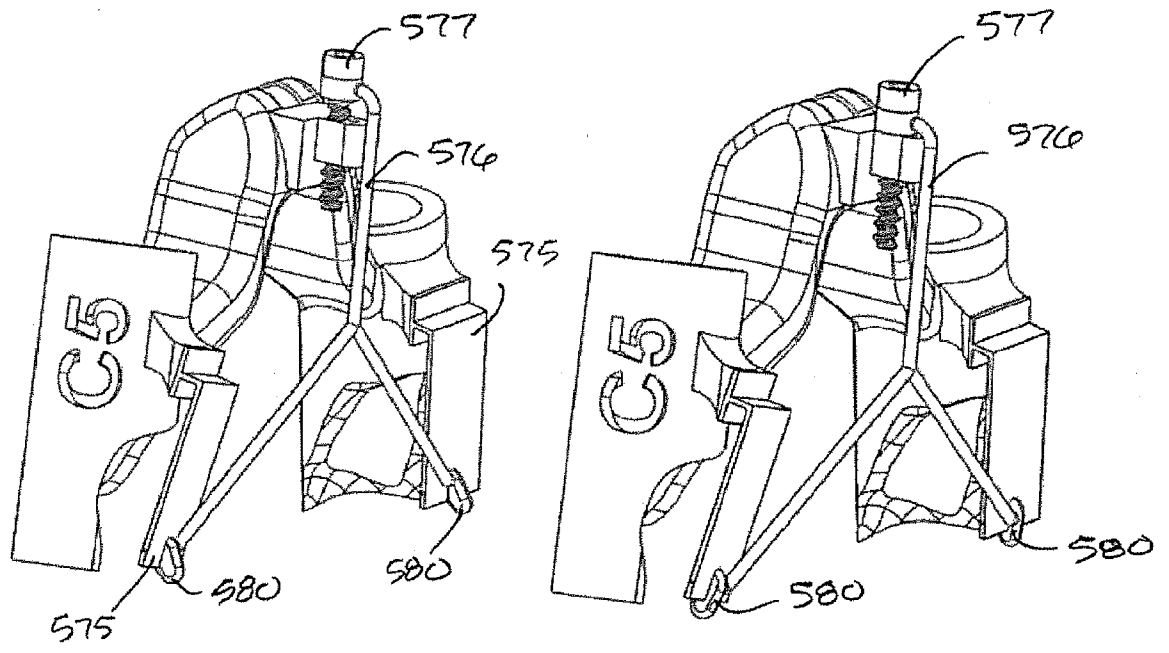
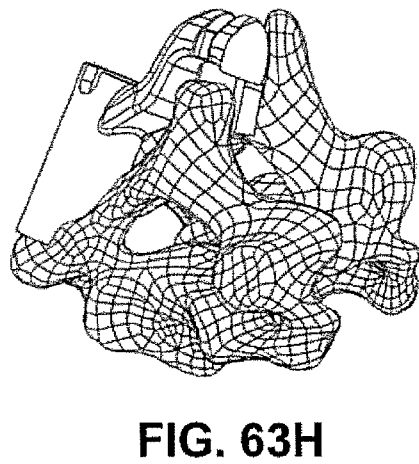
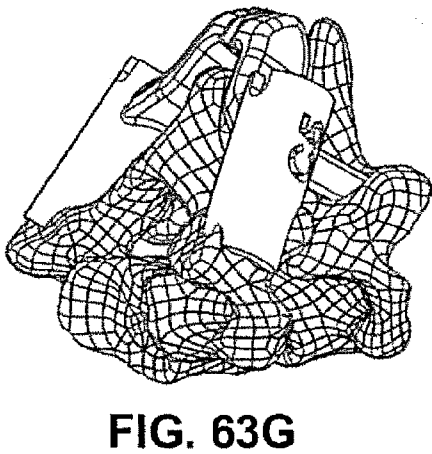
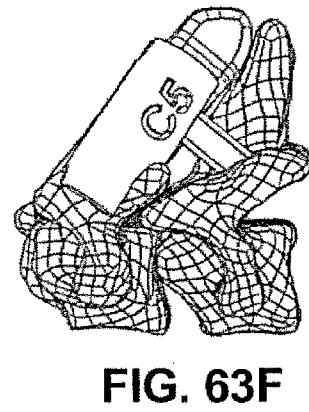
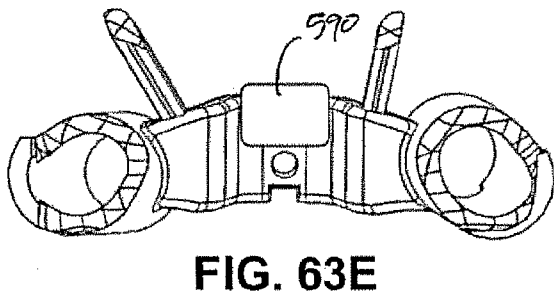
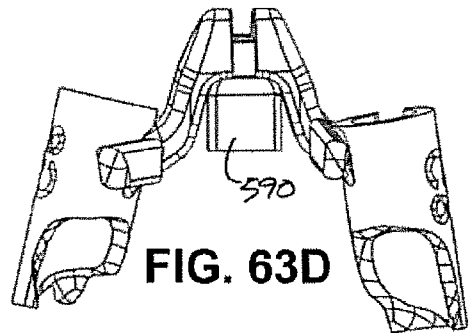
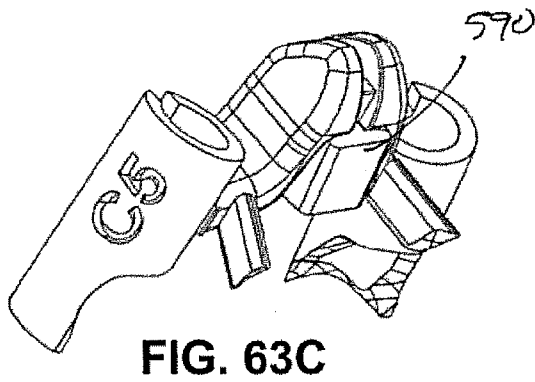
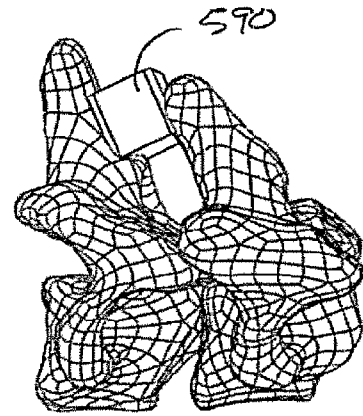
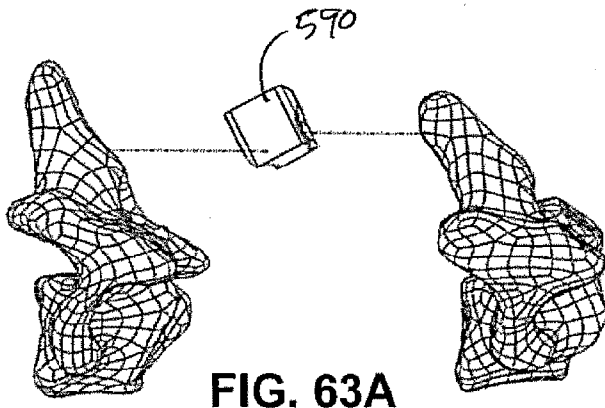


FIG. 62D

FIG. 62E



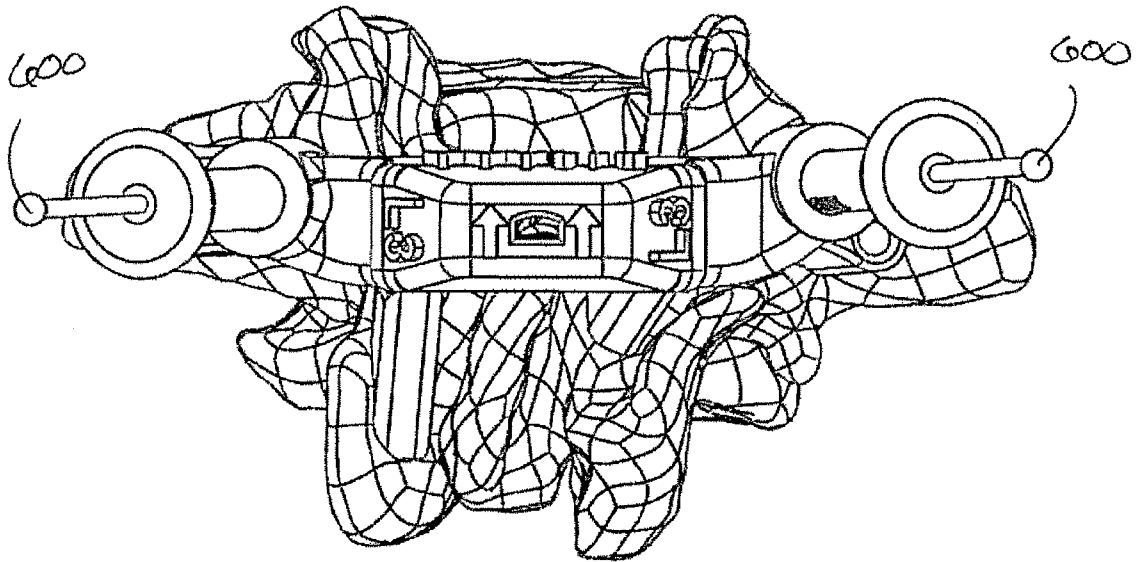


FIG. 64

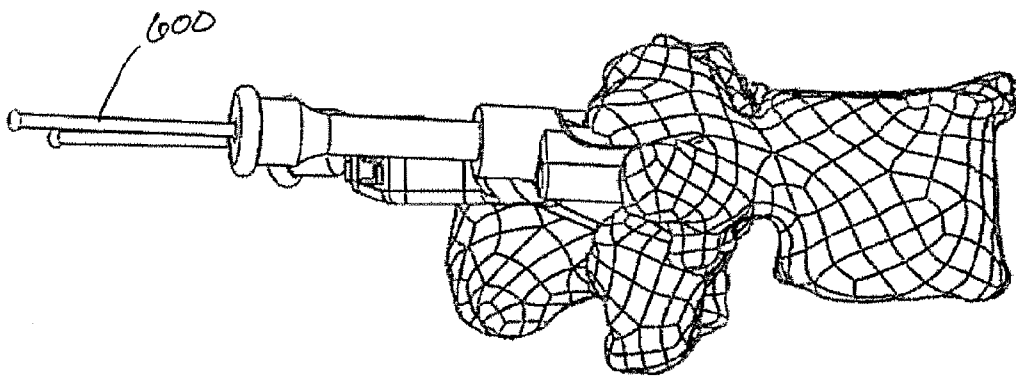


FIG. 65

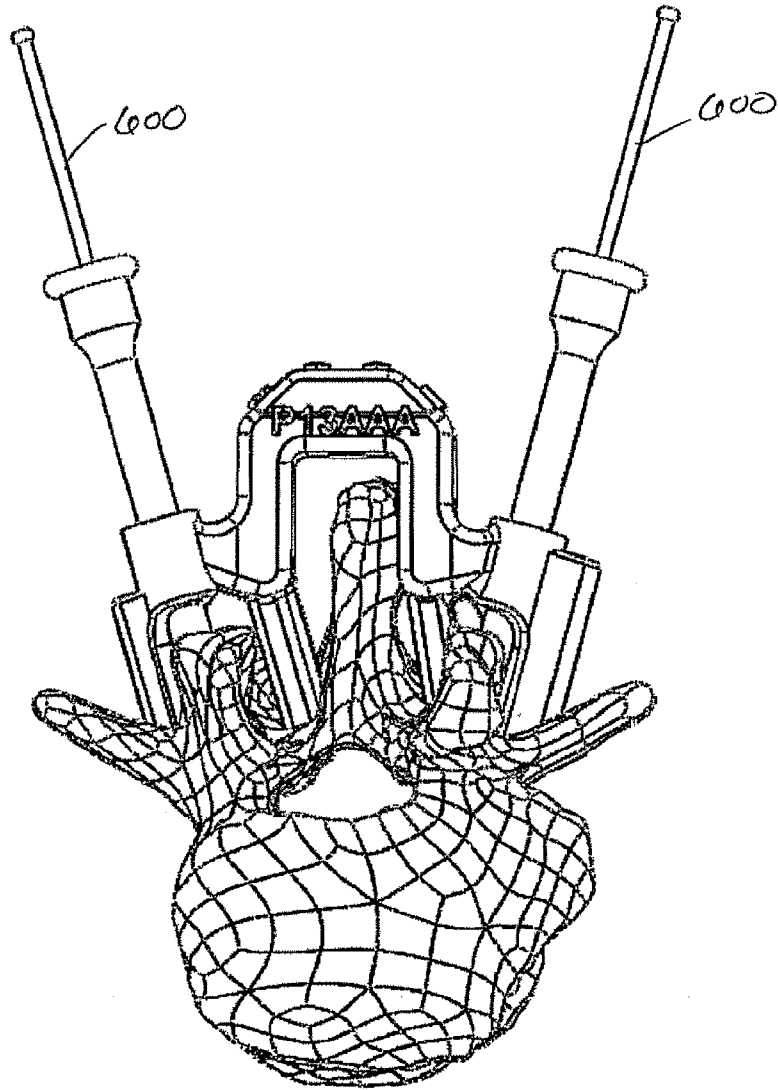


FIG. 66

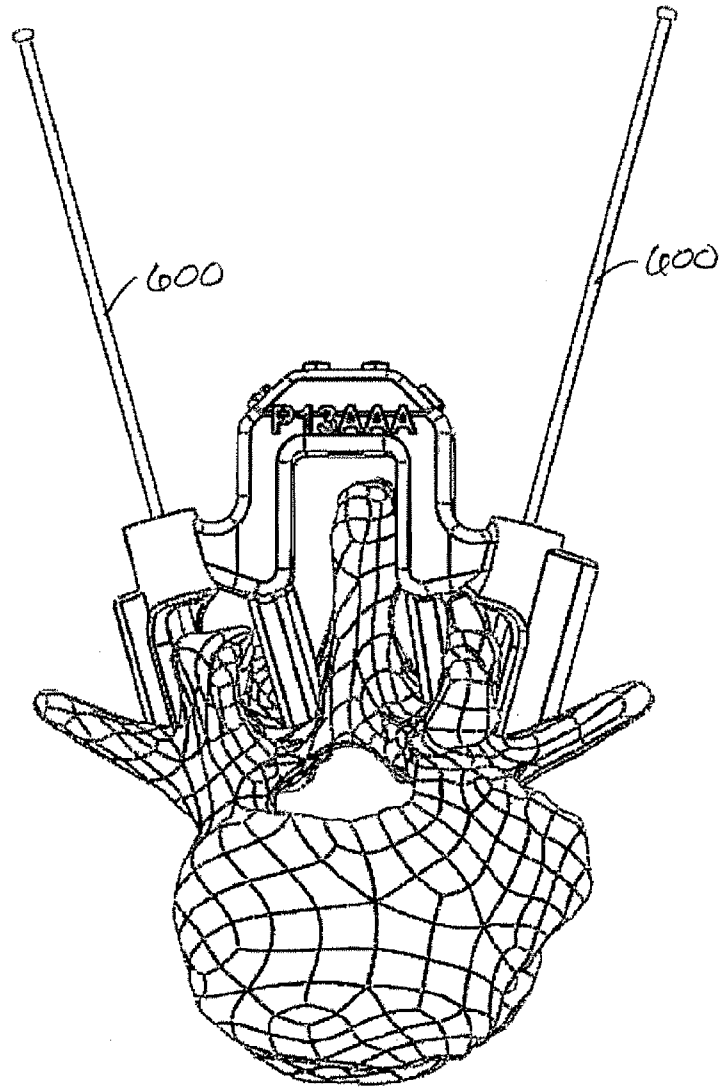


FIG. 67

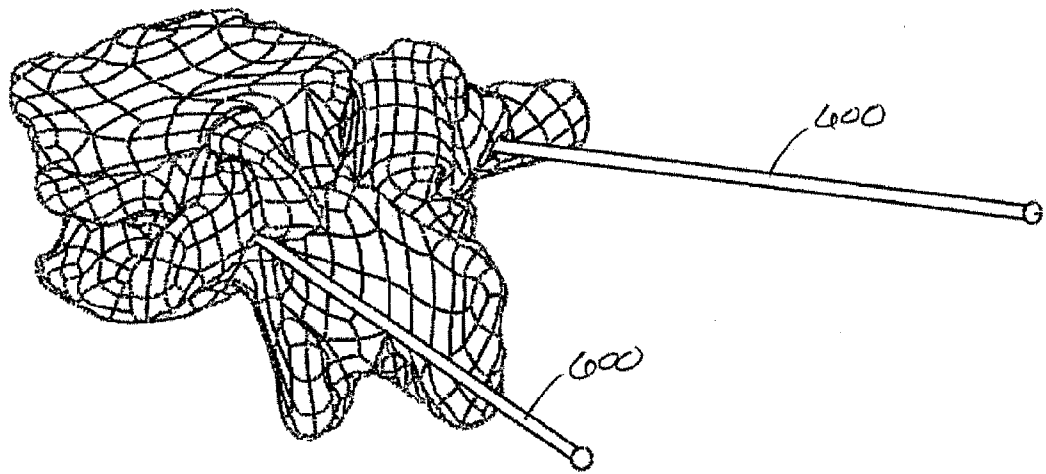


FIG. 68

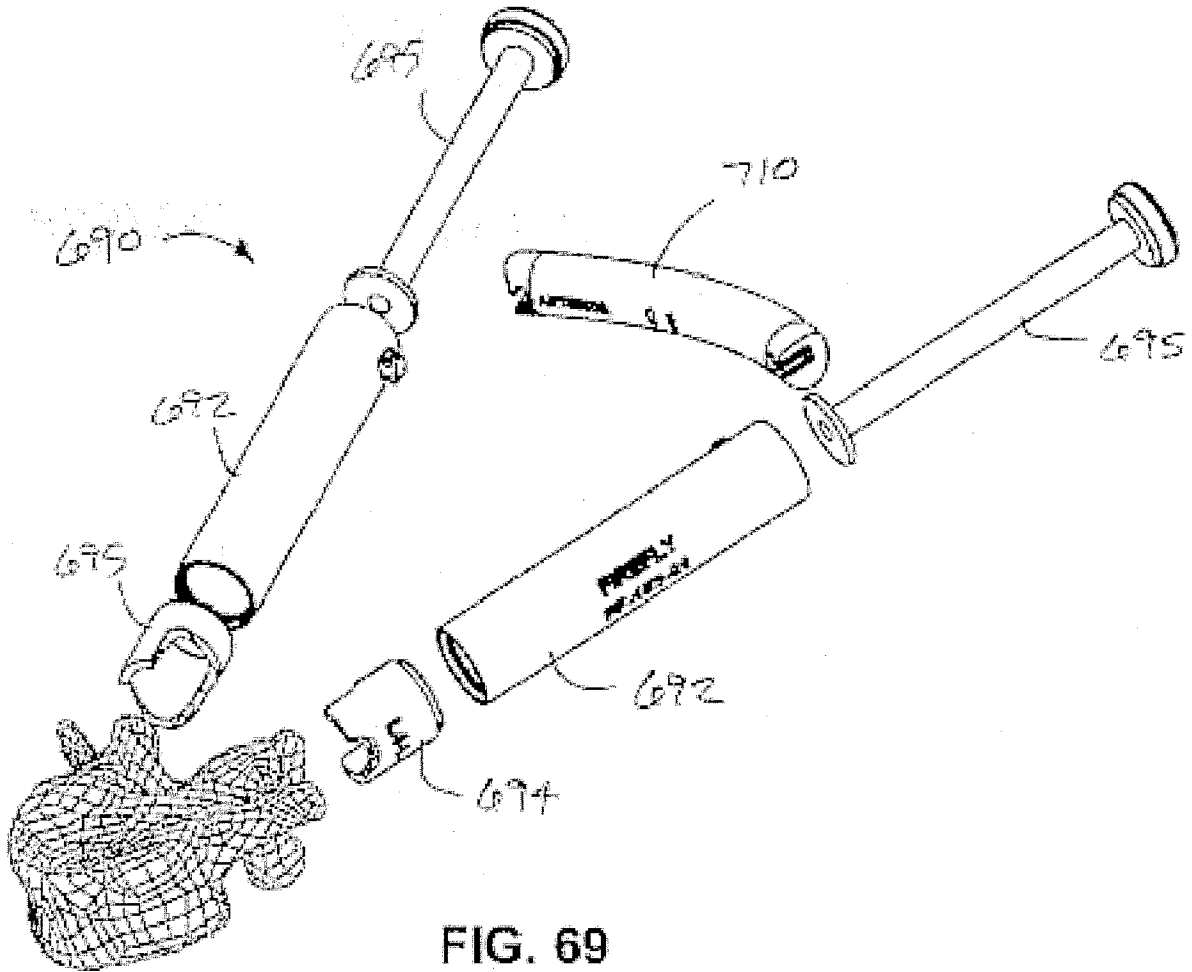


FIG. 69

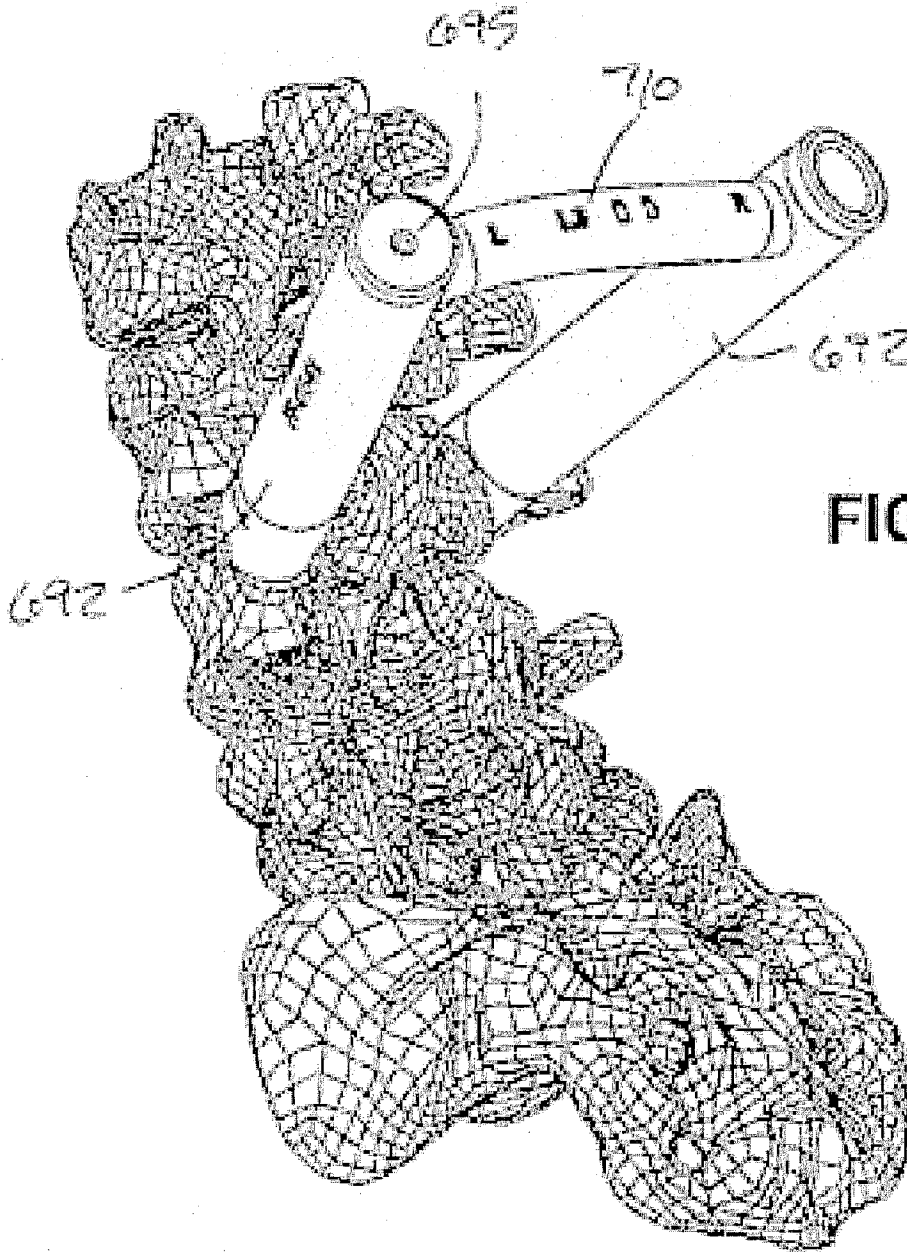


FIG. 70A

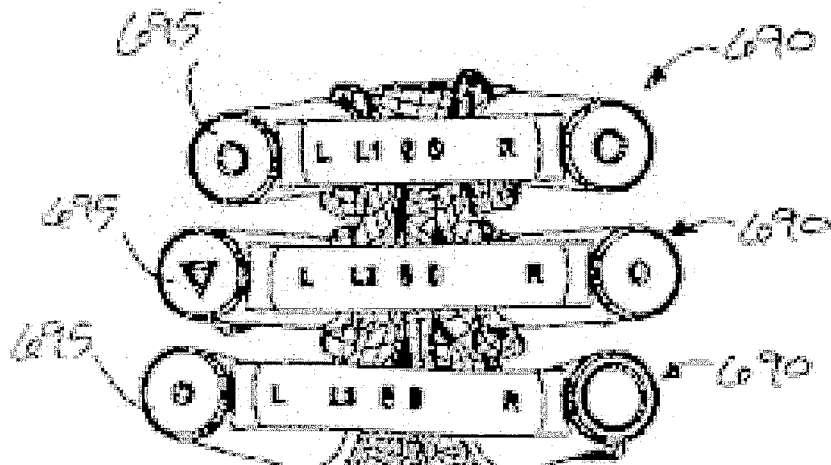
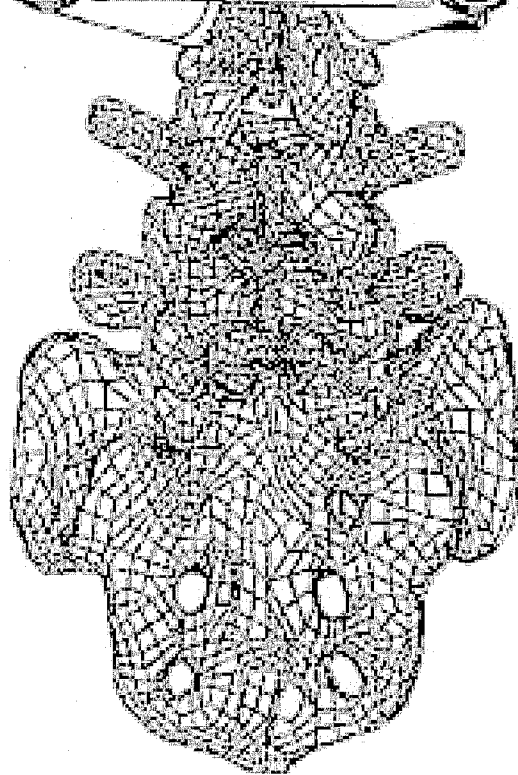


FIG. 70B



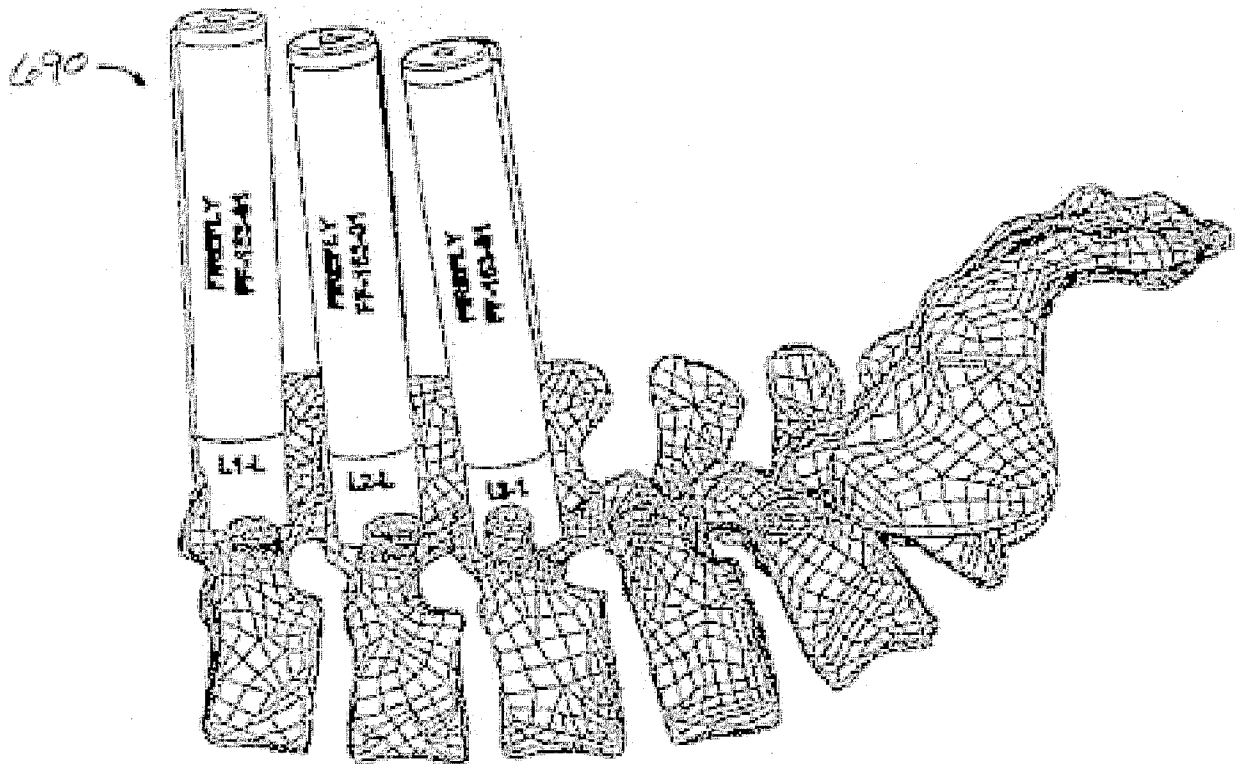


FIG. 71

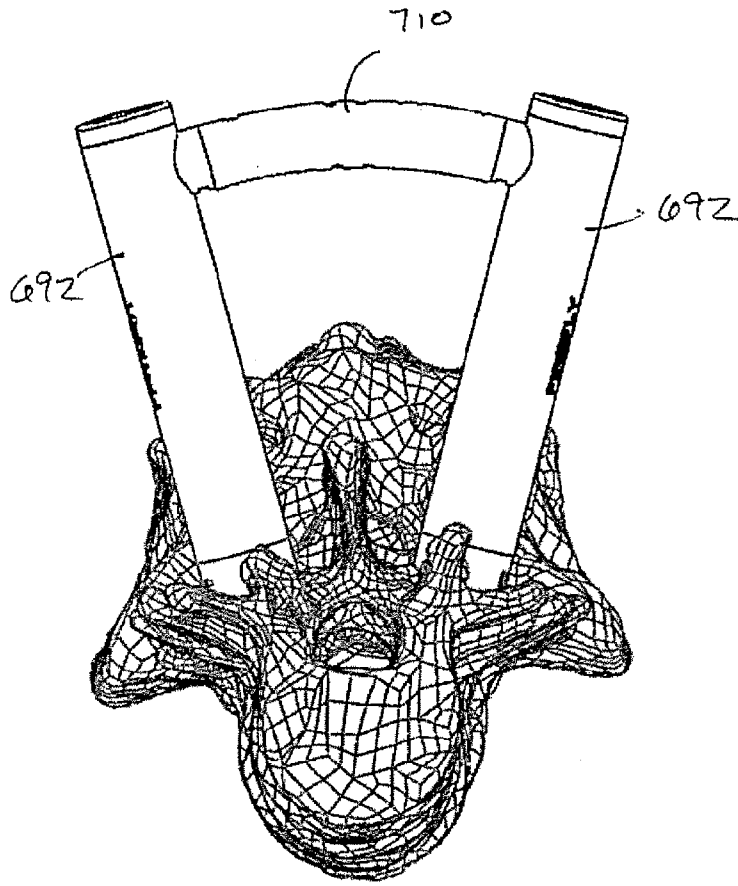


FIG. 72

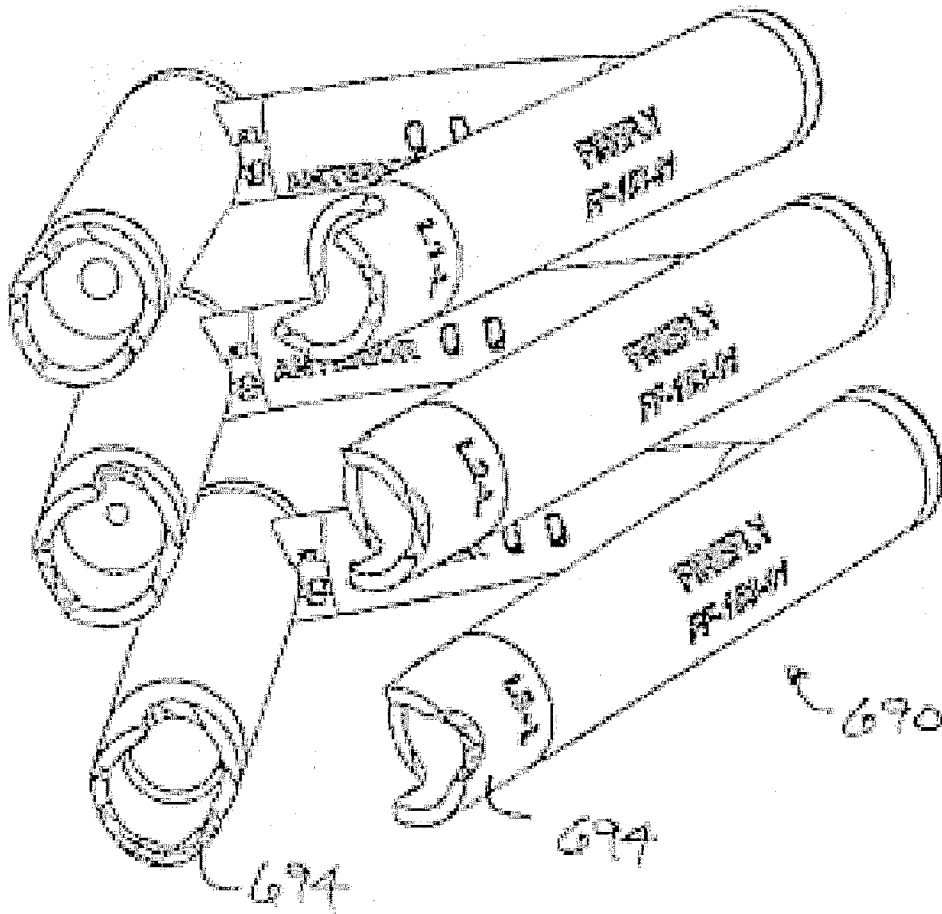


FIG. 73

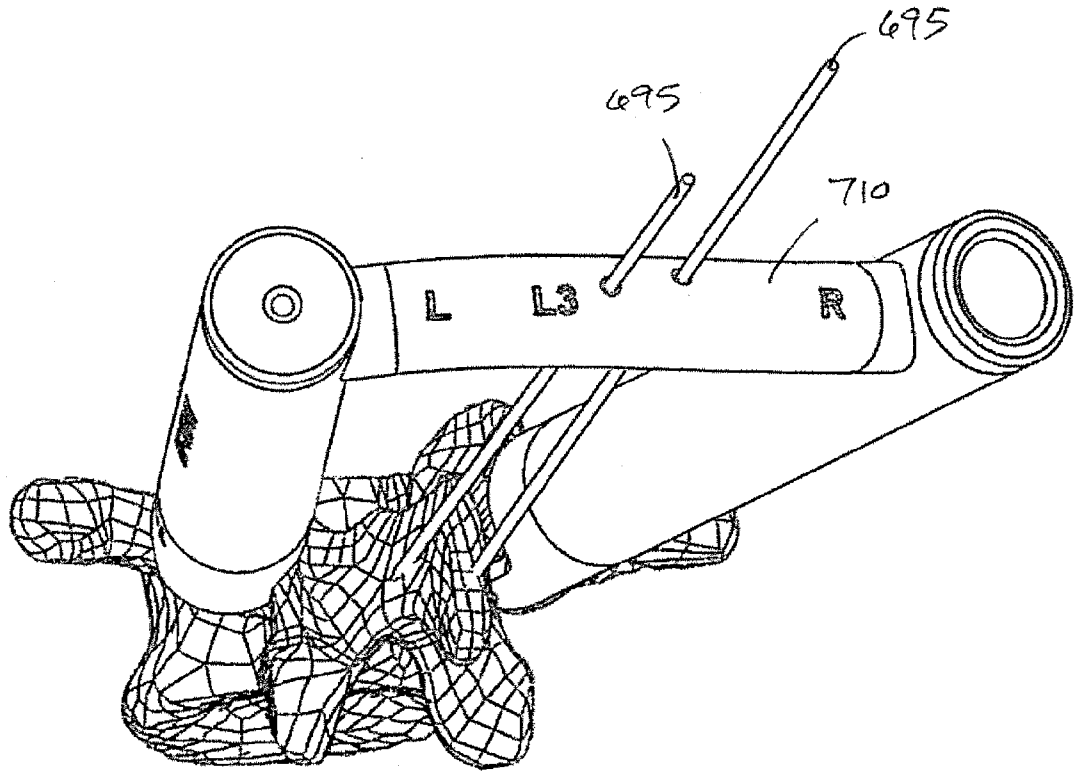


FIG. 74

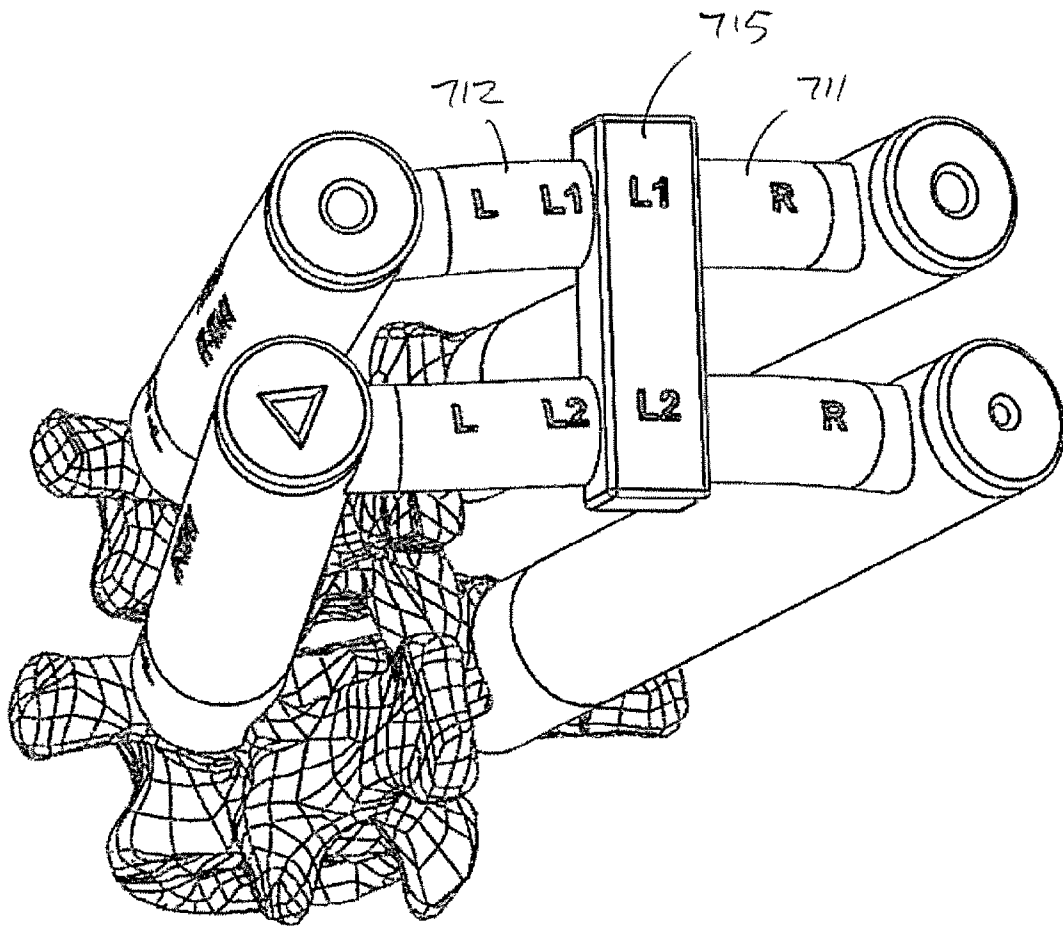


FIG. 75

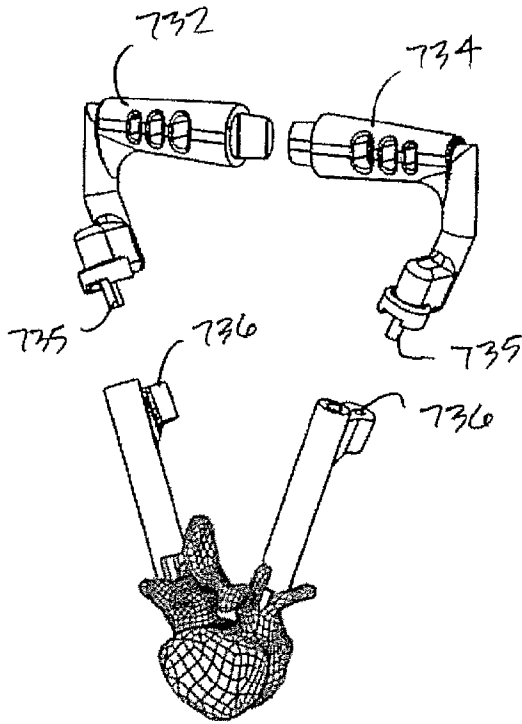


FIG. 76A

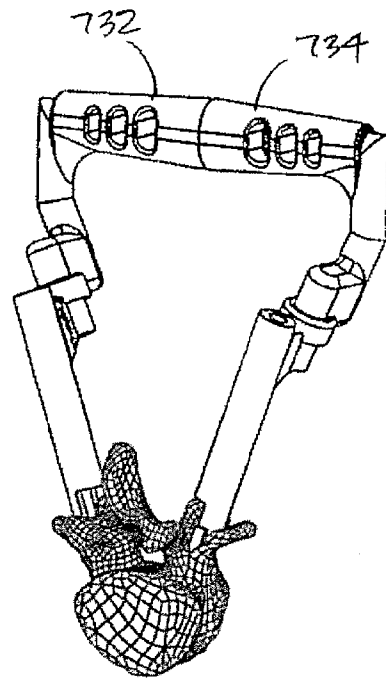


FIG. 76B

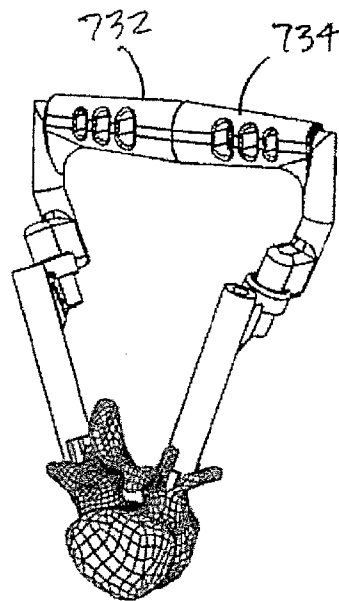


FIG. 76C

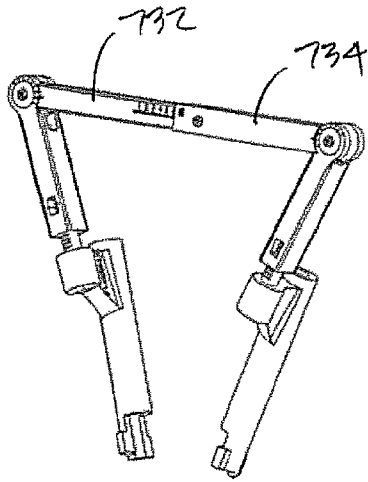


FIG. 77A

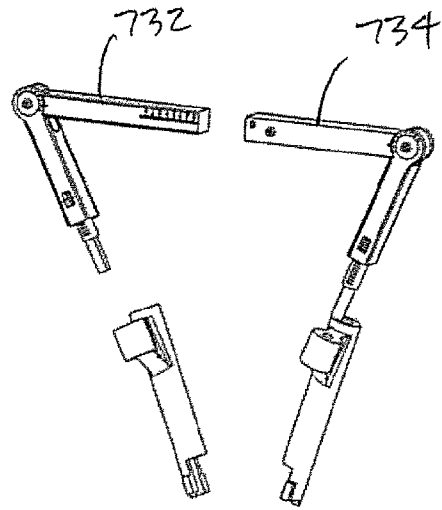


FIG. 77B

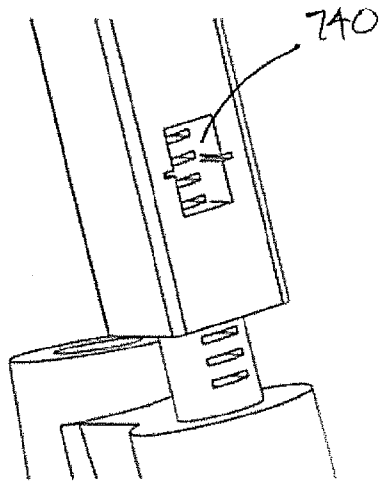


FIG. 77C

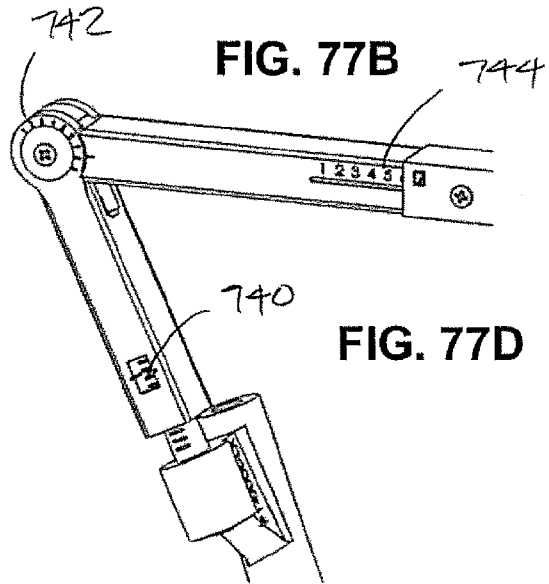


FIG. 77D

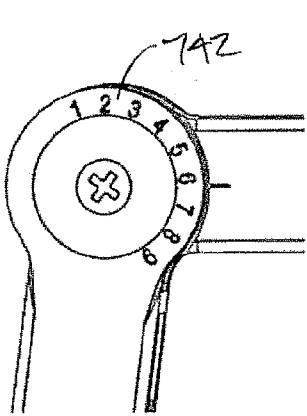


FIG. 77E

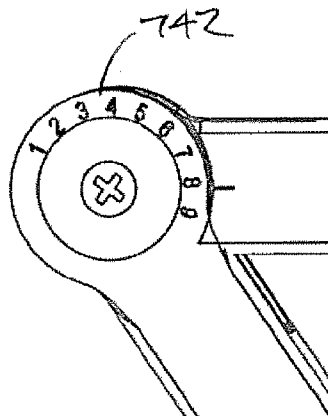


FIG. 77F

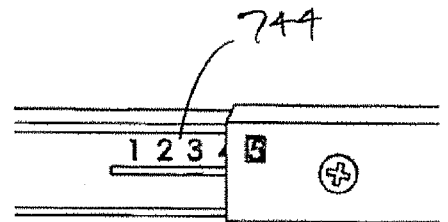


FIG. 77G

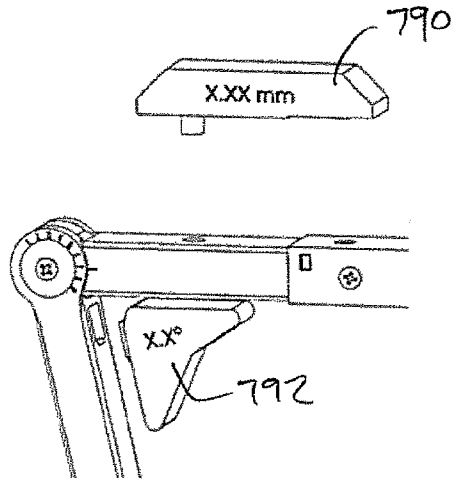


FIG. 78A

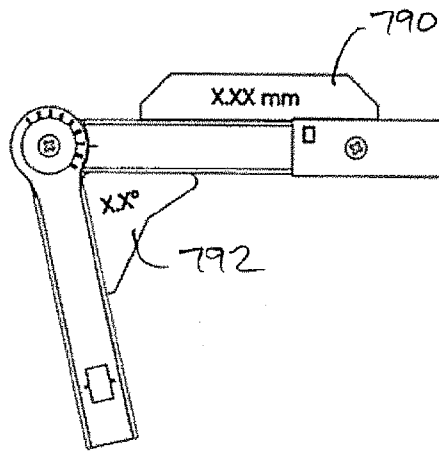


FIG. 78B

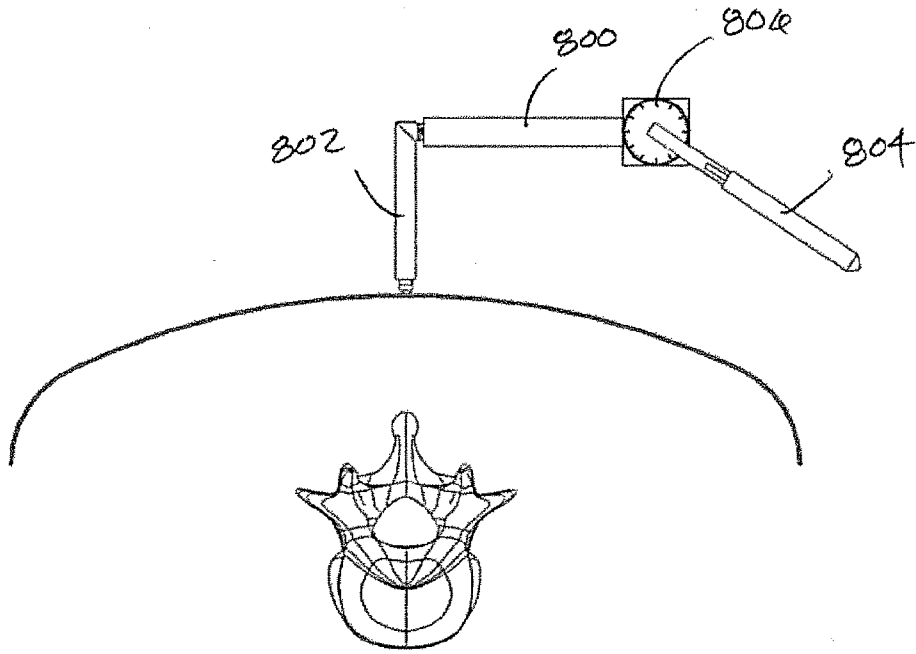


FIG. 79A

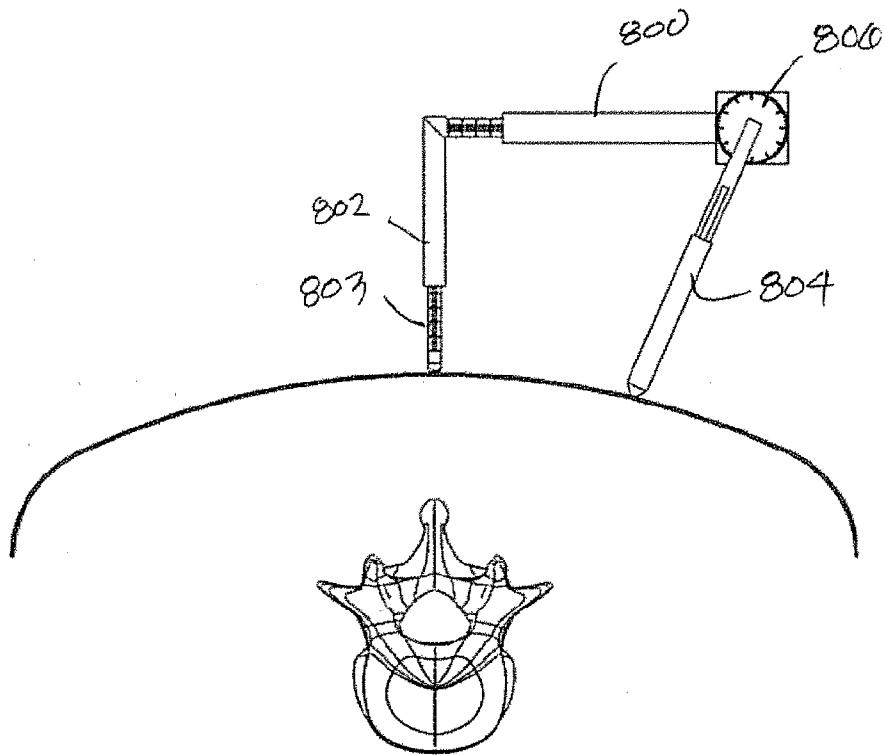


FIG. 79B

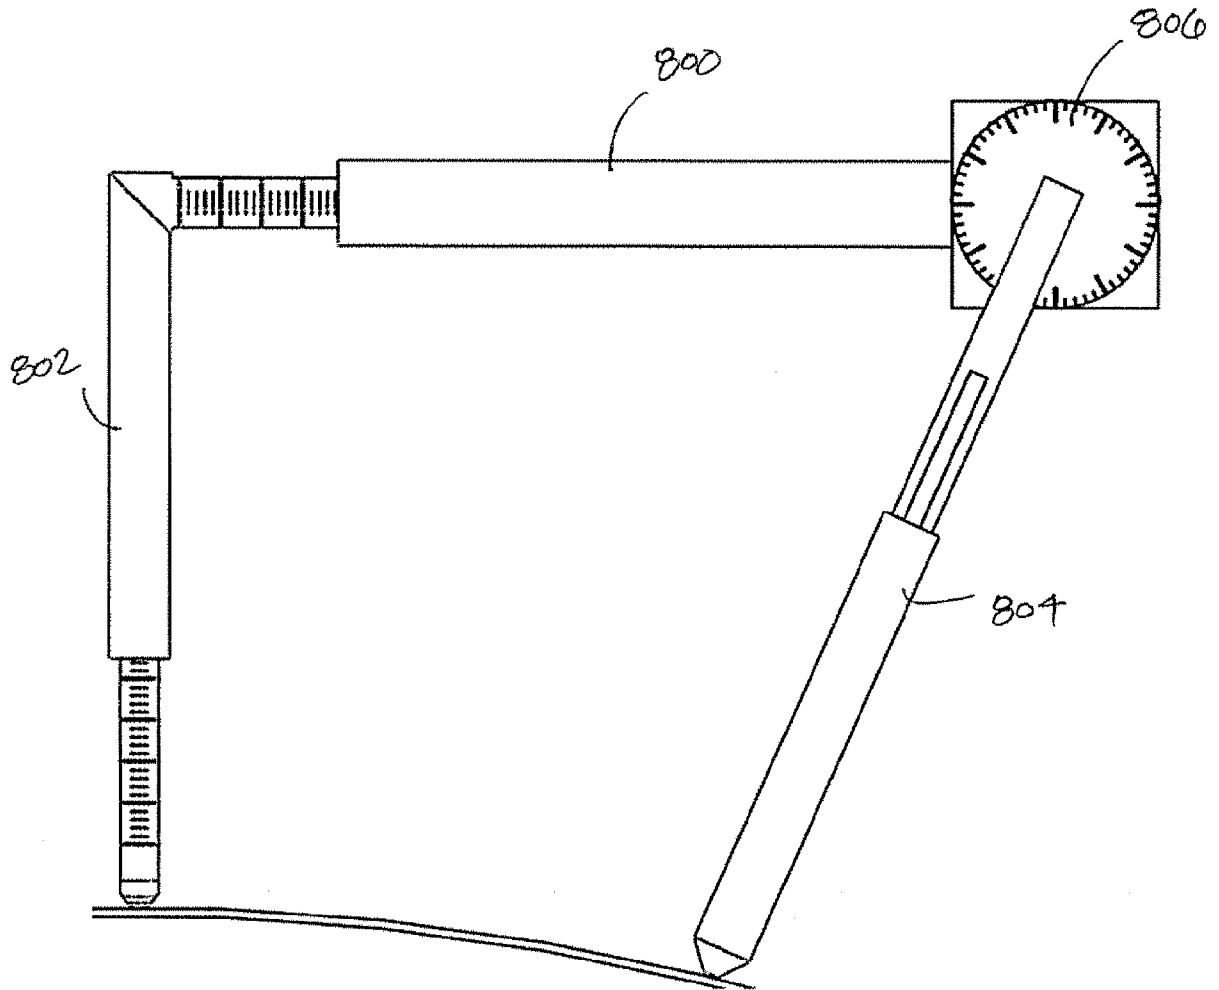


FIG. 80

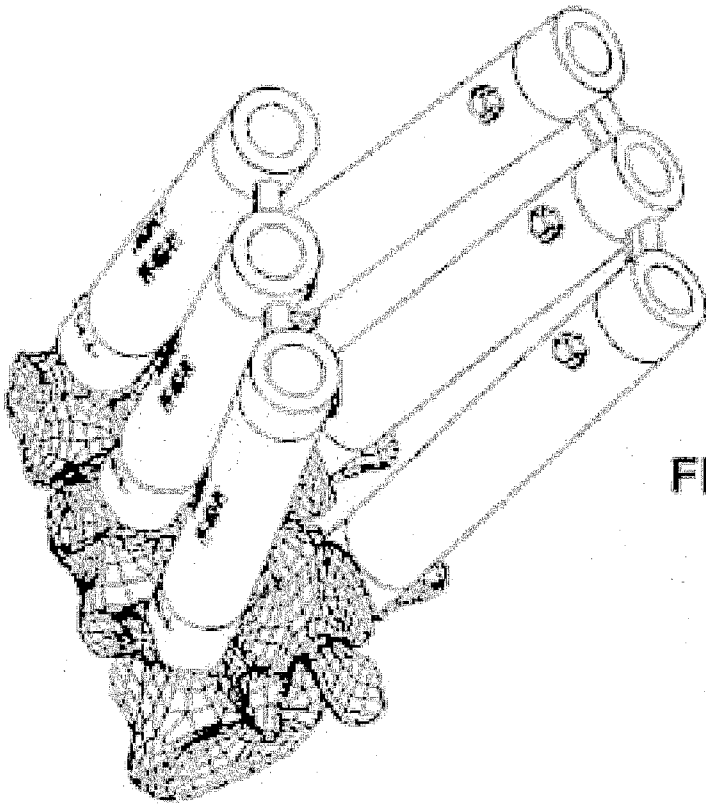


FIG. 81A

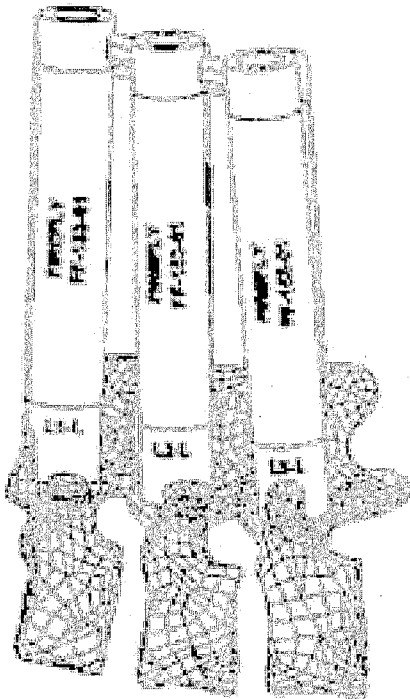


FIG. 81B

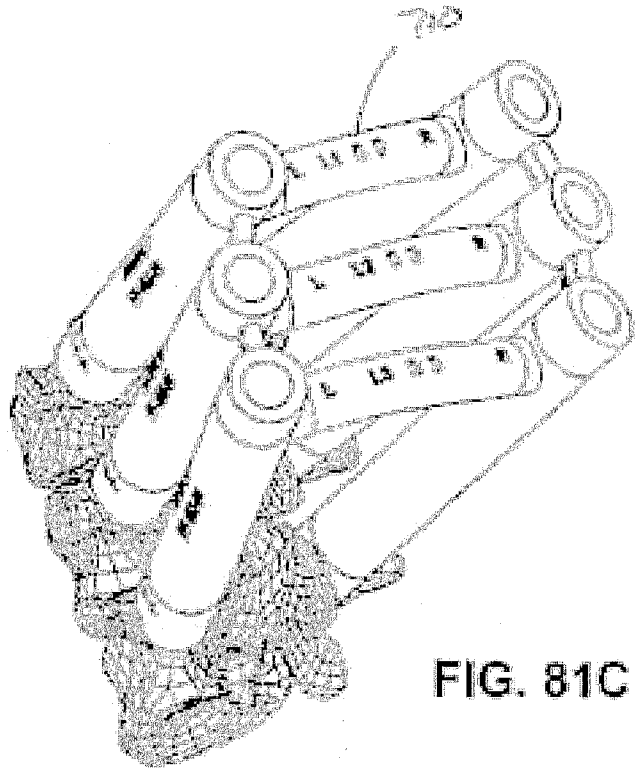


FIG. 81C

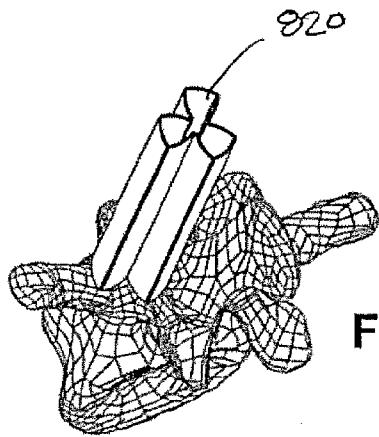


FIG. 82A

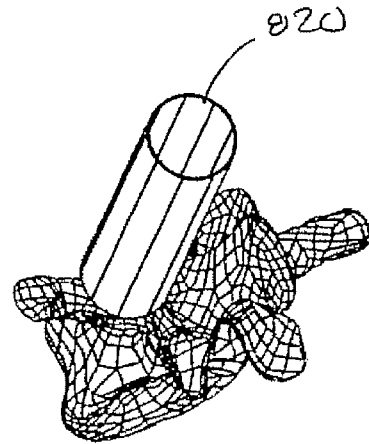


FIG. 82B

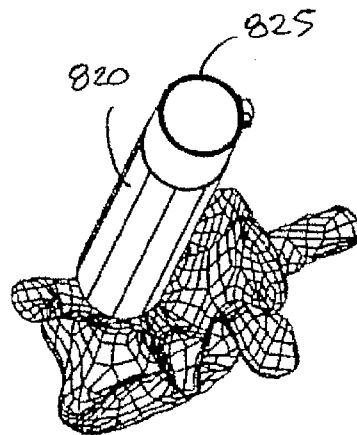


FIG. 82C

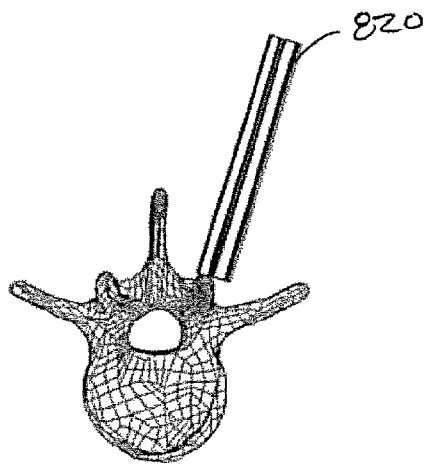


FIG. 83A

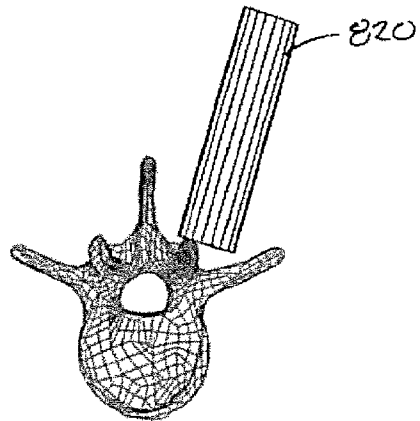


FIG. 83B

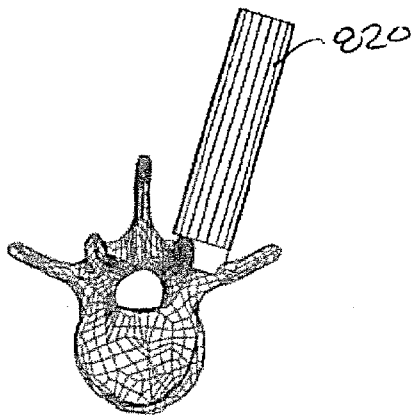


FIG. 83C

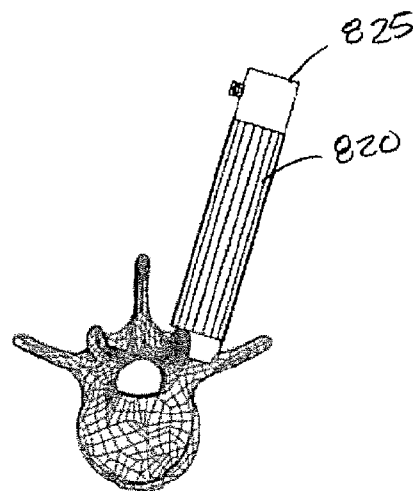


FIG. 83D

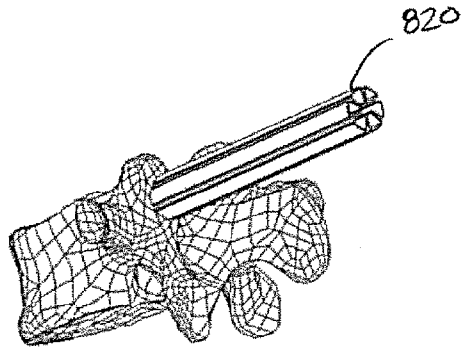


FIG. 84A

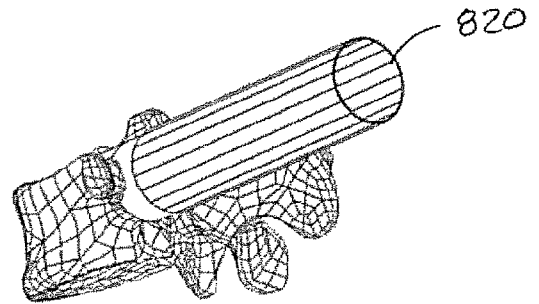


FIG. 84B

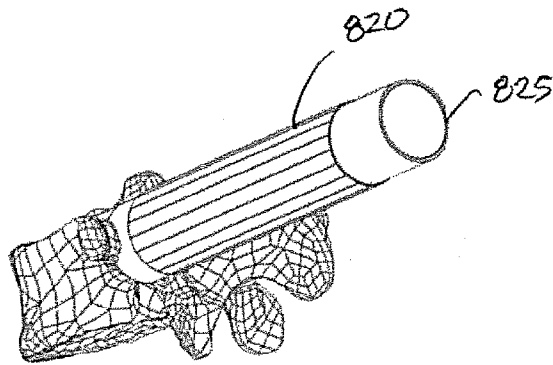


FIG. 84C

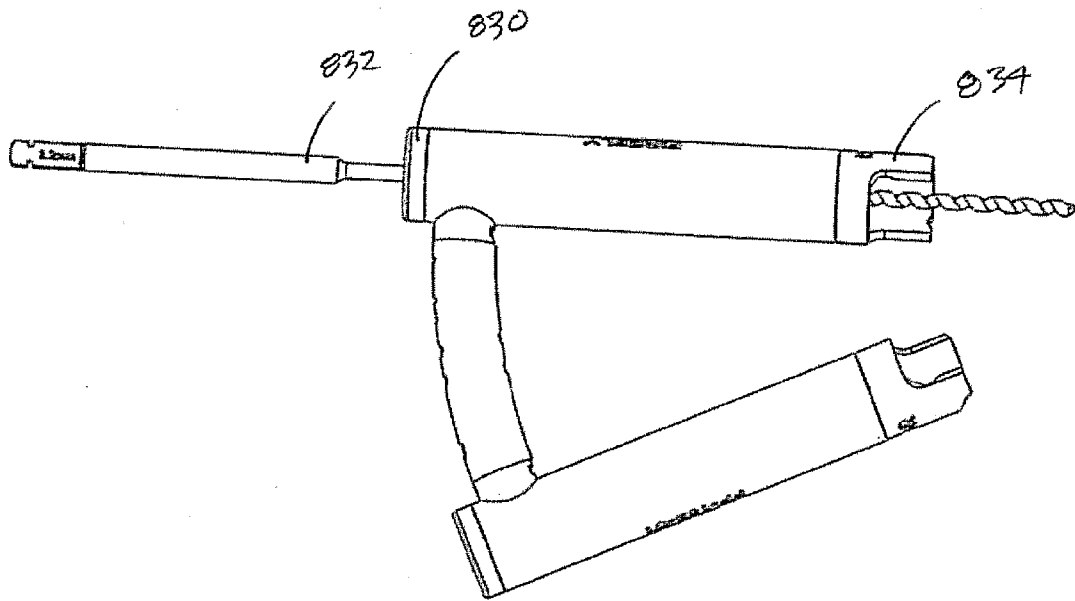


FIG. 85

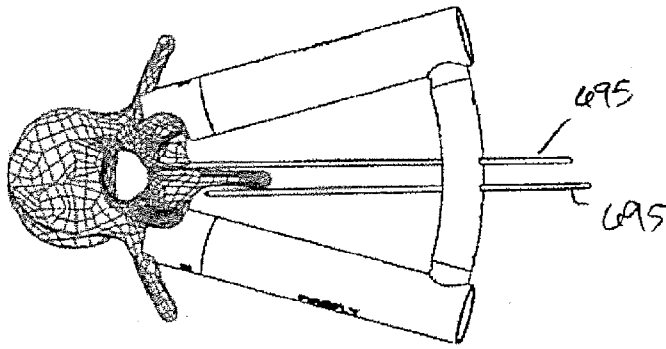


FIG. 86A

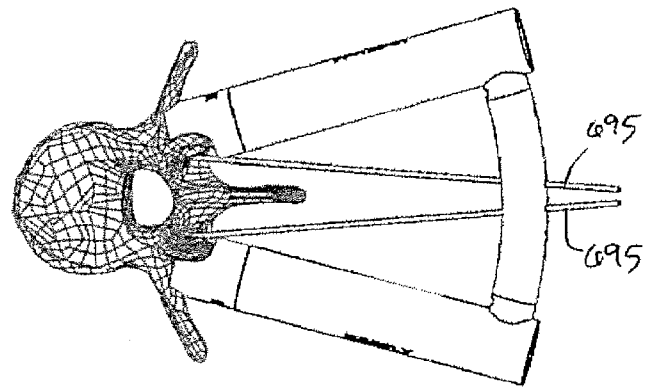


FIG. 86B

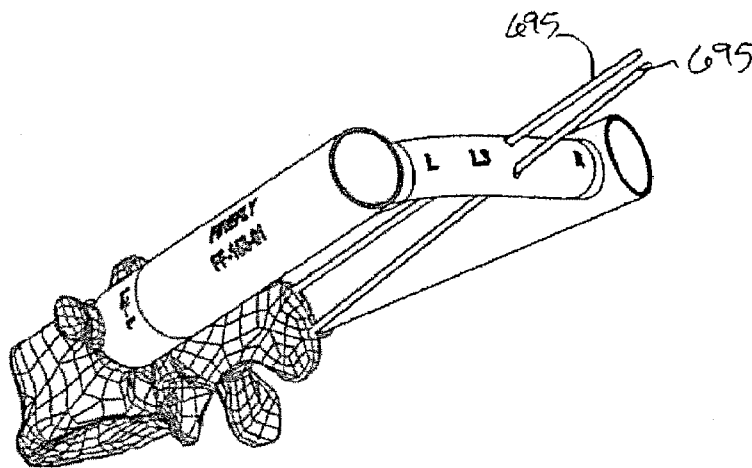
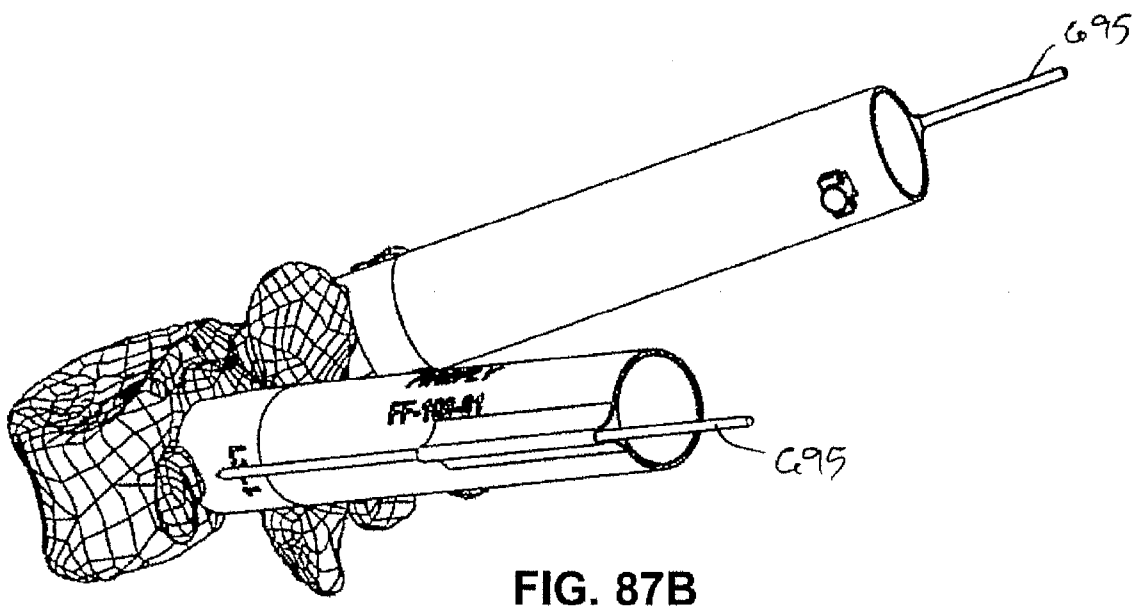
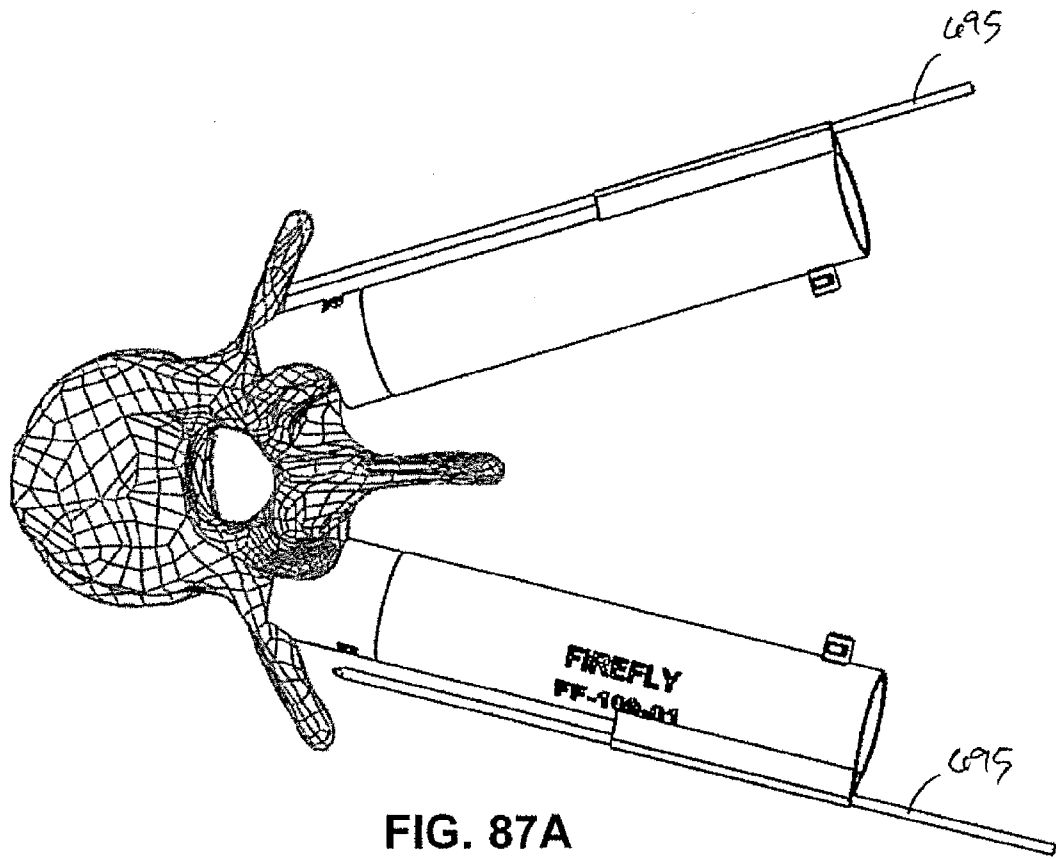
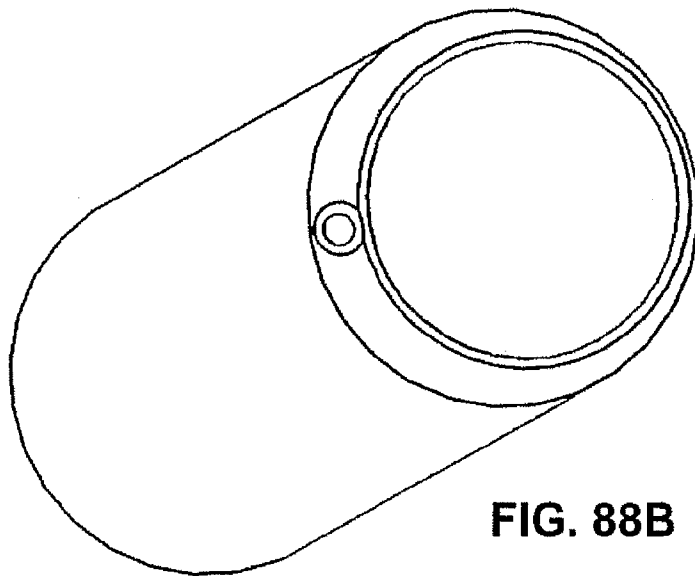
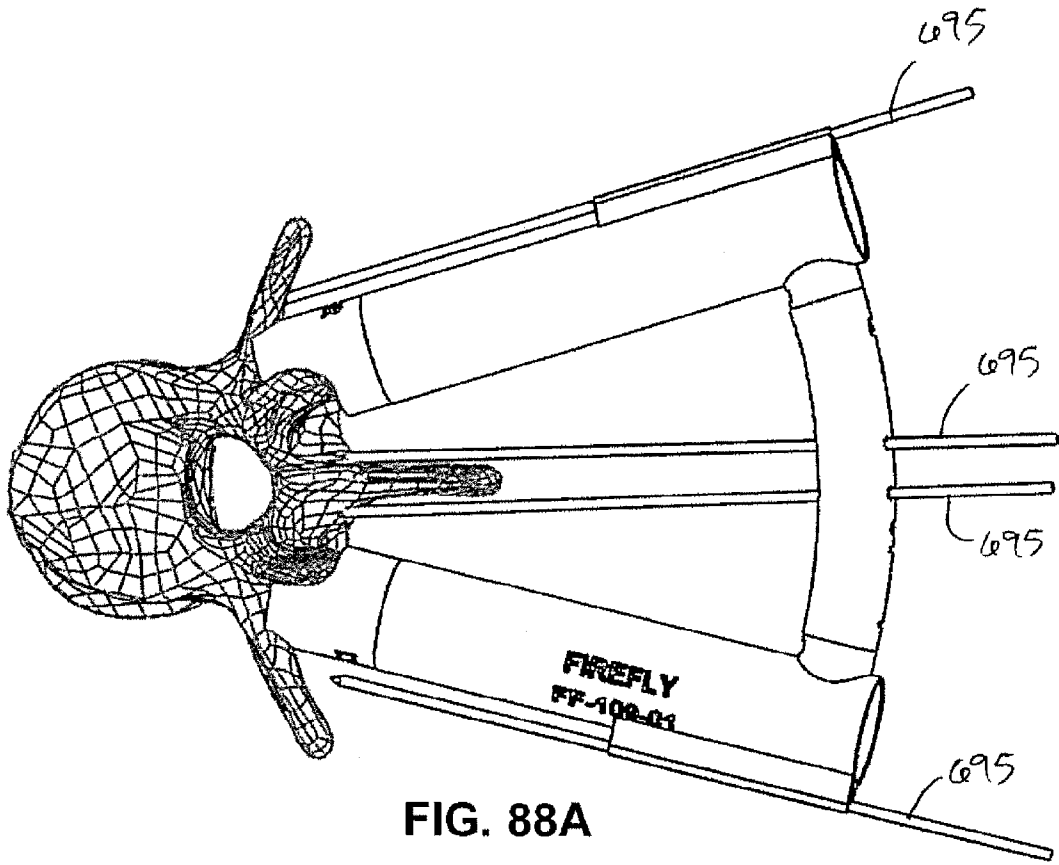


FIG. 86C





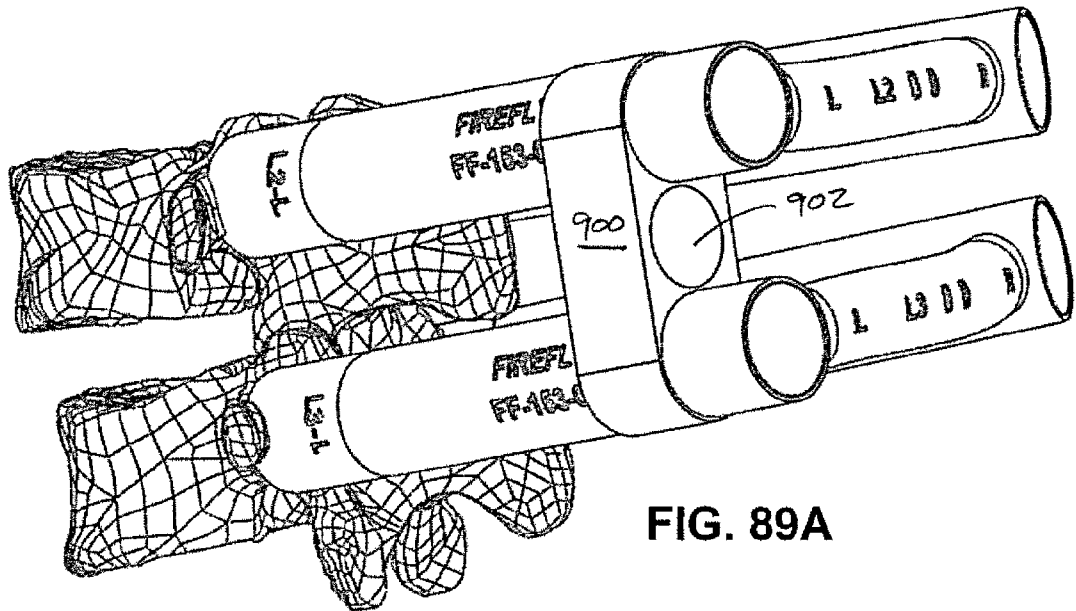


FIG. 89A

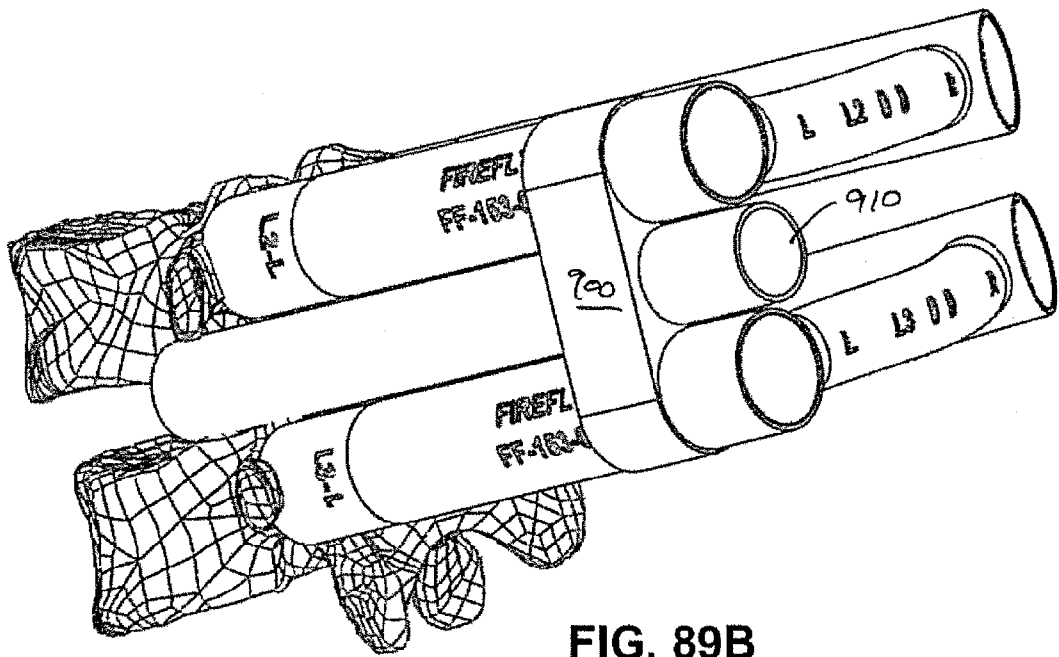
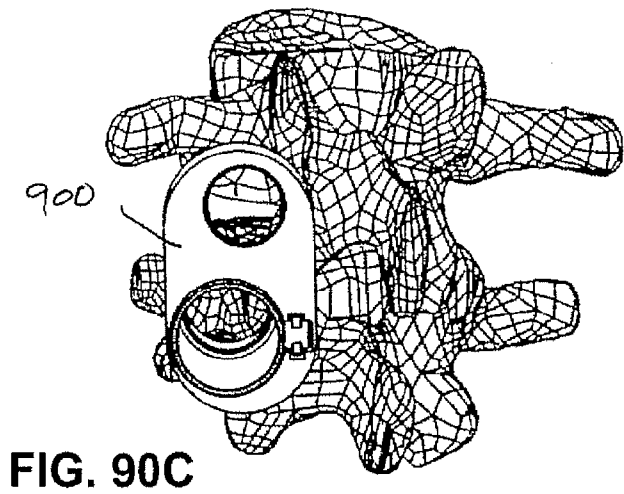
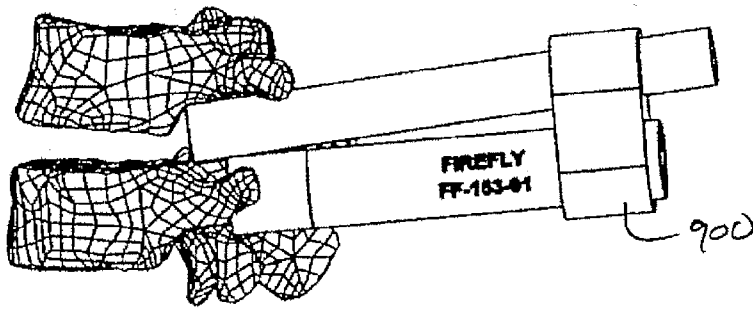
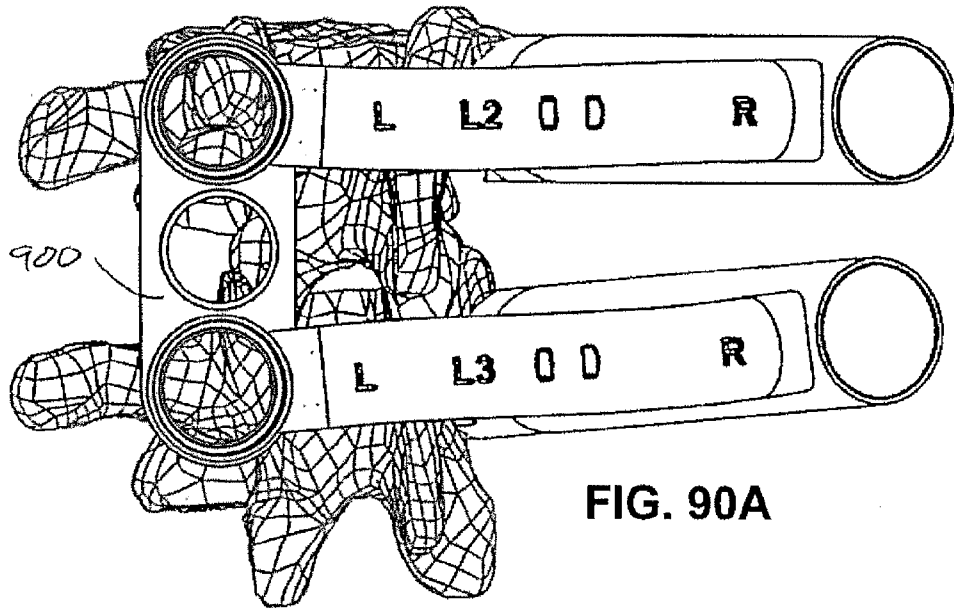


FIG. 89B



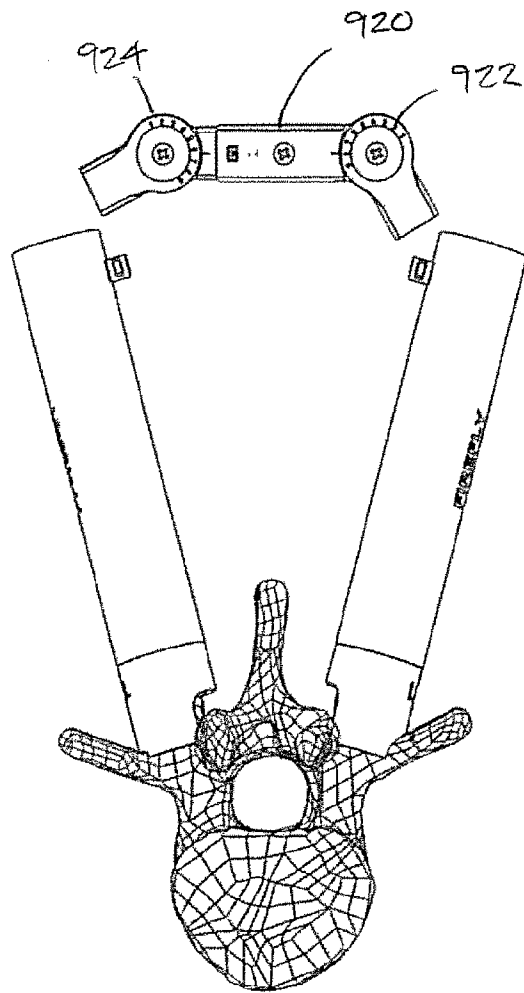


FIG. 91A

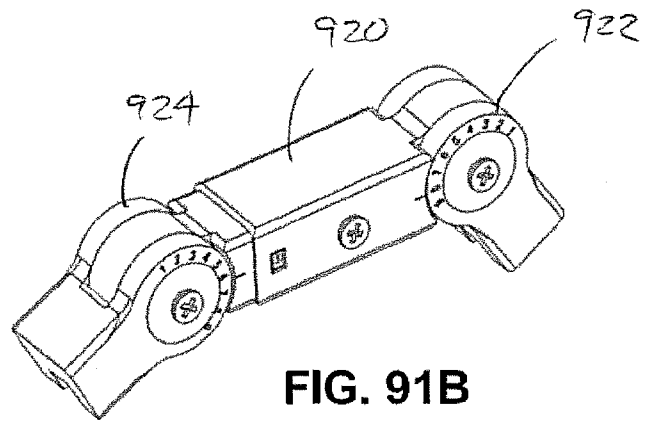


FIG. 91B

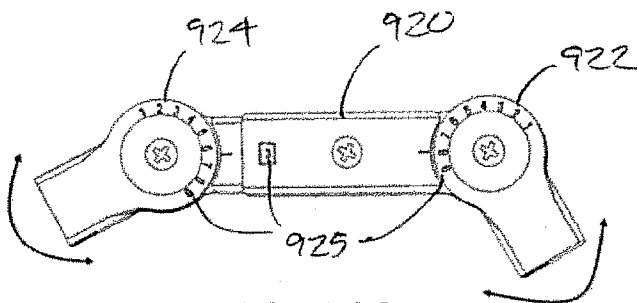


FIG. 91C

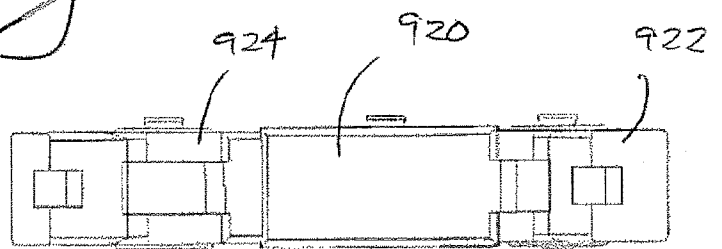


FIG. 91D

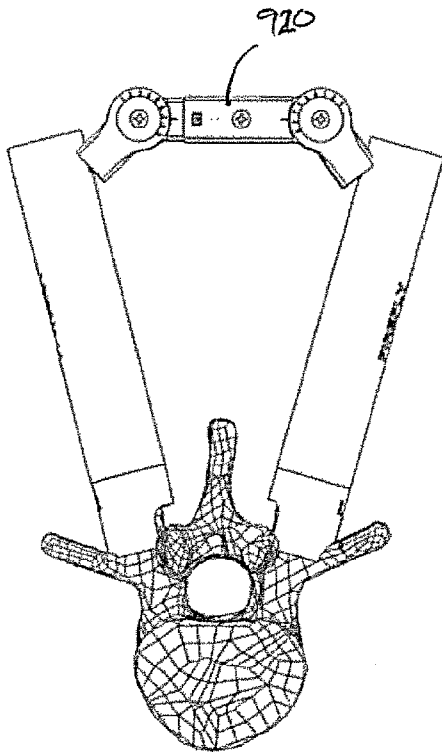


FIG. 92A

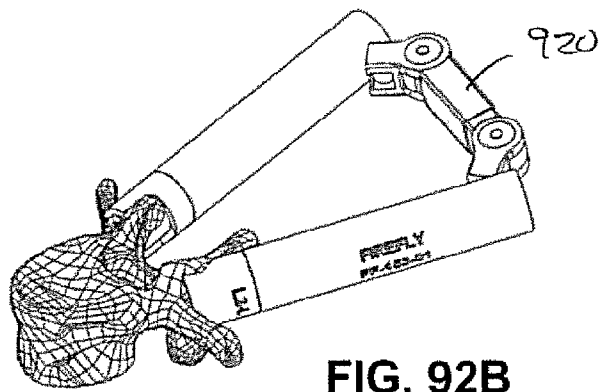


FIG. 92B

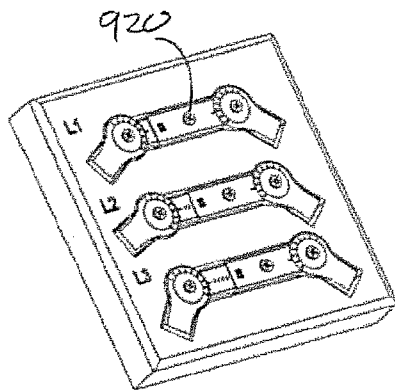


FIG. 92C

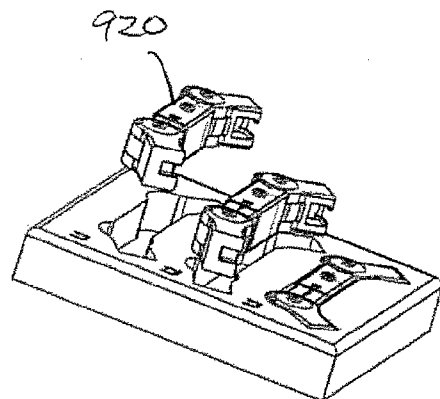


FIG. 92D

FIG. 93A

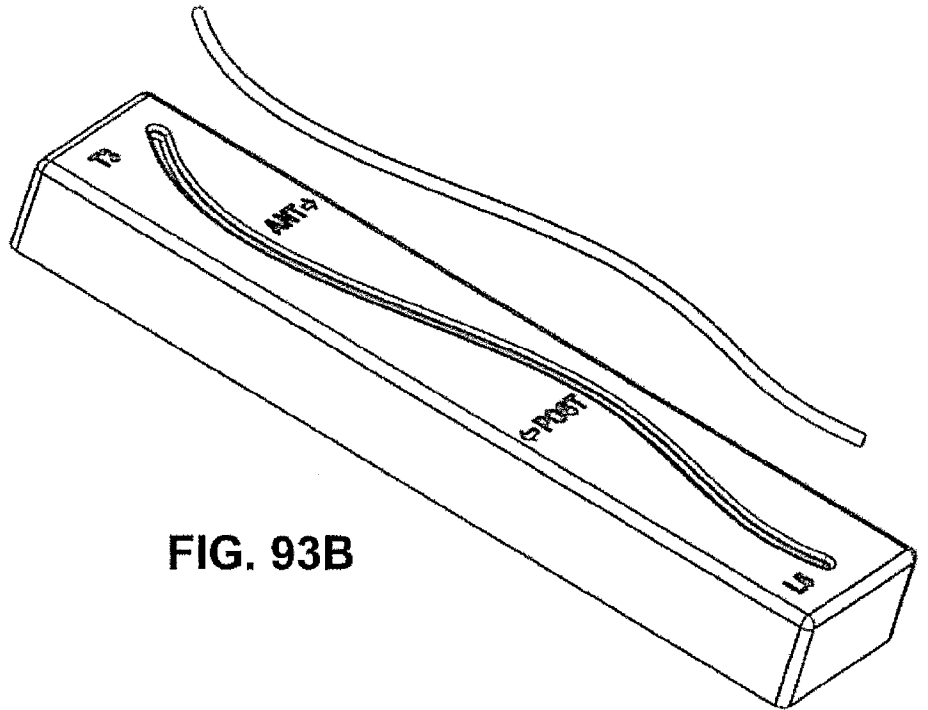
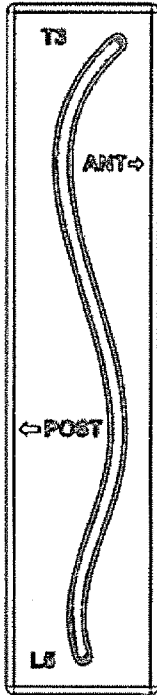


FIG. 93B

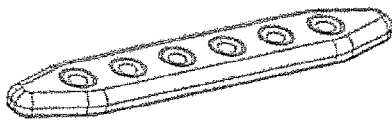


FIG. 93C

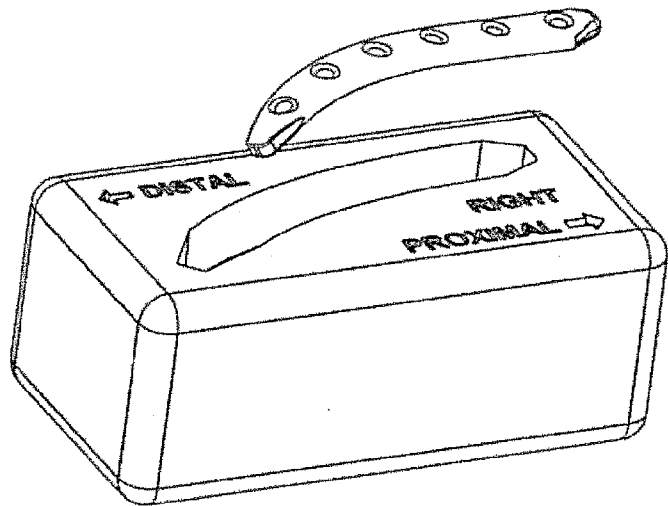


FIG. 93D

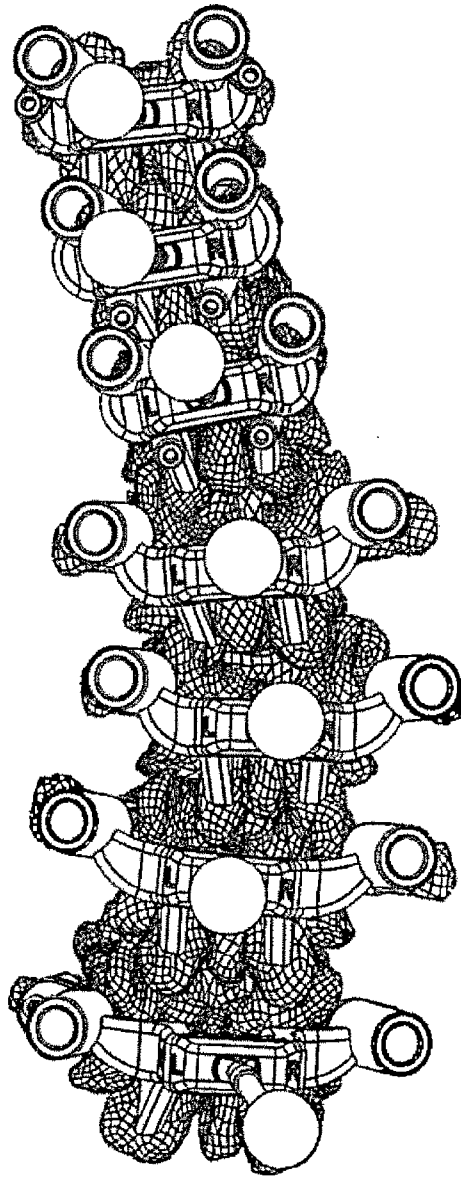


FIG. 94A

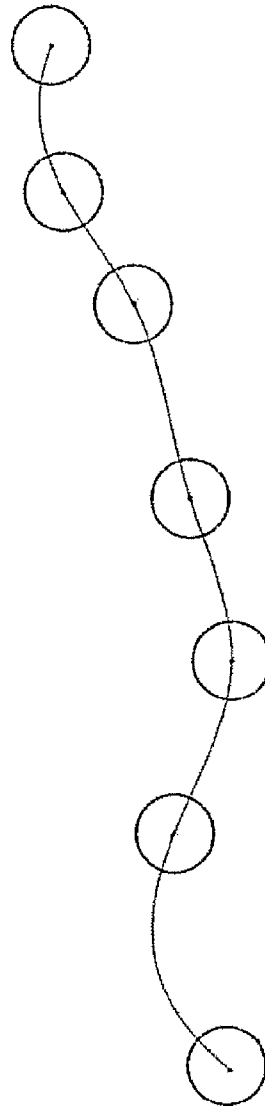


FIG. 94B

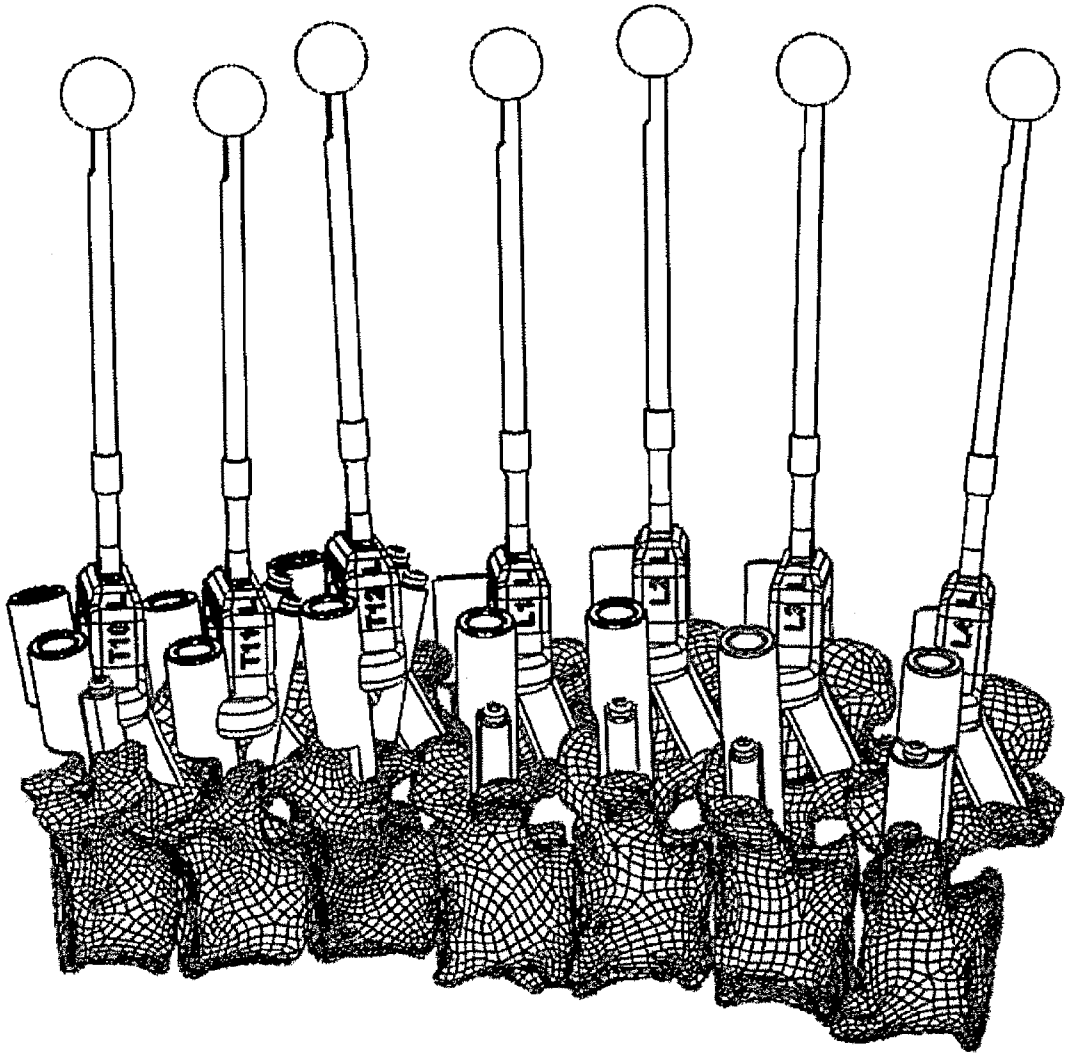


FIG. 94C

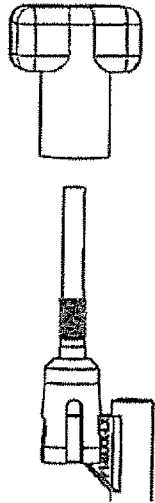


FIG. 95A

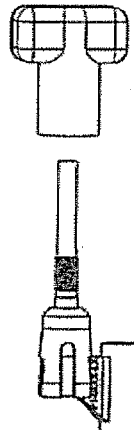


FIG. 95B

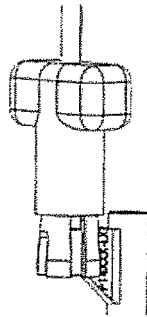


FIG. 95C

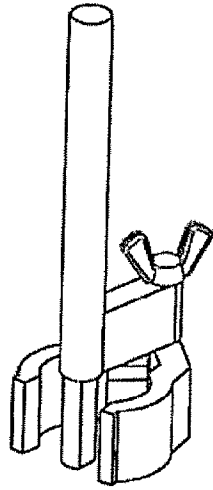


FIG. 96A

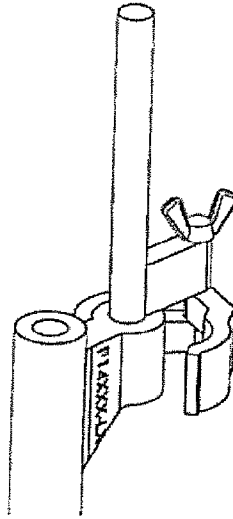


FIG. 96B

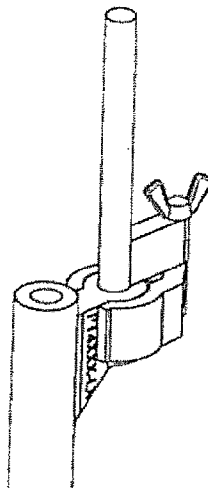


FIG. 96C

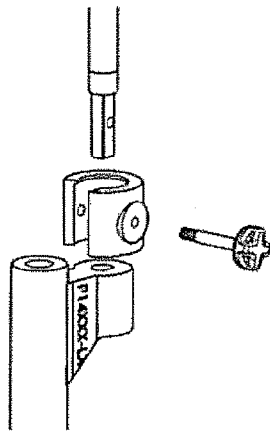


FIG. 97A

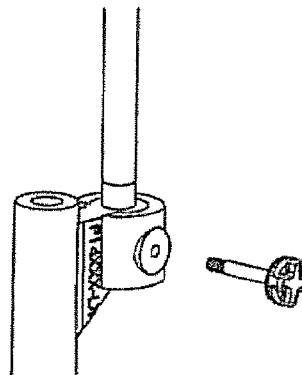


FIG. 97B

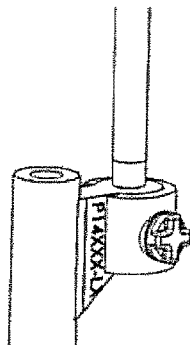


FIG. 97C

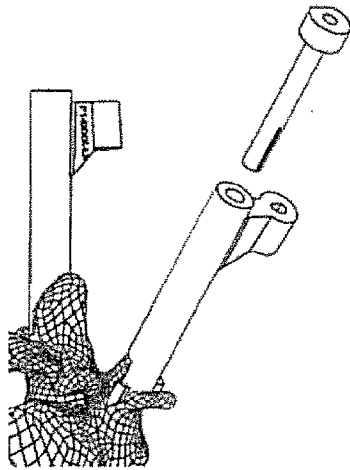


FIG. 98A

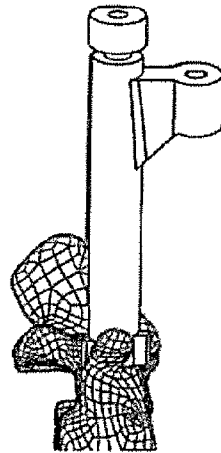


FIG. 98B

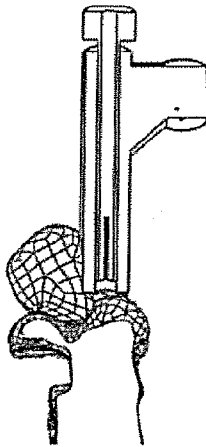


FIG. 98C

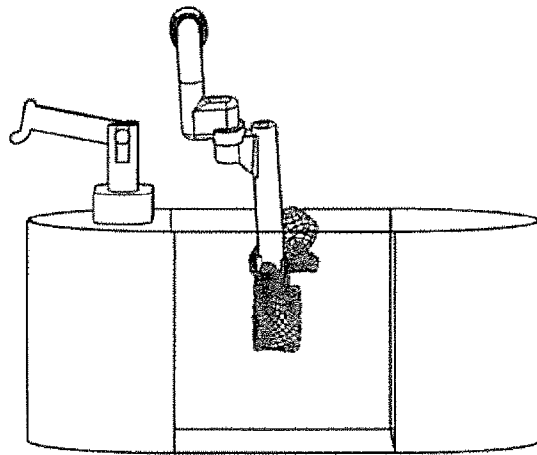


FIG. 99A

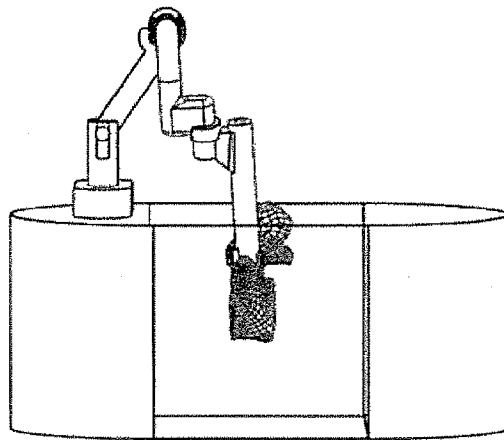


FIG. 99B

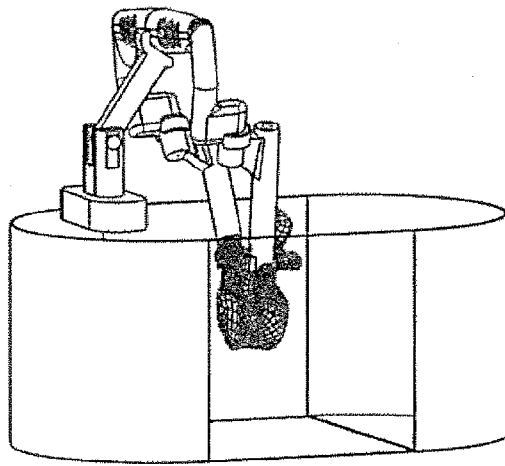


FIG. 99C

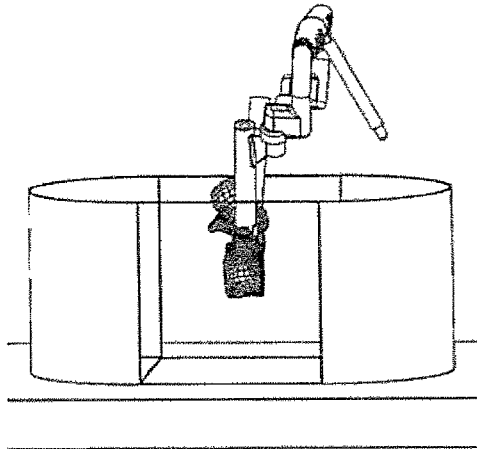


FIG. 99D

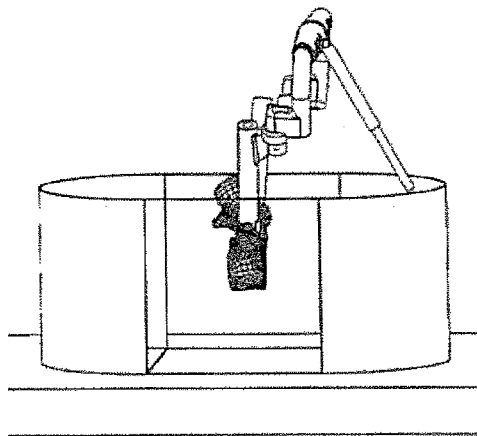


FIG. 99E

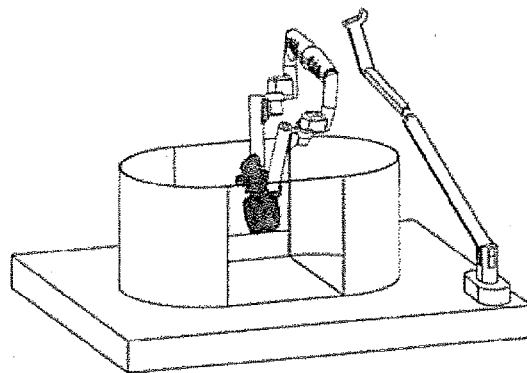


FIG. 99F

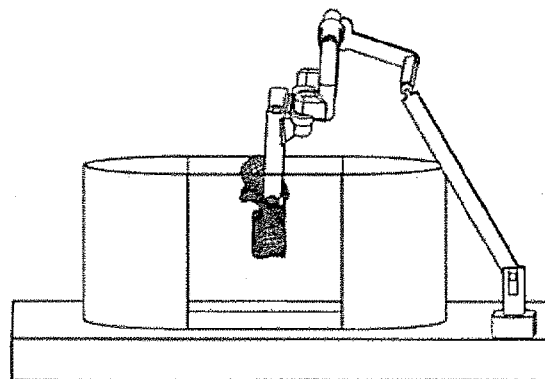


FIG. 99G

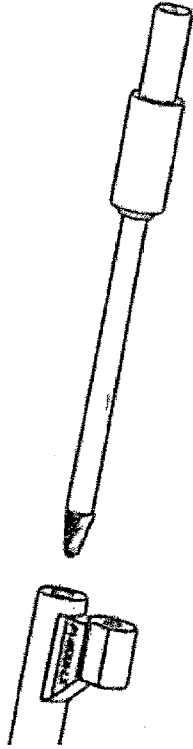


FIG. 100A

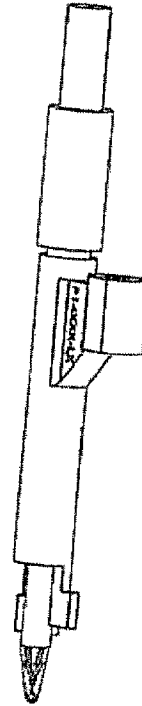


FIG. 100B

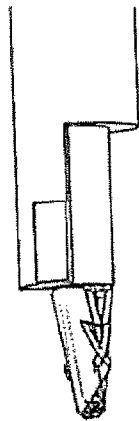


FIG. 100C

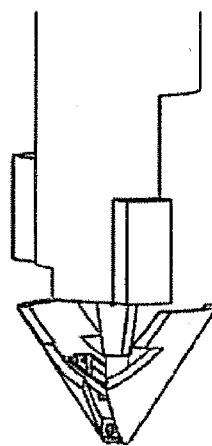


FIG. 100D

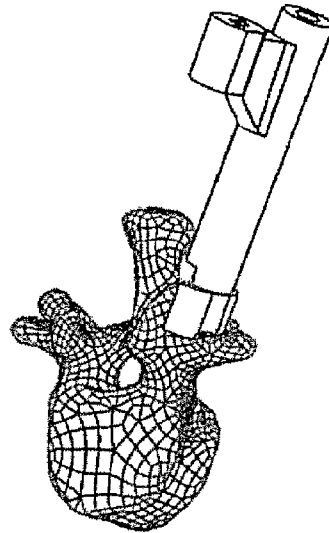


FIG. 101A

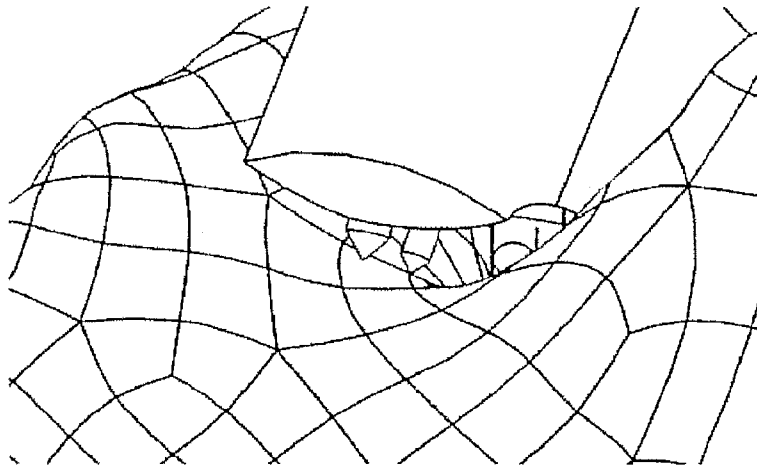


FIG. 101B

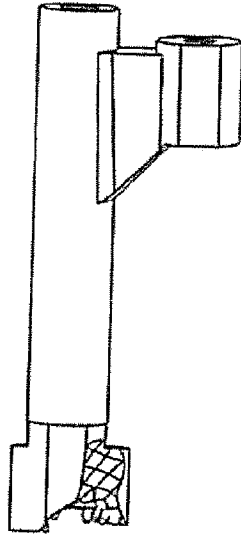


FIG. 101C

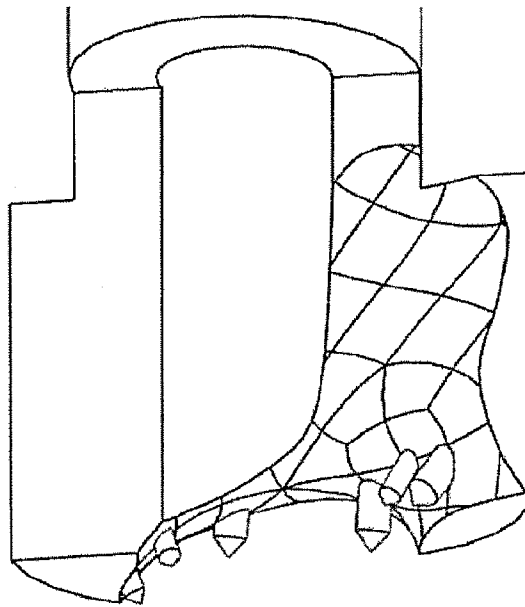


FIG. 101D