



US00D706440S

(12) **United States Design Patent**
Hahr et al.

(10) **Patent No.:** **US D706,440 S**

(45) **Date of Patent:** **** Jun. 3, 2014**

(54) **STIMULATION DEVICE**

(71) Applicant: **Senses Toys Intellectual Property Management UG**, Bielefeld (DE)

(72) Inventors: **Meike Hahr**, Hamburg (DE); **Heiko Tullney**, Hamburg (DE); **Till Muhl**, Hamburg (DE); **Thomas Milewski**, Halstenbek (DE)

(73) Assignee: **Ovo Joint Venture LLC**, Pembroke Park, FL (US)

(**) Term: **14 Years**

(21) Appl. No.: **29/447,969**

(22) Filed: **Mar. 8, 2013**

(30) **Foreign Application Priority Data**

Sep. 10, 2012 (EM) 001342935-0116

(51) **LOC (10) Cl.** **28-03**

(52) **U.S. Cl.**
USPC **D24/215**

(58) **Field of Classification Search**
USPC D24/200, 211, 212, 213, 214, 215;
601/114, 120, 121, 124, 125, 130, 131,
601/134, 135, 136, 137
See application file for complete search history.

(56) **References Cited**

U.S. PATENT DOCUMENTS

D30,230 S *	2/1899	Barnet	D24/214
D447,811 S *	9/2001	Yiu	D24/215
D454,959 S *	3/2002	Harris et al.	D24/215
D620,601 S *	7/2010	TerMeer	D24/215
D637,309 S *	5/2011	Park	D24/215
D643,128 S *	8/2011	Mohamed et al.	D24/215
D648,862 S *	11/2011	Yen	D24/215
D668,346 S *	10/2012	Zeng et al.	D24/215
D673,687 S *	1/2013	Zeng et al.	D24/215
D675,745 S *	2/2013	Nan	D24/215
D675,746 S *	2/2013	Nan	D24/215

D681,225 S *	4/2013	Chen	D24/215
D681,842 S *	5/2013	Chang	D24/215
D685,105 S *	6/2013	Marshall	D24/215
D688,382 S *	8/2013	Marshall	D24/215
D693,017 S *	11/2013	Tai	D24/215
D693,933 S *	11/2013	Tai	D24/215
D694,417 S *	11/2013	Tai	D24/215

* cited by examiner

Primary Examiner — Sandra Snapp

(74) *Attorney, Agent, or Firm* — Merek, Blackmon & Voorhees, LLC

(57) **CLAIM**

The ornamental design for a stimulation device, as shown and described.

DESCRIPTION

FIG. 1 is a top plan view of a stimulation device showing the design;

FIG. 2 is rear elevation view of the stimulation device of FIG. 1;

FIG. 3 is a perspective view taken from the top, front and right side of the stimulation device of FIG. 1, the opposite side being a mirror image thereof;

FIG. 4 is a perspective view taken from the top and right side of the stimulation device of FIG. 1, the opposite side being a mirror image thereof; and,


FIG. 5 is a left side elevation view of the stimulation device of FIG. 1, the right side elevation view being a mirror image thereof.

A perspective view taken from the top, front and left side of the stimulation device of FIG. 1 at an angle corresponding to the angle of the perspective view of FIG. 3 is a mirror image of FIG. 3.

A perspective view taken from the top and left side of the stimulation device of FIG. 1 at an angle corresponding to the angle of the perspective view of FIG. 4 is a mirror image of FIG. 4.

The right side elevation of the stimulation device of FIG. 1 is a mirror image of the left side elevation shown in FIG. 5.

1 Claim, 5 Drawing Sheets

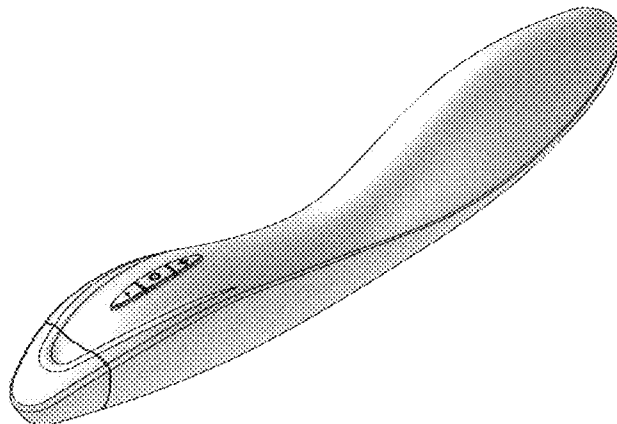

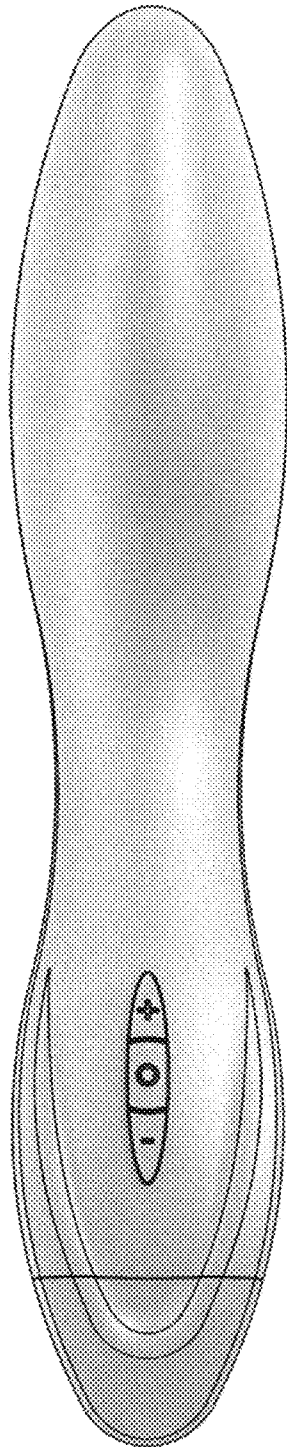


FIG. 1

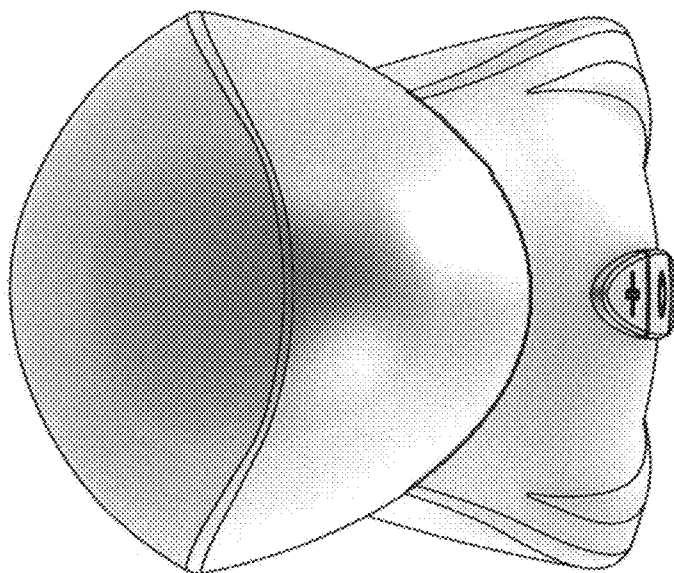


FIG. 2

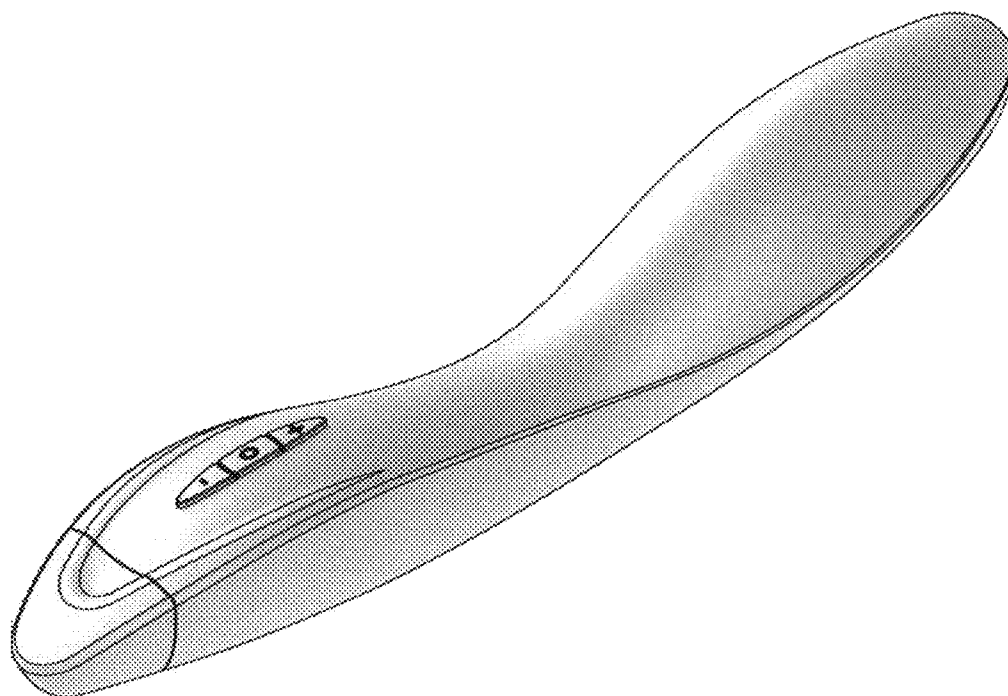


FIG. 3

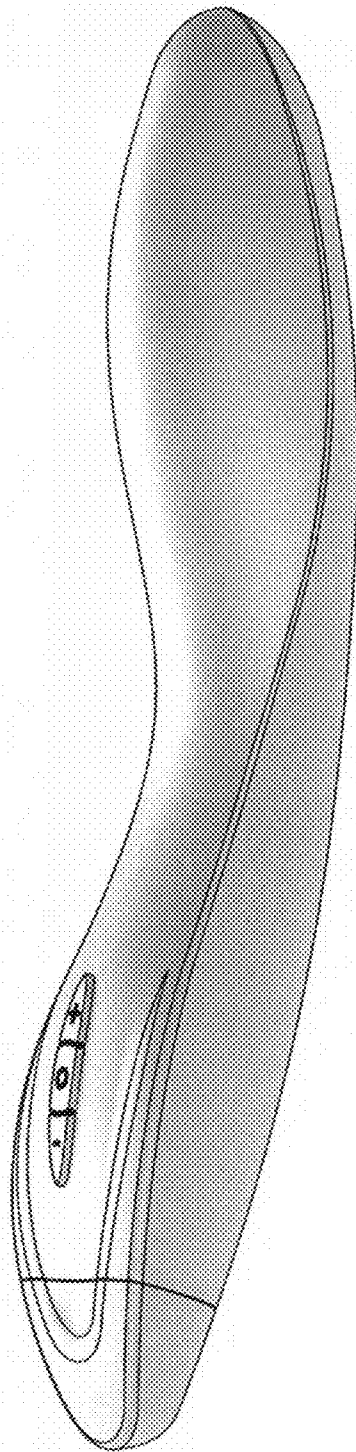


FIG. 4

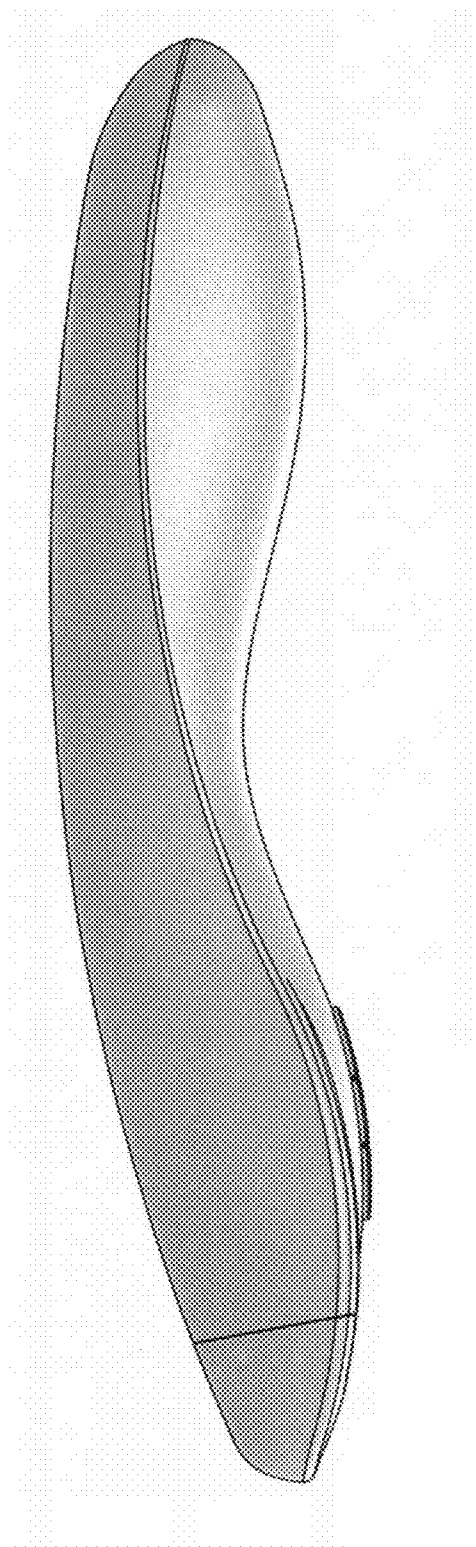


FIG. 5