

## Supporting Information

### Carbon nanotube/polysulfone composite screen-printed electrochemical enzyme biosensors

Samuel Sánchez<sup>a</sup>, Martin Pumera<sup>b</sup>, Enric Cabruja<sup>c</sup>, Esteve Fàbregas<sup>a\*</sup>.


<sup>a</sup>Grup de Sensors i Biosensors, Universitat Autònoma de Barcelona, 08113 Bellaterra, Barcelona, Spain. <sup>b</sup> ICYS, National Institute for Material Science, 1-1 Namiki, Tsukuba, Japan, <sup>c</sup>Centre Nacional de Microelectrònica (CNM) 08113 Bellaterra, Barcelona,

## Supporting Information

Spain.

#### Table of Contents:


- S1. Title and table of contents
- S2. Cyclic voltammograms of CNT 50 electrodes
- S3. Cyclic voltammograms of CNT 200 electrodes
- S4. Cyclic voltammograms of graphite electrodes

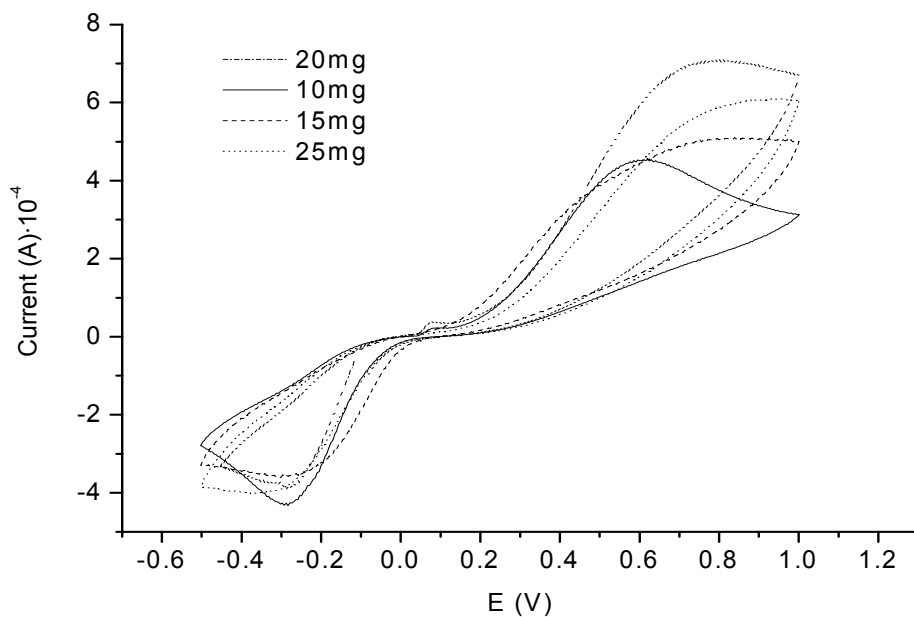

**Supplementary data, Figure S1.**

Comparison of Cyclic Voltammograms of CNT50/PS electrodes. Influence of the carbon loading upon reduction peak current of 0.1 mM potassium ferricyanide.


Supporting electrolyte, PBS buffer (0.1 M, pH 7.0); Scan rate, 50 mV/s

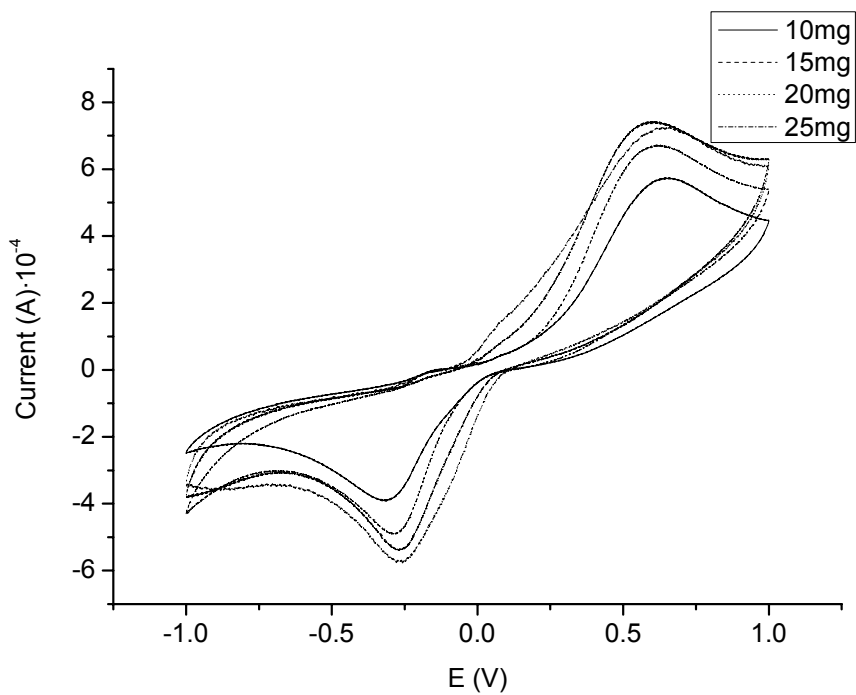

**Supplementary data, Figure S2.**

Comparison of Cyclic Voltammograms of CNT200/PS electrodes. Influence of the carbon loading upon reduction peak current of 0.1 mM potassium ferricyanide.

Supporting electrolyte, PBS buffer (0.1 M, pH 7.0); Scan rate, 50 mV/s

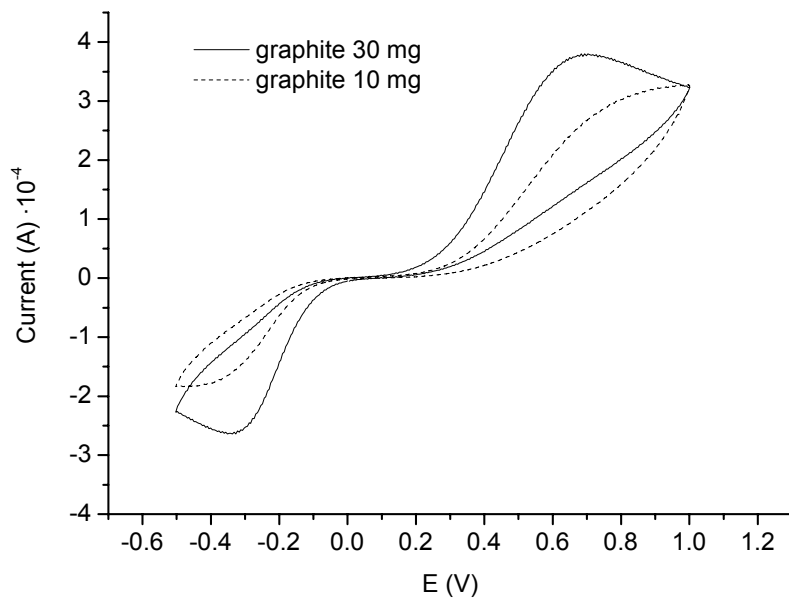

**Supplementary data, Figure S3.**

Comparison of Cyclic Voltammograms of graphite/PS electrodes. Influence of the carbon loading upon reduction peak current of 0.1 mM potassium ferricyanide.

Supporting electrolyte, PBS buffer (0.1 M, pH 7.0); Scan rate, 50 mV/s